

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033115\
 Data File : BF078116.D
 Acq On : 31 Mar 2015 16:13
 Operator : TP/IZ
 Sample : G1712-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.321	35	38	41	rVB	70022	78411	20.21%	3.385%
2	1.470	50	51	55	rVB3	4412	4919	1.27%	0.212%
3	1.721	71	73	86	rBV	185075	269460	69.46%	11.634%
4	7.048	537	539	541	rBV	185484	202864	52.29%	8.758%
5	8.625	674	677	679	rBV	256382	284337	73.29%	12.276%
6	10.785	864	866	869	rBB2	340637	341052	87.91%	14.725%
7	12.625	1025	1027	1029	rBV	399177	375185	96.71%	16.198%
8	15.928	1313	1316	1318	rBV	293656	387961	100.00%	16.750%
9	17.586	1458	1461	1465	rBV2	1444	5432	1.40%	0.235%
10	17.769	1474	1477	1482	rBV	273180	366577	94.49%	15.827%


Sum of corrected areas: 2316198

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033115\
Data File : BF078116.D
Acq On : 31 Mar 2015 16:13
Operator : TP/IZ
Sample : G1712-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

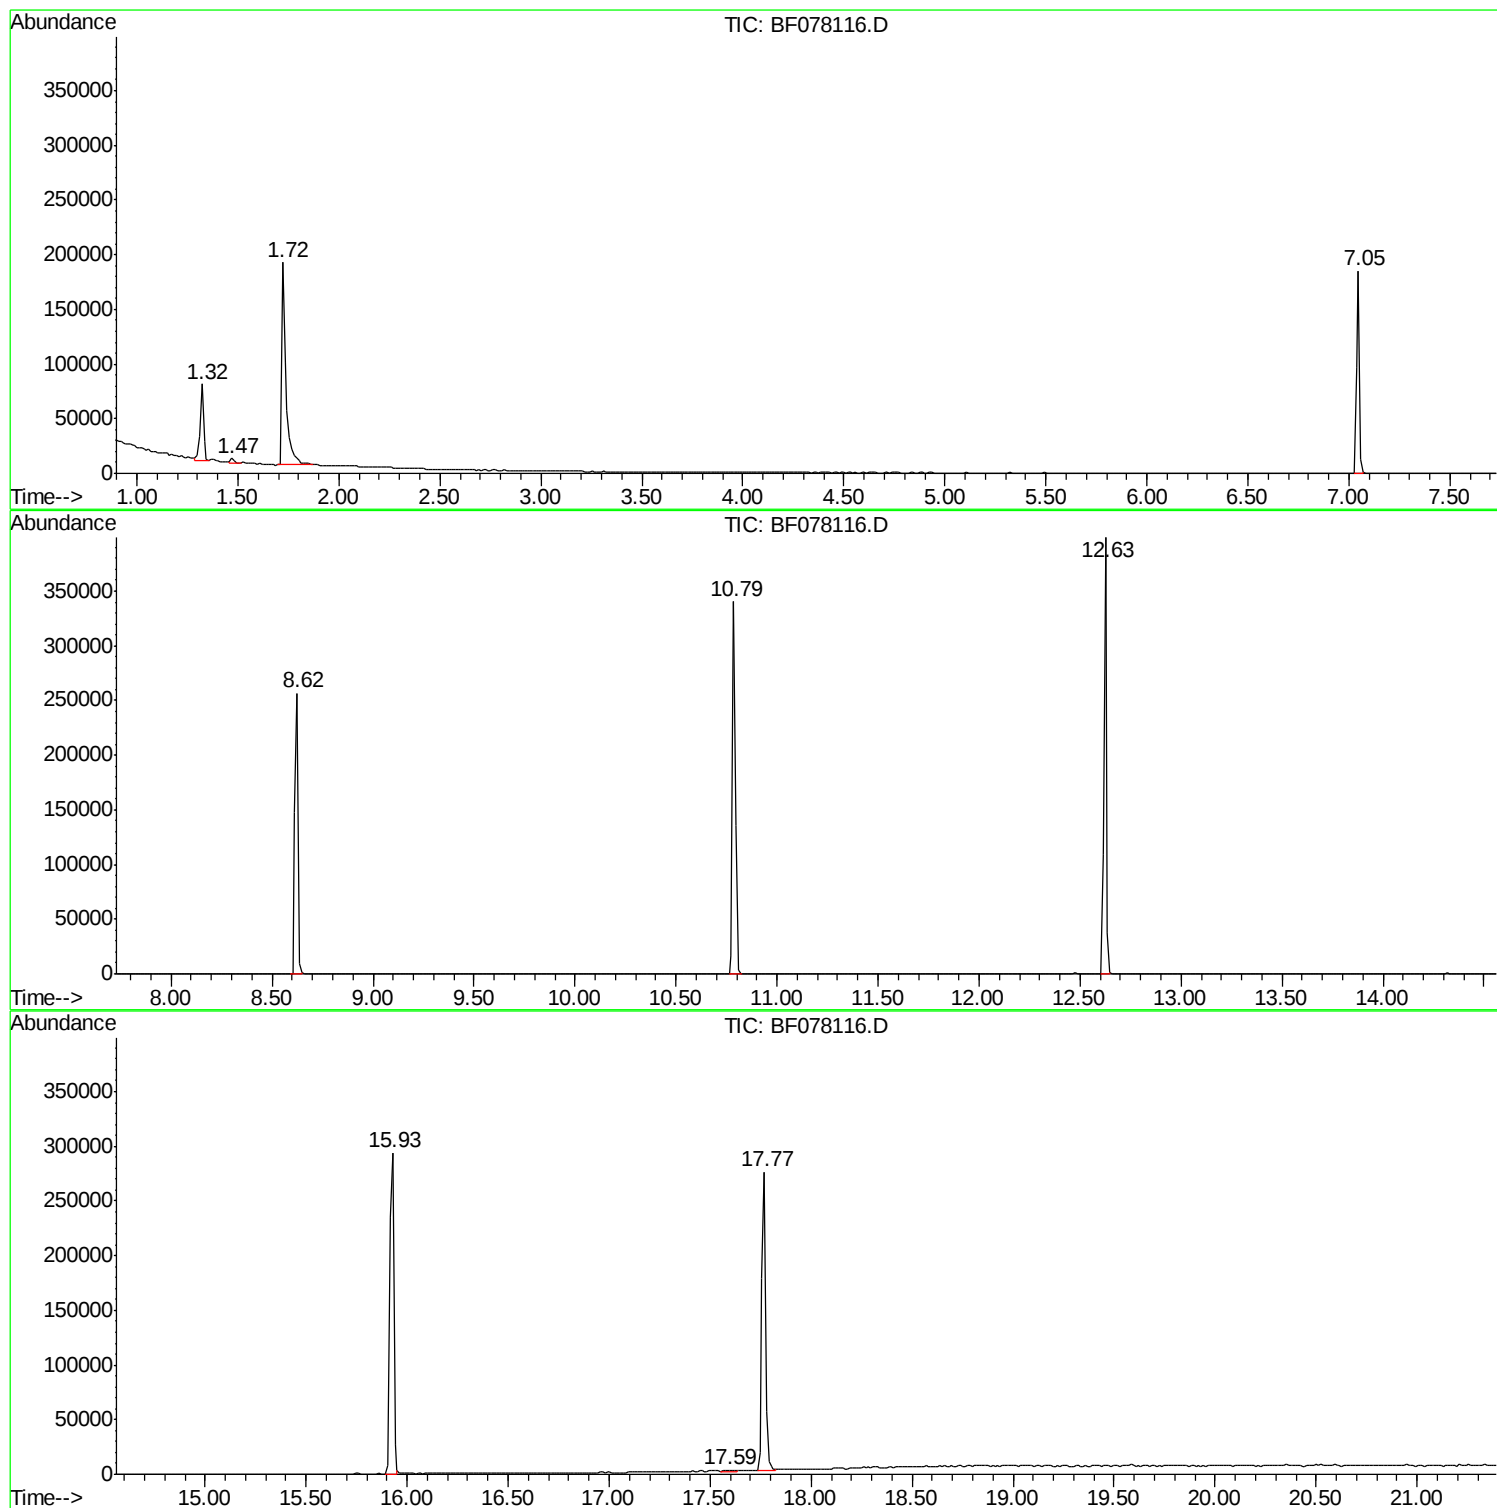

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF033115\
Data_File : BF078116.D
Acq_On : 31-Mar-2015 16:133
Operator : TP/IZZ
Sample : G1712-055
Misc :
ALS_Vial : 9 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
