

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033115\
 Data File : BF078123.D
 Acq On : 31 Mar 2015 19:34
 Operator : TP/IZ
 Sample : G1698-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 Z2-0116

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.321	34	38	41	rVB	260509	388104	26.13%	3.957%
2	1.481	49	52	55	rVB	321986	367267	24.72%	3.745%
3	1.721	71	73	89	rVB	118753	182765	12.30%	1.863%
4	4.773	339	340	346	rBB	19315	33588	2.26%	0.342%
5	5.333	387	389	397	rBB	348050	408388	27.49%	4.164%
6	6.636	501	503	511	rBB	232558	239742	16.14%	2.444%
7	6.762	511	514	516	rBV	870585	858060	57.76%	8.748%
8	7.047	537	539	541	rBV	215045	219938	14.81%	2.242%
9	7.230	553	555	557	rBV	973448	865582	58.27%	8.825%
10	7.745	597	600	602	rBV	707077	676610	45.55%	6.898%
11	8.625	674	677	679	rBV	270716	299789	20.18%	3.057%
12	9.973	792	795	797	rBV	1319720	1454224	97.89%	14.827%
13	10.785	864	866	869	rVB	379018	361822	24.36%	3.689%
14	11.768	949	952	954	rBV	767944	775316	52.19%	7.905%
15	12.625	1024	1027	1029	rBV	348343	376622	25.35%	3.840%
16	14.614	1199	1201	1204	rBV	1209774	1485543	100.00%	15.146%
17	15.894	1311	1313	1316	rBV	407908	412544	27.77%	4.206%
18	17.597	1459	1462	1465	rBV	351775	402231	27.08%	4.101%


Sum of corrected areas: 9808135

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033115\
Data File : BF078123.D
Acq On : 31 Mar 2015 19:34
Operator : TP/IZ
Sample : G1698-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
Z2-0116

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

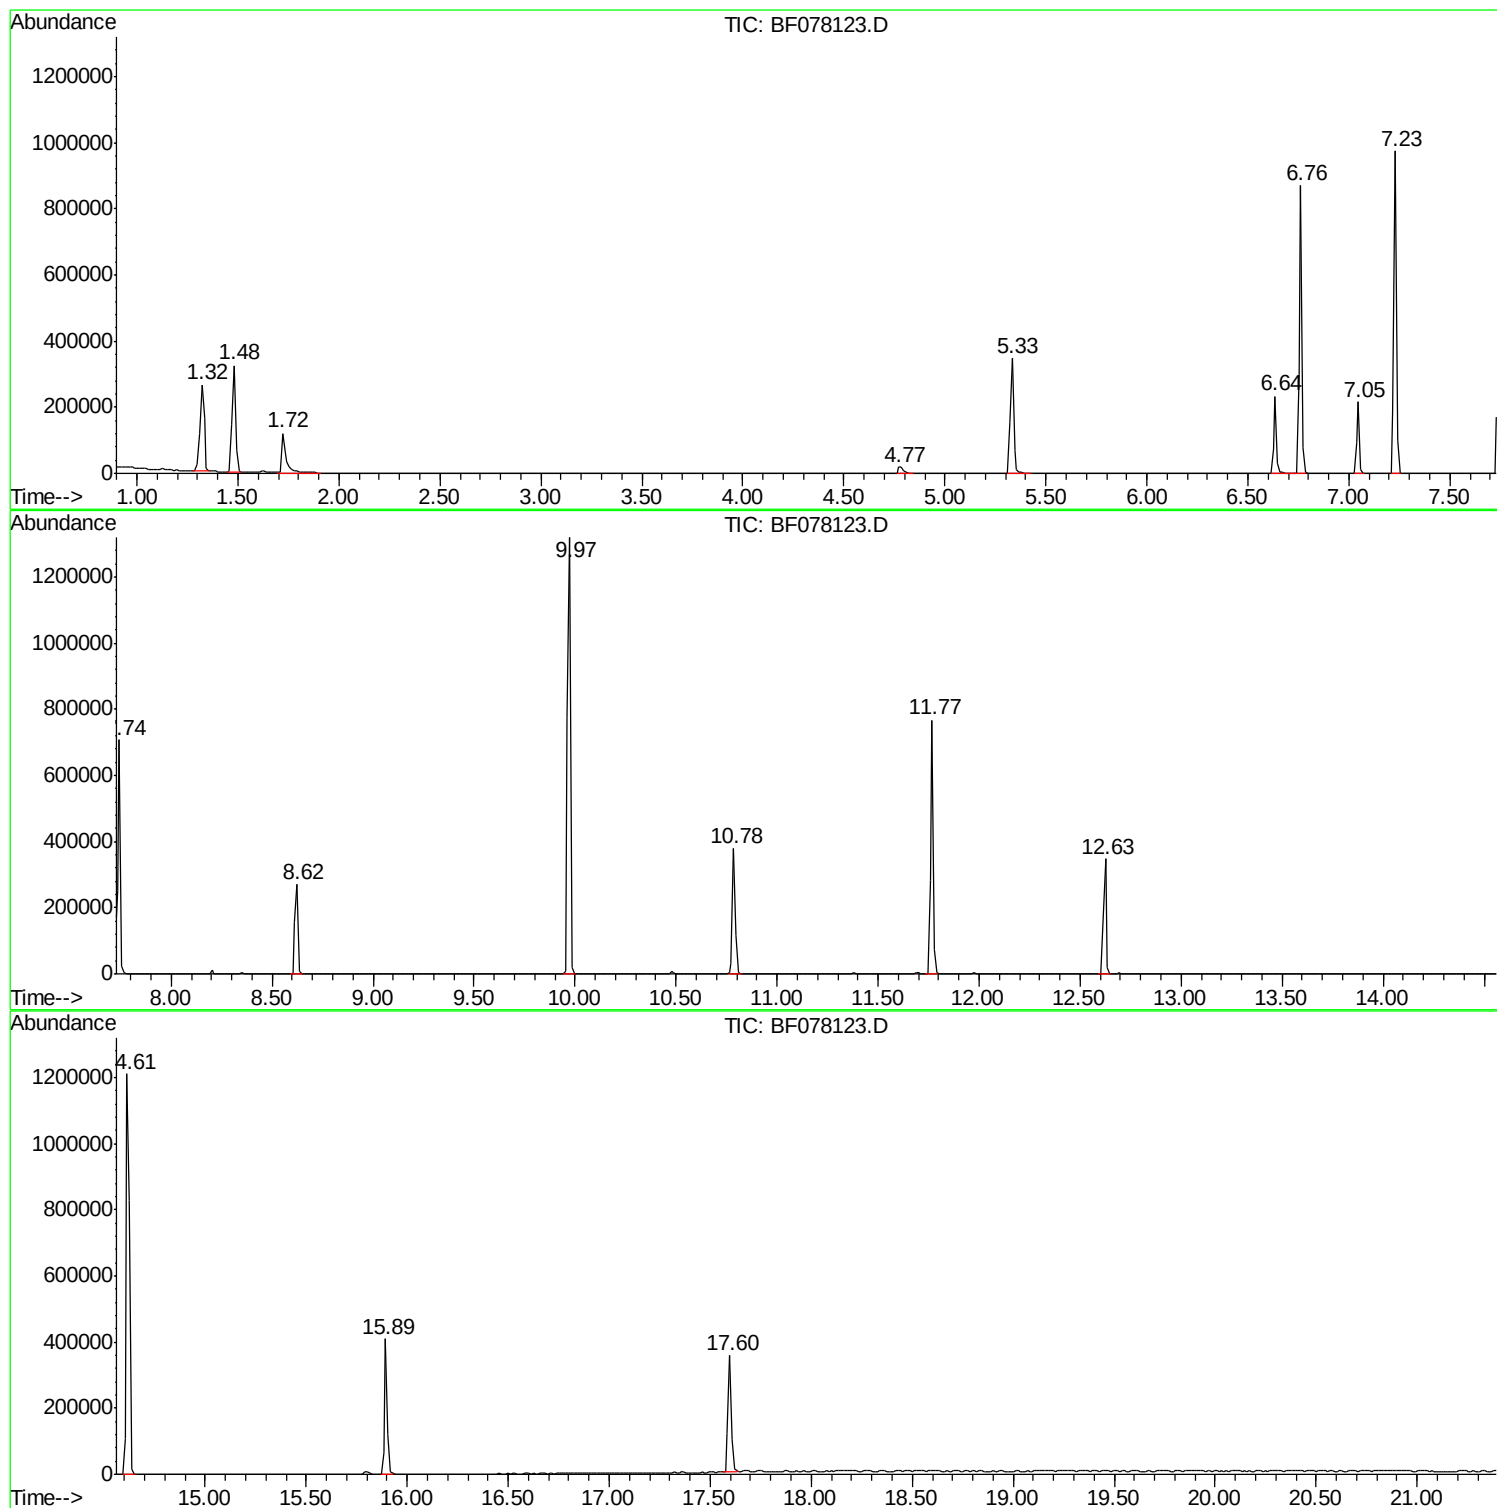

Data Path : Z:\HPCHEM1\BNA F\DATA\BF033115\
Data File : BF078123.D
Acq On : 31 Mar 2015 19:34
Operator : TP/IZ
Sample : G1698-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
Z2-0116










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Butane, 2-methoxy-2-methyl- Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.48	33.40 ng	367267	1,4-Dichlorobenzene-d4	7.05

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2		1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	23
3		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
4		Silane, tetramethyl-	88	C4H12Si	000075-76-3	12
5		Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9

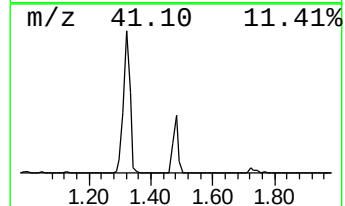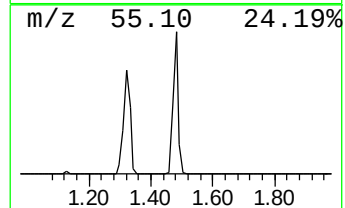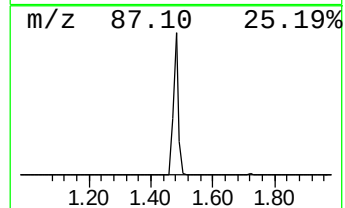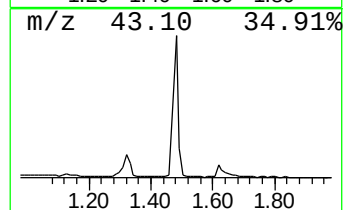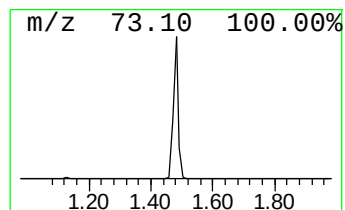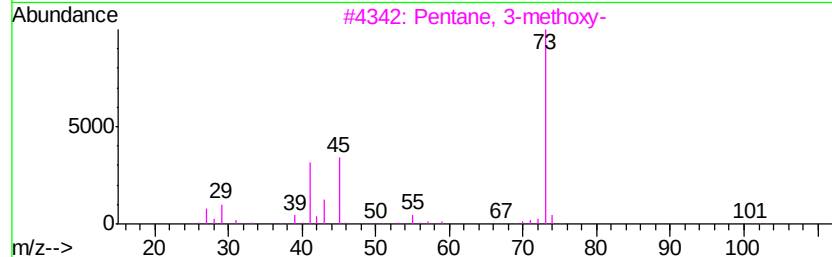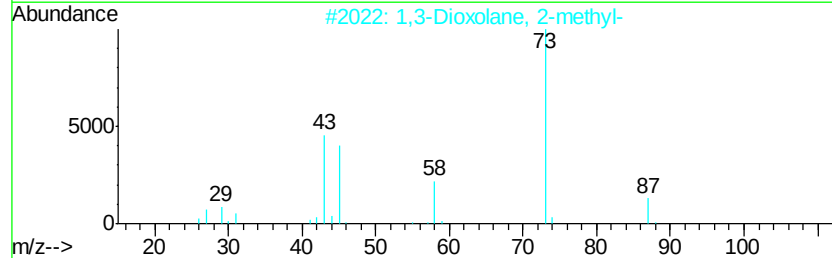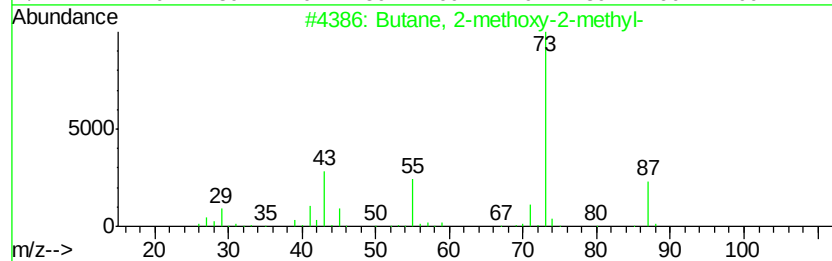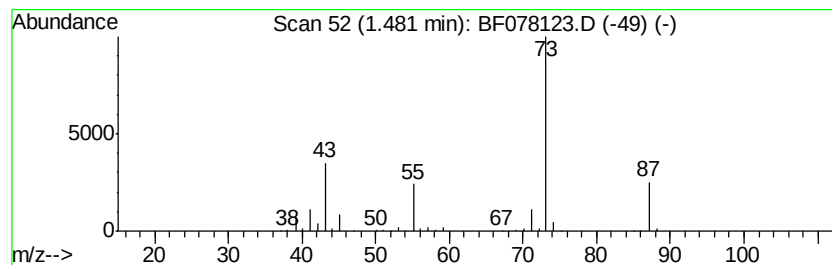

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033115\
Data File : BF078123.D
Acq On : 31 Mar 2015 19:34
Operator : TP/IZ
Sample : G1698-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
Z2-0116










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.77	3.05 ng	33588	1,4-Dichlorobenzene-d4	7.05

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56	
2	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	9	
3	Acetone	58	C3H6O	000067-64-1	7	
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	7	
5	Diacetamide	101	C4H7NO2	000625-77-4	7	

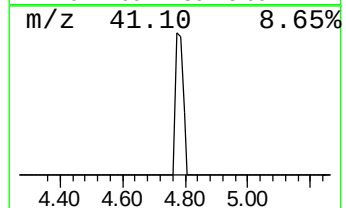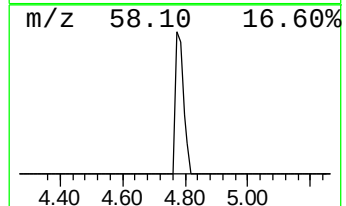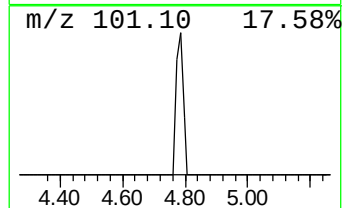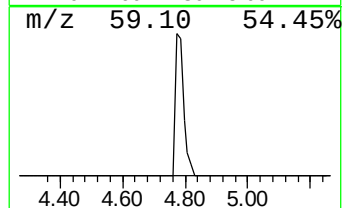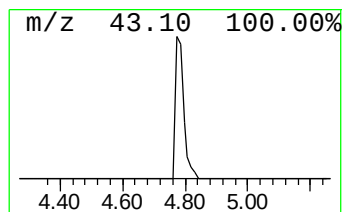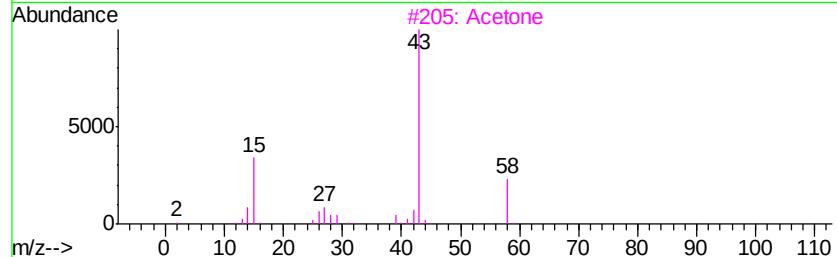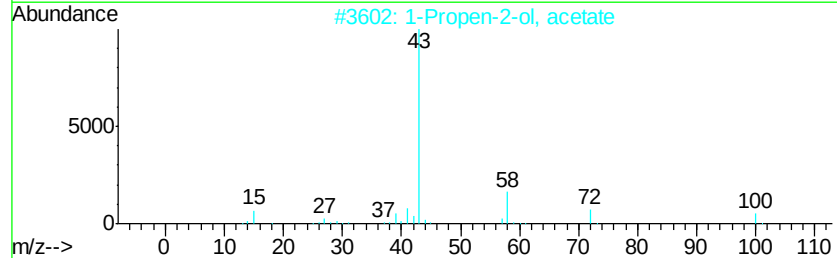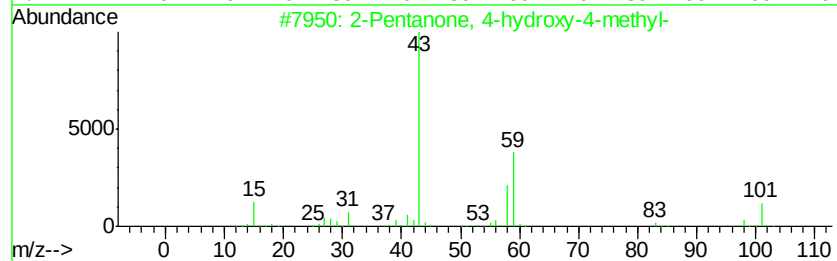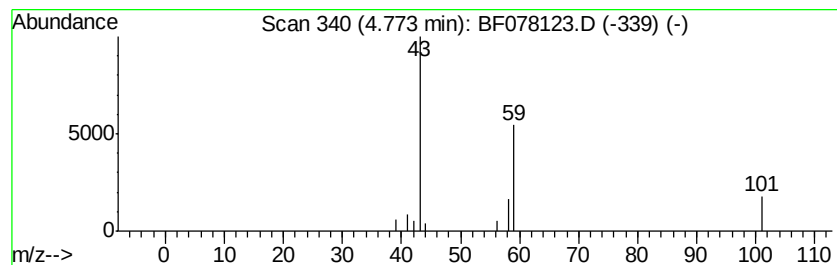

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033115\
Data File : BF078123.D
Acq On : 31 Mar 2015 19:34
Operator : TP/IZ
Sample : G1698-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
Z2-0116










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 unknown6.76 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.76	78.03 ng	858060	1,4-Dichlorobenzene-d4	7.05

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

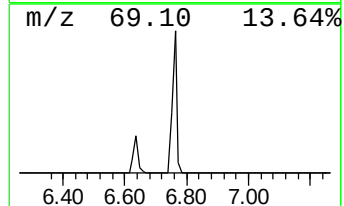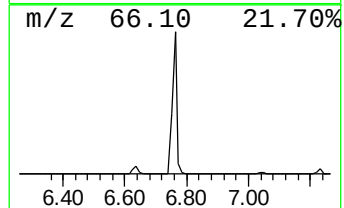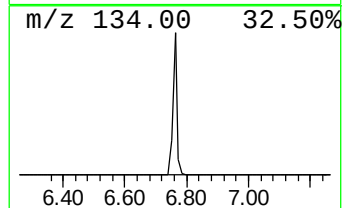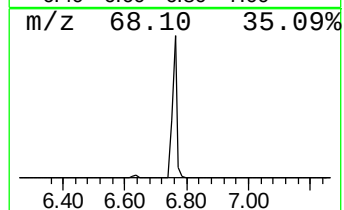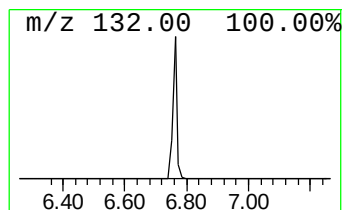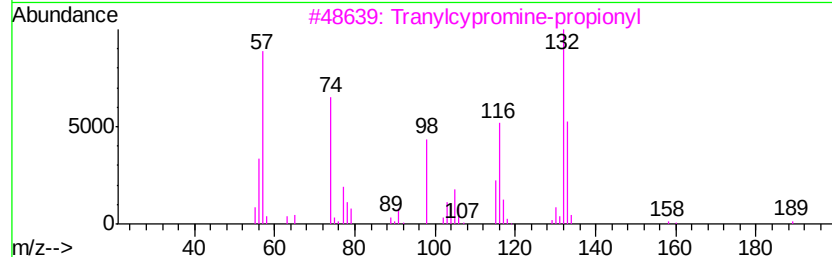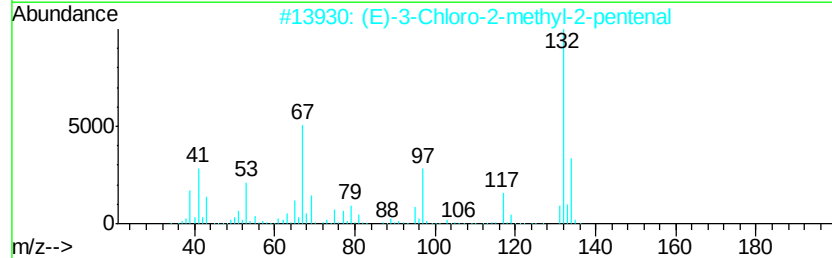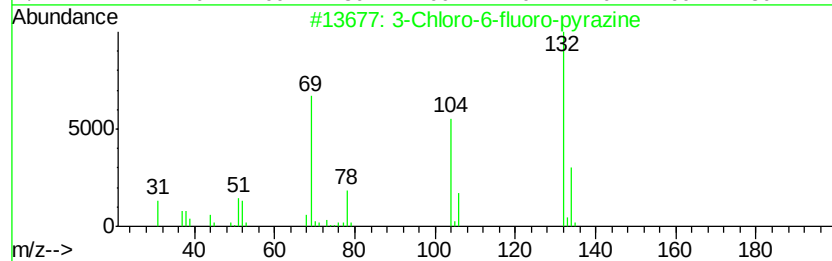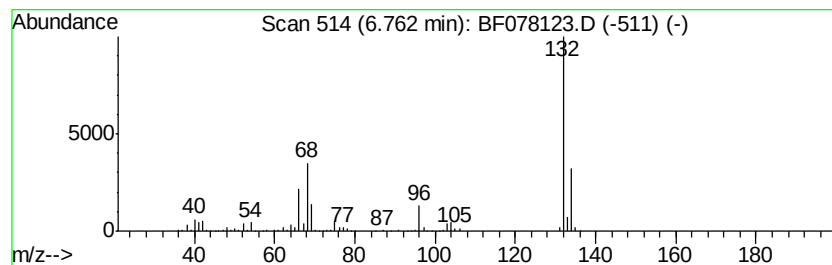

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033115\
Data File : BF078123.D
Acq On : 31 Mar 2015 19:34
Operator : TP/IZ
Sample : G1698-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
Z2-0116

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	1.48	33.4	ng	367267	1	7.05	219938	20.0
2-Pentanone, 4-hy...	4.77	3.0	ng	33588	1	7.05	219938	20.0
unknown6.76	6.76	78.0	ng	858060	1	7.05	219938	20.0