

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033115\
 Data File : BF078127.D
 Acq On : 31 Mar 2015 21:29
 Operator : TP/IZ
 Sample : G1696-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S32-0461

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.321	35	38	41	rVB	227250	328883	17.94%	2.922%
2	1.481	49	52	55	rVB	286666	365346	19.93%	3.246%
3	1.607	61	63	71	rVV	71392	160826	8.77%	1.429%
4	1.721	71	73	100	rVB	1055462	1833224	100.00%	16.288%
5	4.784	339	341	347	rBV	15833	27025	1.47%	0.240%
6	5.333	387	389	398	rBB	290897	375896	20.50%	3.340%
7	6.636	501	503	511	rBB	183095	208603	11.38%	1.853%
8	6.762	511	514	516	rBV	790775	839162	45.78%	7.456%
9	7.048	537	539	541	rBV	202068	216914	11.83%	1.927%
10	7.230	553	555	557	rBV	975237	873015	47.62%	7.757%
11	7.745	597	600	602	rBV	661566	670409	36.57%	5.956%
12	8.625	674	677	679	rBV	223210	292972	15.98%	2.603%
13	9.974	792	795	797	rBV	1169869	1409090	76.86%	12.519%
14	10.785	864	866	869	rVB	381403	351273	19.16%	3.121%
15	11.768	949	952	954	rBV	761787	793384	43.28%	7.049%
16	12.625	1024	1027	1029	rBV	320766	378461	20.64%	3.363%
17	14.614	1199	1201	1204	rBV	1276814	1350759	73.68%	12.001%
18	15.894	1310	1313	1316	rBV	389000	399339	21.78%	3.548%
19	17.563	1457	1459	1462	rBV	303676	380639	20.76%	3.382%


Sum of corrected areas: 11255220

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033115\
Data File : BF078127.D
Acq On : 31 Mar 2015 21:29
Operator : TP/IZ
Sample : G1696-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S32-0461

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

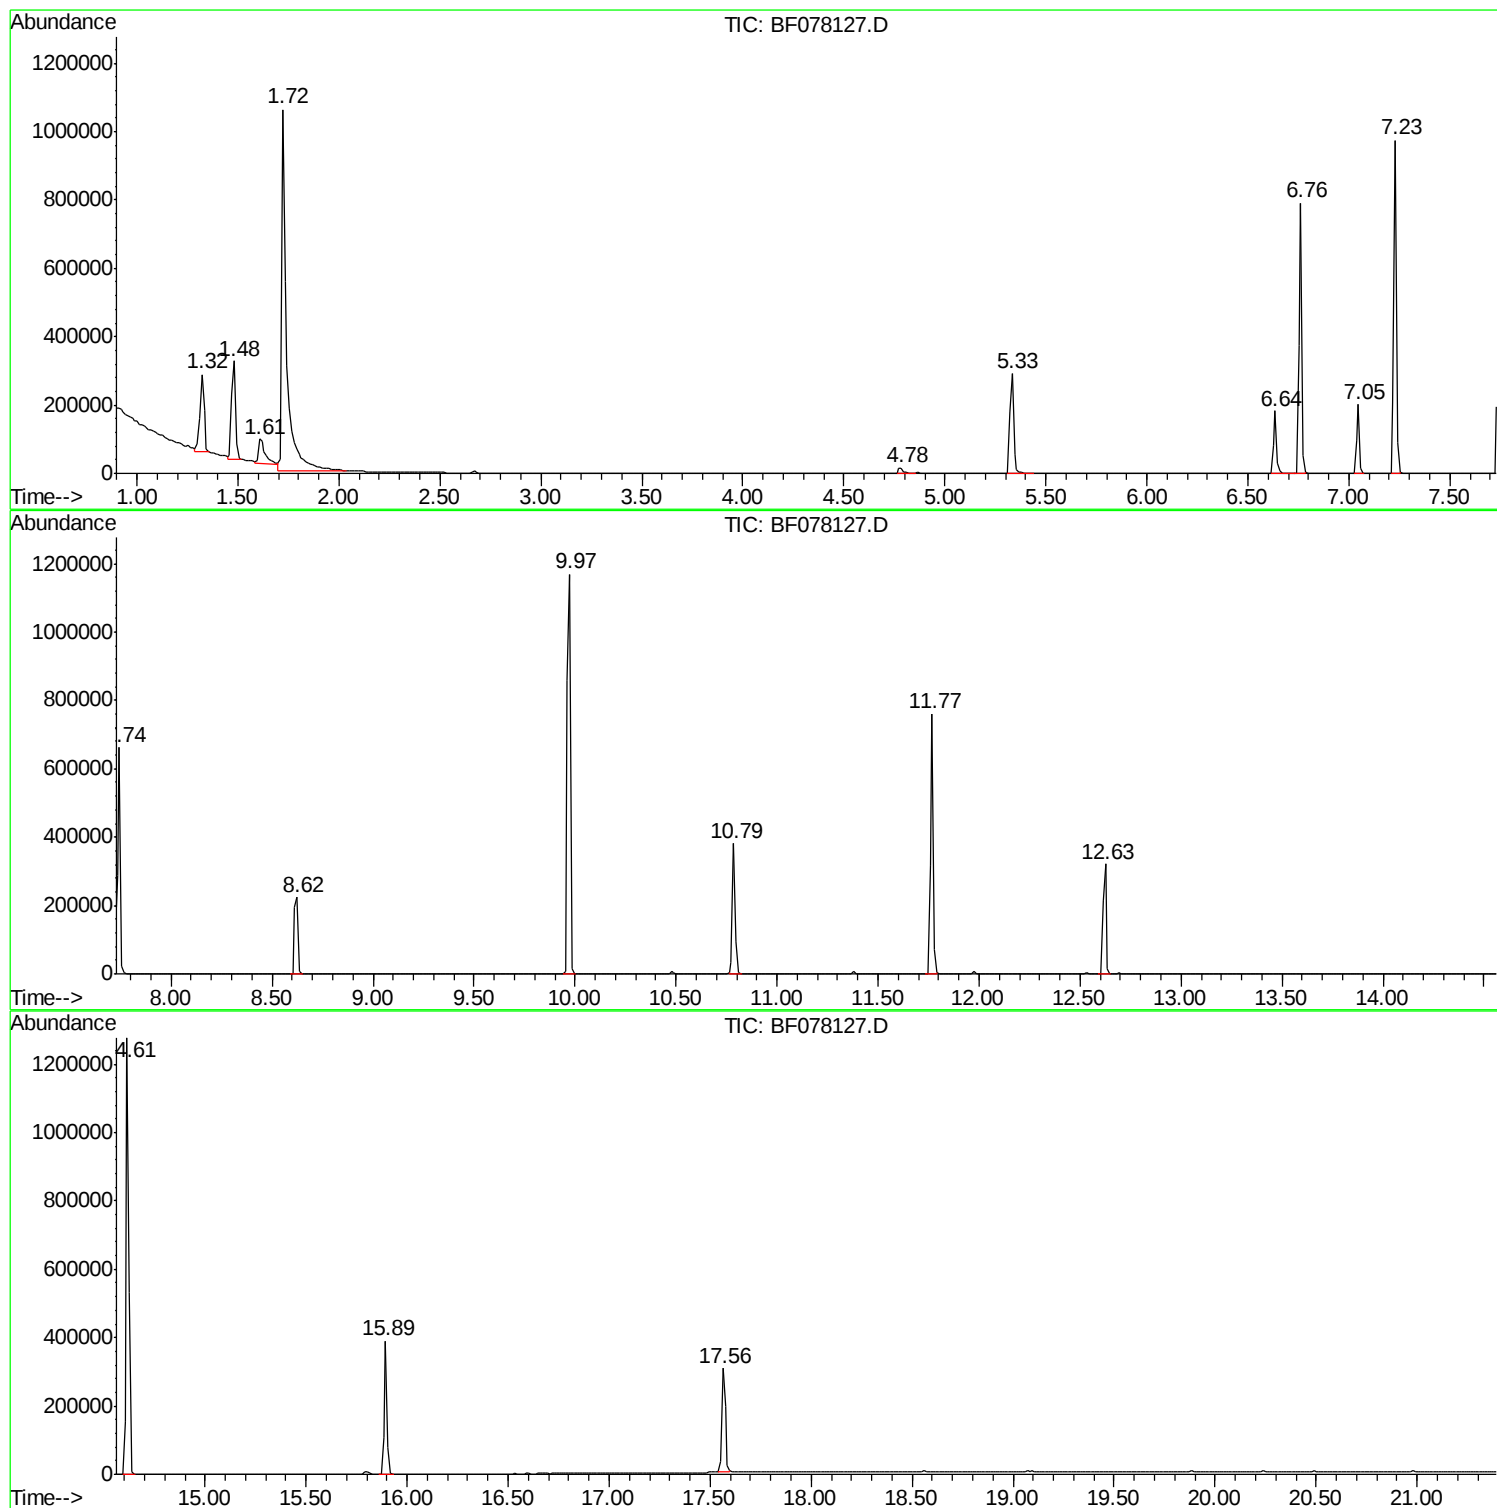

Data Path : Z:\HPCHEM1\BNA F\DATA\BF033115\
Data File : BF078127.D
Acq On : 31 Mar 2015 21:29
Operator : TP/IZ
Sample : G1696-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S32-0461










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Butane, 2-methoxy-2-methyl- Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.48	33.69 ng	365346	1,4-Dichlorobenzene-d4	7.05

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	56
3		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
4		Silane, tetramethyl-	88	C4H12Si	000075-76-3	12
5		1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9

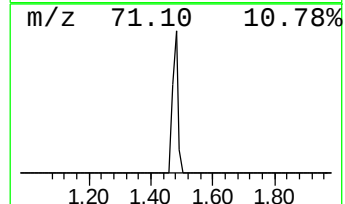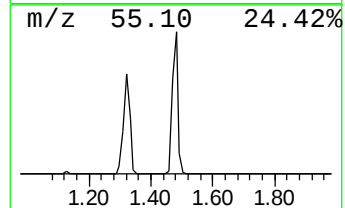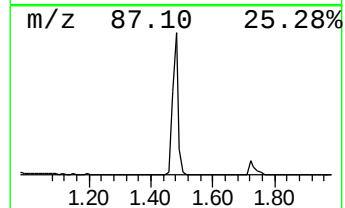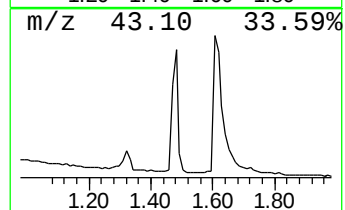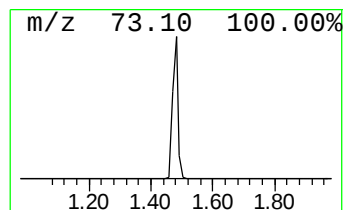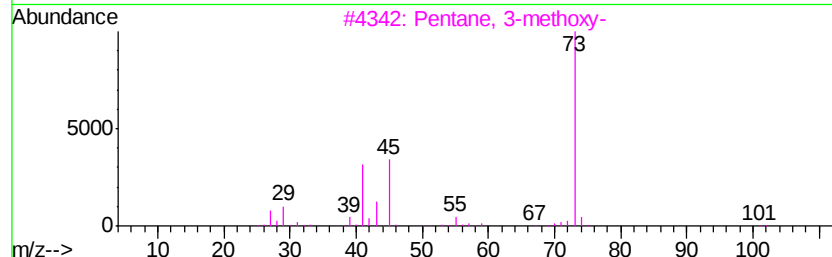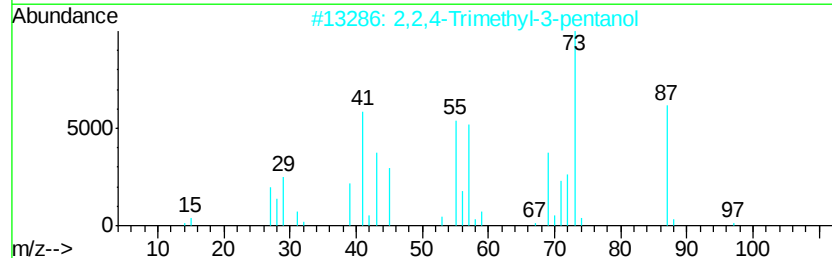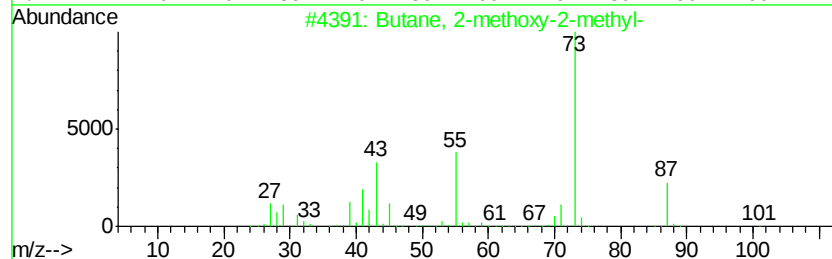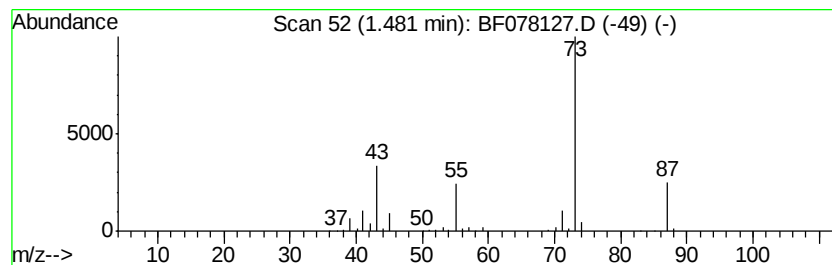

Data Path : Z:\HPCHEM1\BNA F\DATA\BF033115\
Data File : BF078127.D
Acq On : 31 Mar 2015 21:29
Operator : TP/IZ
Sample : G1696-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S32-0461









Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 unknown6.76 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.76	77.37 ng	839162	1,4-Dichlorobenzene-d4	7.05

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

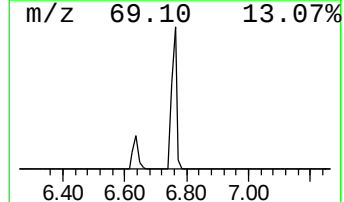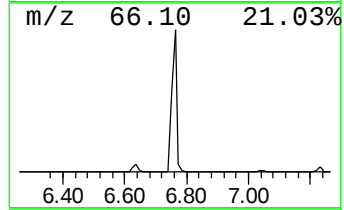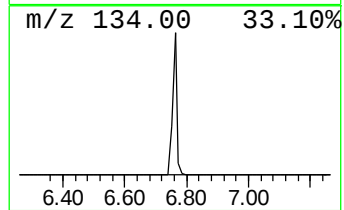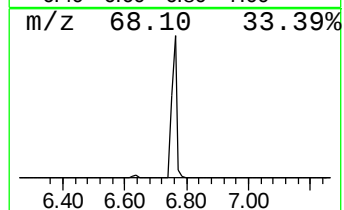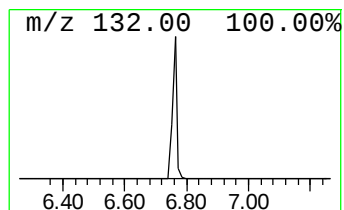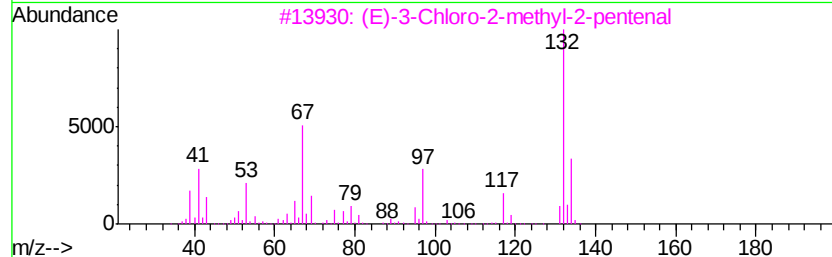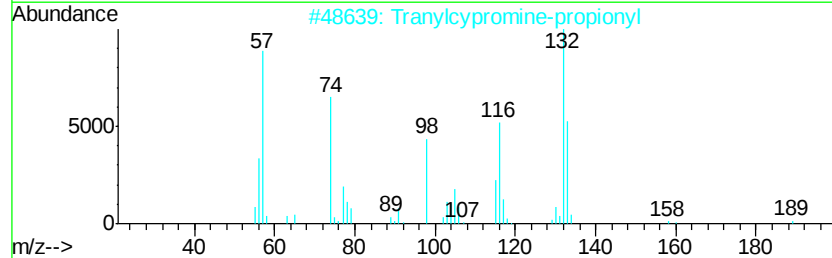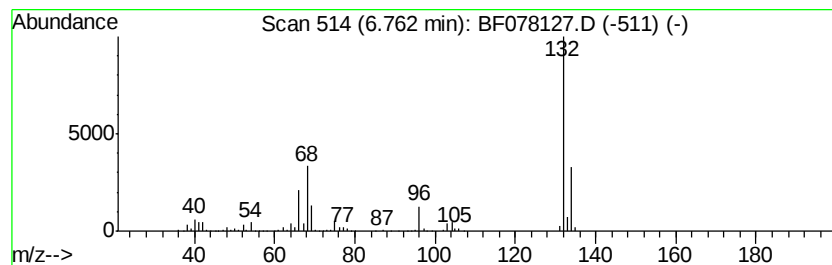

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033115\
Data File : BF078127.D
Acq On : 31 Mar 2015 21:29
Operator : TP/IZ
Sample : G1696-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S32-0461

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	1.48	33.7	ng	365346	1	7.05	216914	20.0
unknown6.76	6.76	77.4	ng	839162	1	7.05	216914	20.0