
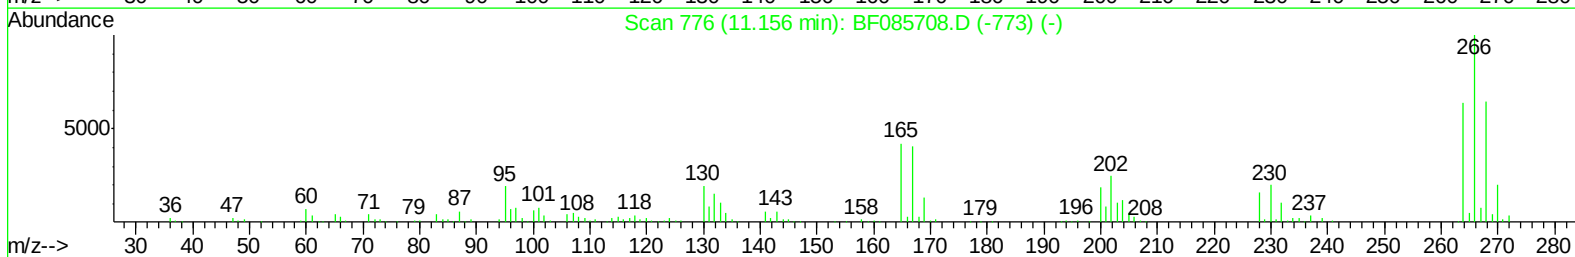
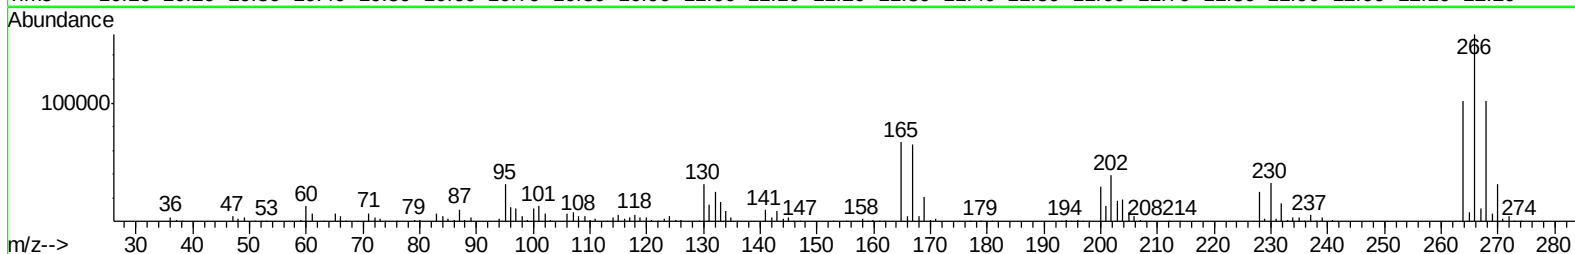


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033116\
Data File : BF085922.D
Acq On : 31 Mar 2016 12:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 03:36:08 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 30 12:31:18 2016
Response via : Initial Calibration

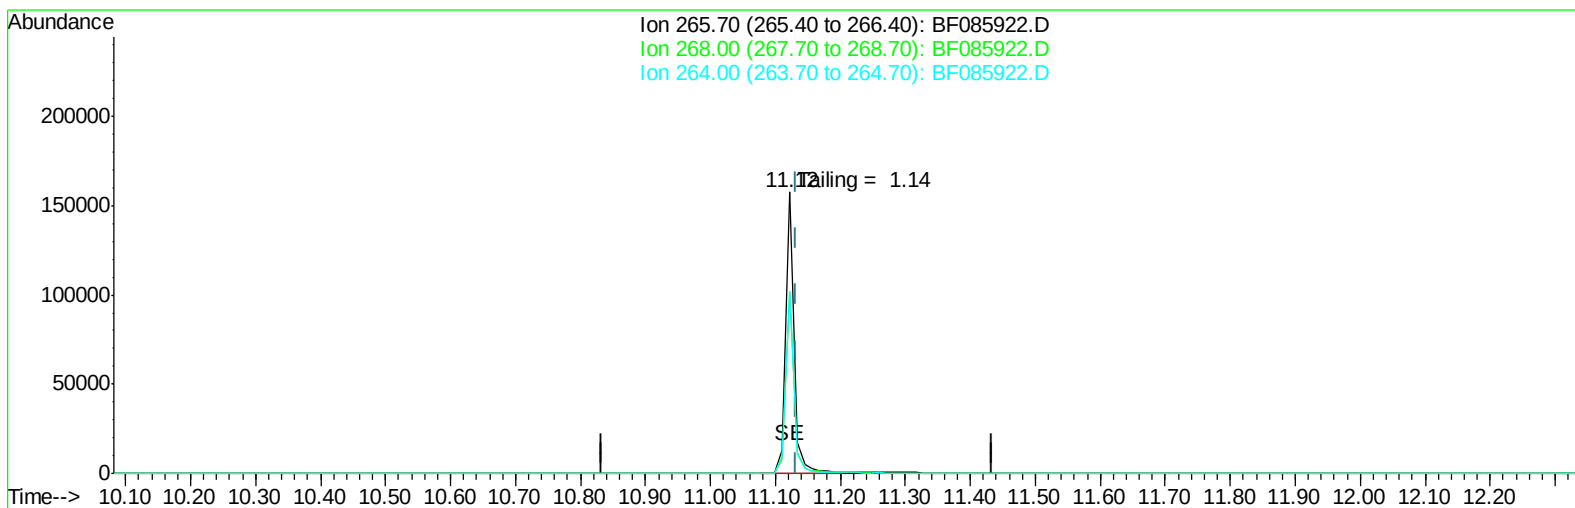

TIC: BF085922.D

(69) Pentachlorophenol (C)




11.122min (-0.012) 74325.55ng

response 141327

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.39
264.00	63.30	64.58
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033116\
Data File : BF085922.D
Acq On : 31 Mar 2016 12:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 03:36:08 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 30 12:31:18 2016
Response via : Initial Calibration

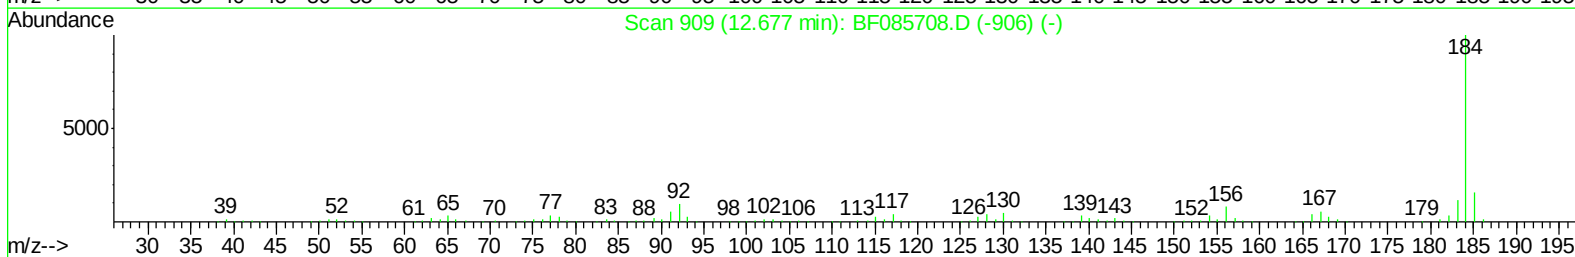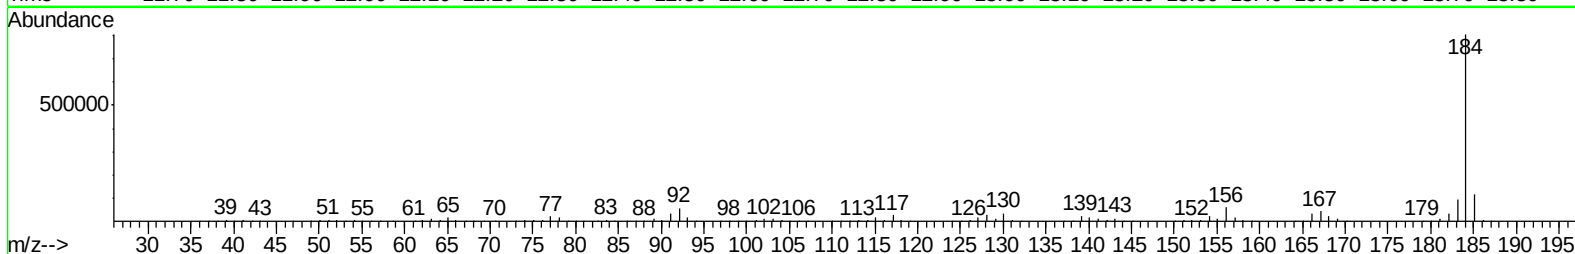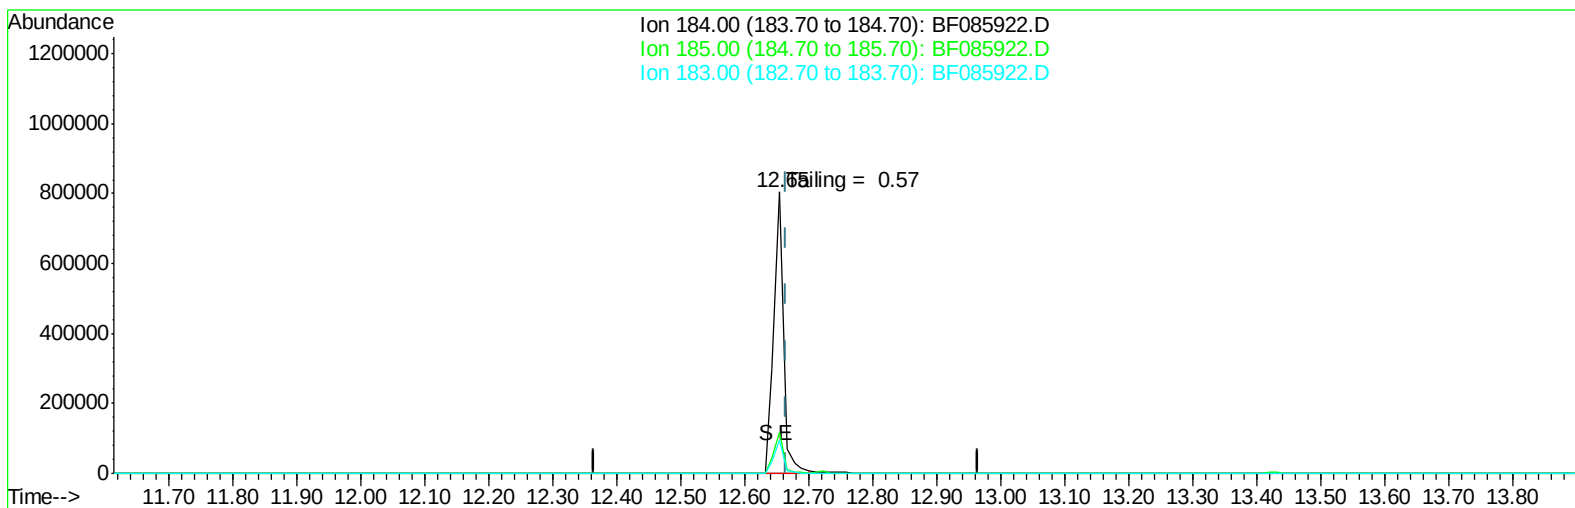

TIC: BF085922.D

(76) Benzidine

12.653min (-0.012) 43506.87ng

response 861102

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.38
183.00	11.80	11.97
0.00	0.00	0.00