

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033116\
 Data File : BF085935.D
 Acq On : 31 Mar 2016 18:52
 Operator : UM/SJ
 Sample : H1976-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-6

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.373	268	270	286	rBV	843996	1239728	36.62%	6.163%
2	6.424	360	362	371	rBV	767275	781883	23.10%	3.887%
3	6.550	371	373	376	rBV	2029172	2160225	63.82%	10.739%
4	6.790	392	394	396	rBV	575979	611635	18.07%	3.040%
5	6.939	405	407	410	rBV	1851152	2069735	61.14%	10.289%
6	7.362	441	444	446	rBV	1343511	1870896	55.27%	9.300%
7	8.070	504	506	509	rBV	865464	806880	23.84%	4.011%
8	9.156	598	601	603	rBV	3274695	3384984	100.00%	16.827%
9	9.545	633	635	637	rBV	65100	66939	1.98%	0.333%
10	9.830	657	660	662	rBV	857891	843285	24.91%	4.192%
11	10.619	726	729	731	rBV	1929474	1838302	54.31%	9.138%
12	10.733	737	739	743	rVB	40724	46340	1.37%	0.230%
13	11.305	787	789	792	rBV2	603473	761113	22.48%	3.784%
14	11.842	834	836	838	rBV	63864	70269	2.08%	0.349%
15	12.631	902	905	913	rBV3	22975	49670	1.47%	0.247%
16	12.894	926	928	931	rBV	2413953	2292563	67.73%	11.397%
17	13.796	1004	1007	1011	rBV2	29654	48448	1.43%	0.241%
18	13.945	1018	1020	1023	rVB	609745	540934	15.98%	2.689%
19	14.117	1032	1035	1037	rBV3	22041	50092	1.48%	0.249%
20	14.208	1040	1043	1047	rVB6	35436	58725	1.73%	0.292%
21	15.362	1141	1144	1147	rBV	431649	523648	15.47%	2.603%


Sum of corrected areas: 20116294

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033116\
Data File : BF085935.D
Acq On : 31 Mar 2016 18:52
Operator : UM/SJ
Sample : H1976-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-6

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

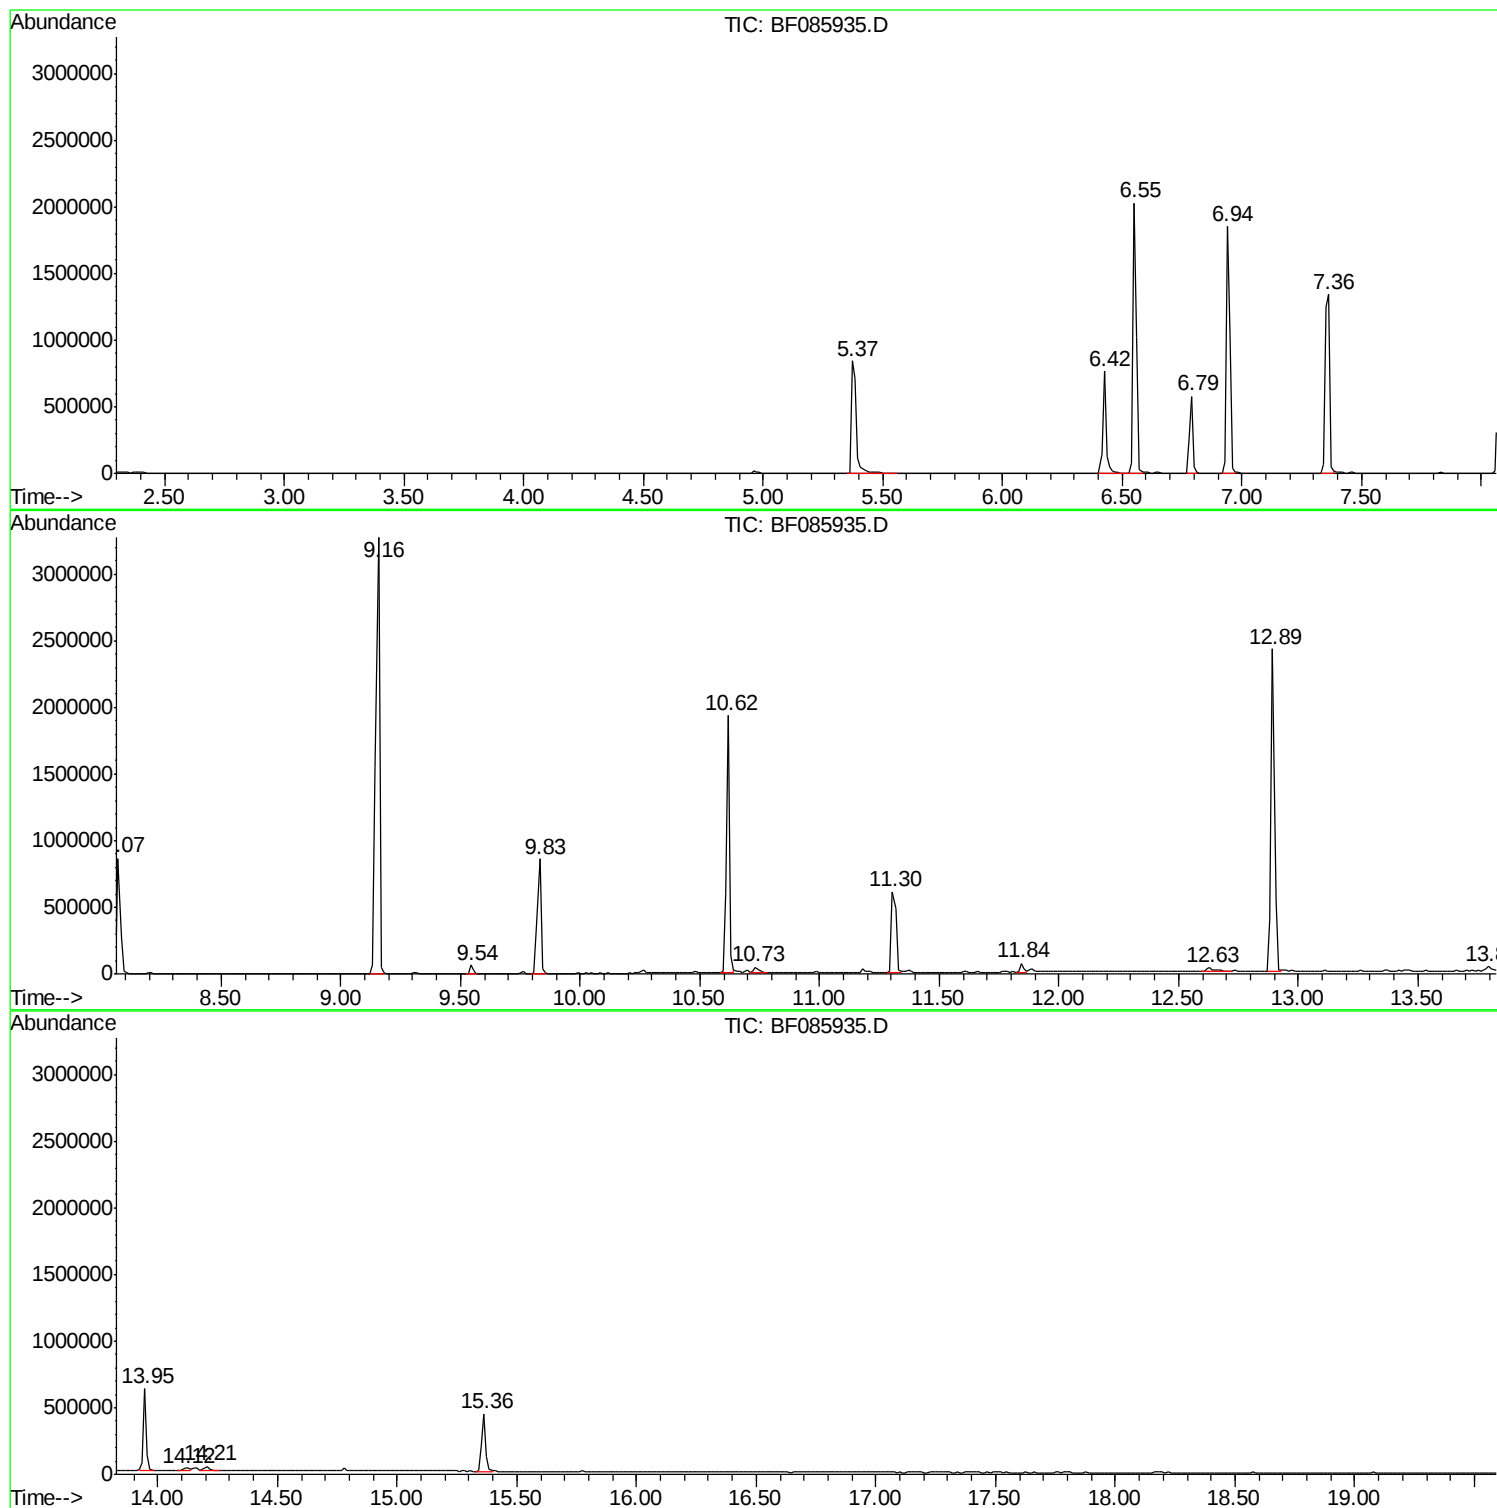

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033116\
Data File : BF085935.D
Acq On : 31 Mar 2016 18:52
Operator : UM/SJ
Sample : H1976-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-6










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.55 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.55	70.64 ng	2160230	1,4-Dichlorobenzene-d4	6.79

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2			5-Aminoindole	132	C8H8N2	005192-03-0	12
3			Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
4			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5			1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	9

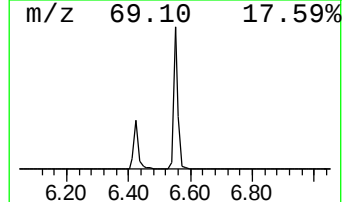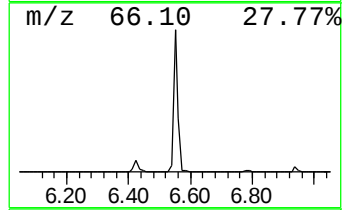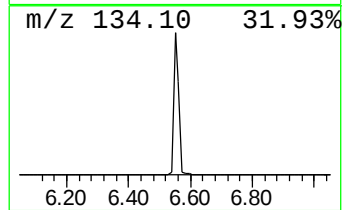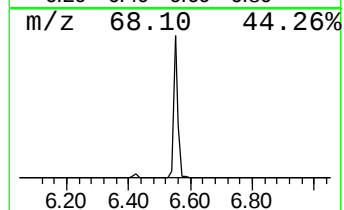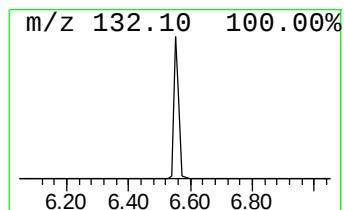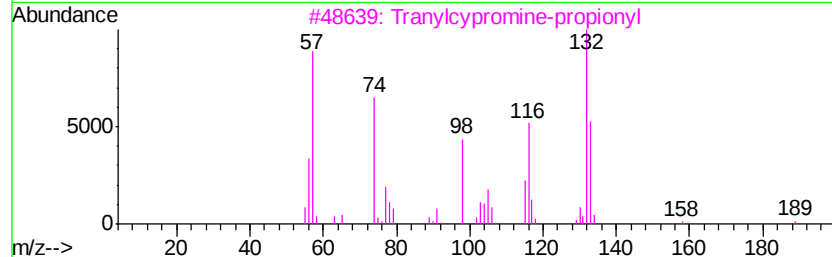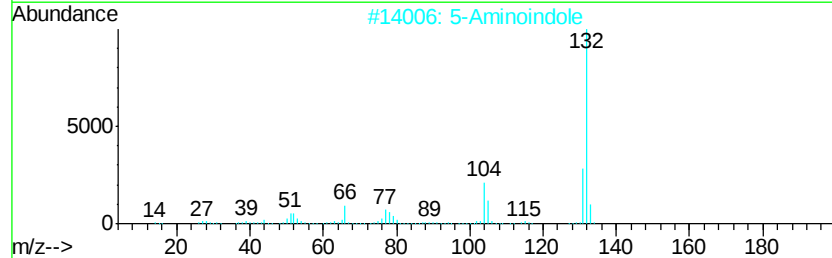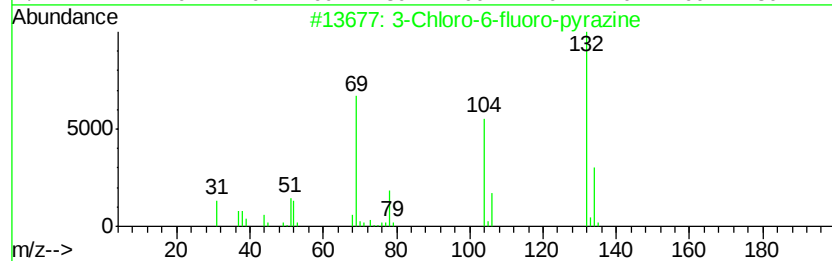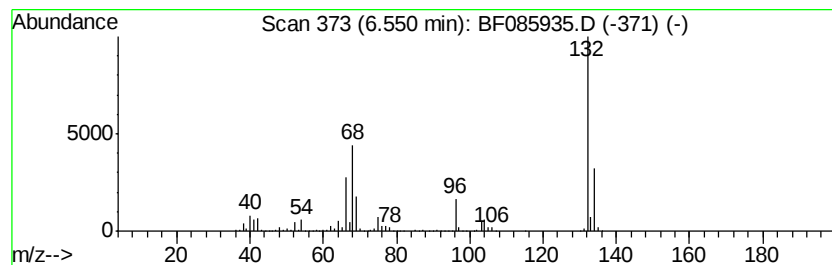

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033116\
Data File : BF085935.D
Acq On : 31 Mar 2016 18:52
Operator : UM/SJ
Sample : H1976-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-6

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.55	6.55	70.6	ng	2160230	1	6.79	611635	20.0