

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033116\
 Data File : BF085937.D
 Acq On : 31 Mar 2016 19:50
 Operator : UM/SJ
 Sample : H1976-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.961	232	234	244	rBV	28038	41249	1.10%	0.181%
2	5.384	269	271	273	rBV	1135623	1394900	37.23%	6.113%
3	6.424	360	362	371	rBV	1040478	983432	26.25%	4.310%
4	6.550	371	373	376	rBV	1974685	2490412	66.47%	10.914%
5	6.790	391	394	396	rBV	681164	691201	18.45%	3.029%
6	6.939	405	407	410	rBV	1944071	2349546	62.71%	10.296%
7	7.362	441	444	446	rBV	1891160	2184560	58.31%	9.573%
8	8.070	504	506	509	rBV	917108	890620	23.77%	3.903%
9	9.156	598	601	603	rBV	3759540	3746603	100.00%	16.419%
10	9.545	633	635	637	rBV	116022	111436	2.97%	0.488%
11	9.830	657	660	662	rBV	958678	953798	25.46%	4.180%
12	10.265	694	698	699	rBV	43911	50580	1.35%	0.222%
13	10.619	726	729	731	rBV	2105708	2011023	53.68%	8.813%
14	10.733	737	739	743	rBV	65815	72961	1.95%	0.320%
15	11.179	776	778	780	rBV	42897	42356	1.13%	0.186%
16	11.305	787	789	792	rBV	636993	850402	22.70%	3.727%
17	11.842	834	836	842	rBV	43884	52698	1.41%	0.231%
18	12.631	902	905	910	rBV3	23864	48517	1.29%	0.213%
19	12.894	926	928	931	rBV	2544124	2641538	70.50%	11.576%
20	13.796	1004	1007	1011	rBV2	25803	44453	1.19%	0.195%
21	13.945	1018	1020	1023	rVB	649775	586164	15.65%	2.569%
22	15.362	1141	1144	1147	rBV	457717	580902	15.50%	2.546%


Sum of corrected areas: 22819351

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033116\
Data File : BF085937.D
Acq On : 31 Mar 2016 19:50
Operator : UM/SJ
Sample : H1976-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

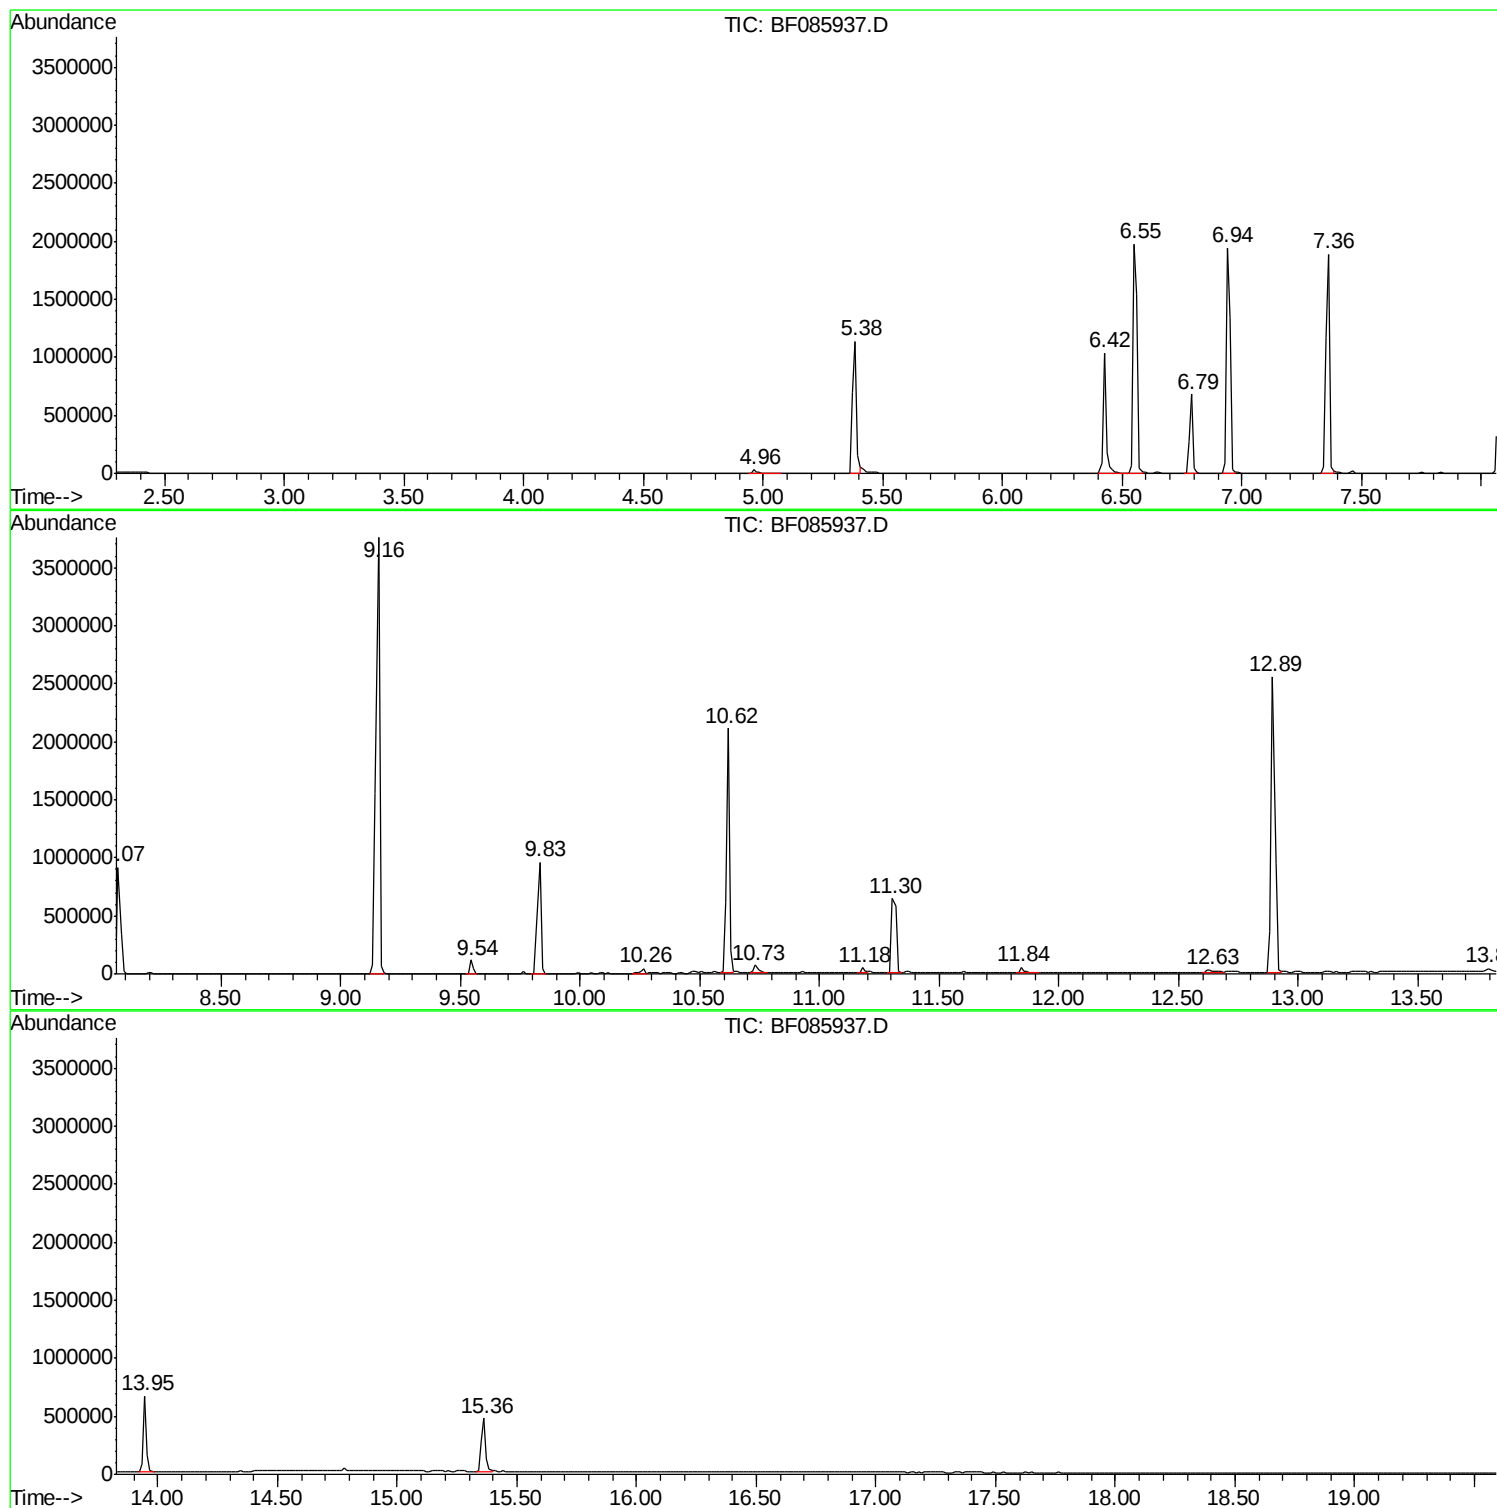

DbaaaPathh::ZZ\NRP8888M1BBAFNDATA\B0033166\
 DbaaaFile::BB0089937DD
 Aeqq00n ::331Mar2006 199500
 Oppaaaor ::UMMSJ
 Sample ::H0906004
 Misc ::
 ASSVaal ::166 SampleMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :
 MW-1

QqaattMebbdd::ZZ\NRP8888M1BBAFMEH00S8200BB0324166MM
 QqaattTitle ::ASBPBNASSANDABBSF00R55P000NTC6AIBBATION

TICCLibbaay ::CC\DATA\BBS6EN0\$S002LL
 TICInteggaionPaaameess:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
