


Data Path : Z:\HPCHEM1\BNA_F\Data\BF033116\
 Data File : BF085922.D
 Acq On : 31 Mar 2016 12:27
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 30 12:31:18 2016

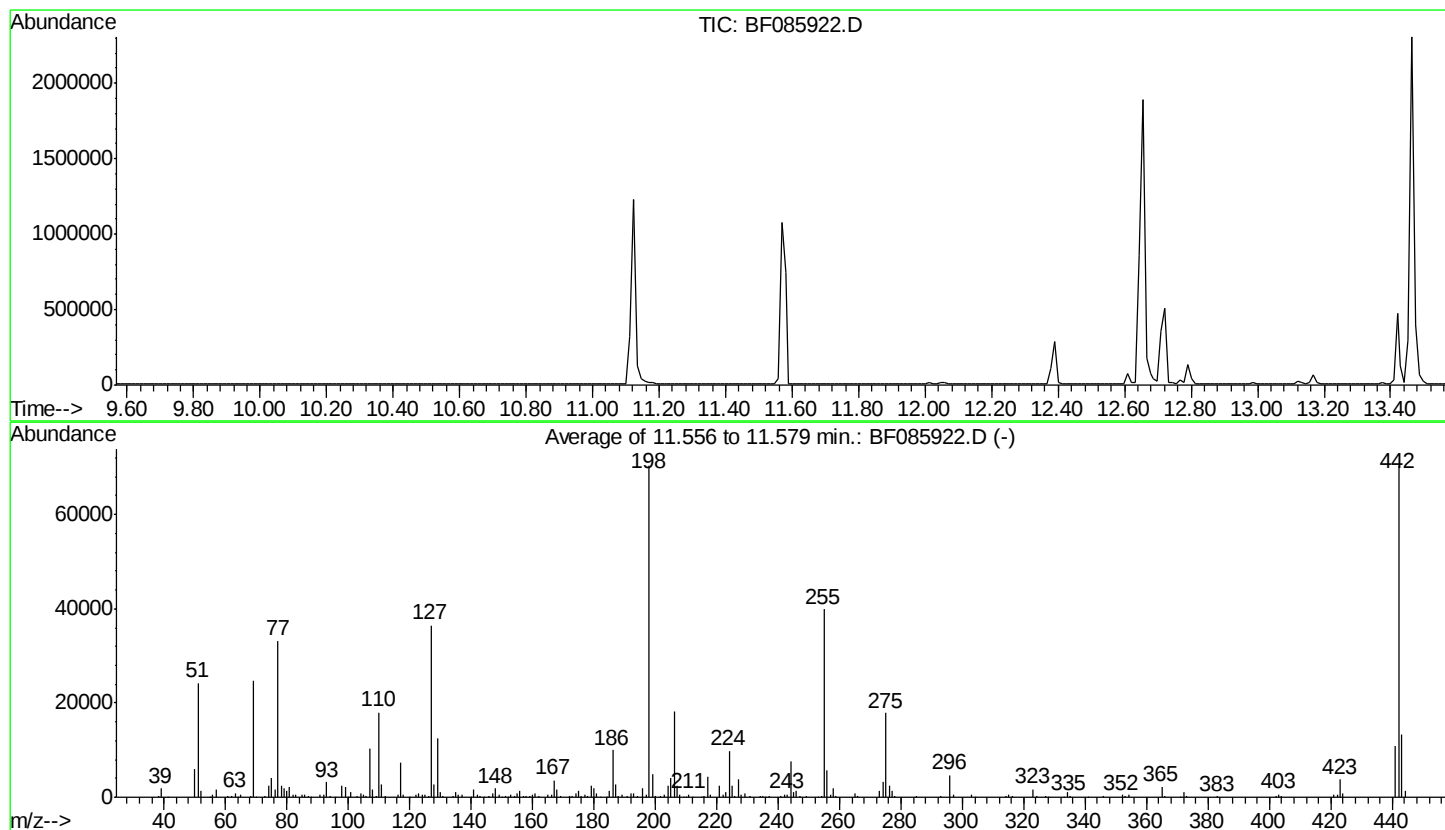

AutoFind: Scans 811, 812, 813; Background Corrected with Scan 808

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	24231	PASS
68	69	0.00	2	1.3	311	PASS
69	198	0.00	100	35.2	24806	PASS
70	69	0.00	2	0.5	134	PASS
127	198	10	80	51.9	36518	PASS
197	198	0.00	2	0.7	515	PASS
198	198	100	100	100.0	70376	PASS
199	198	5	9	6.8	4800	PASS
275	198	10	60	25.5	17925	PASS
365	198	1	100	3.1	2198	PASS
441	442	0.01	24	15.4	10808	PASS
442	198	50	100	100.0	70341	PASS
443	442	15	24	18.9	13327	PASS