


Data Path : Z:\HPCHEM1\BNA_F\Data\BF033116\
Data File : BF085946.D
Acq On : 1 Apr 2016 00:10
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 30 12:31:18 2016

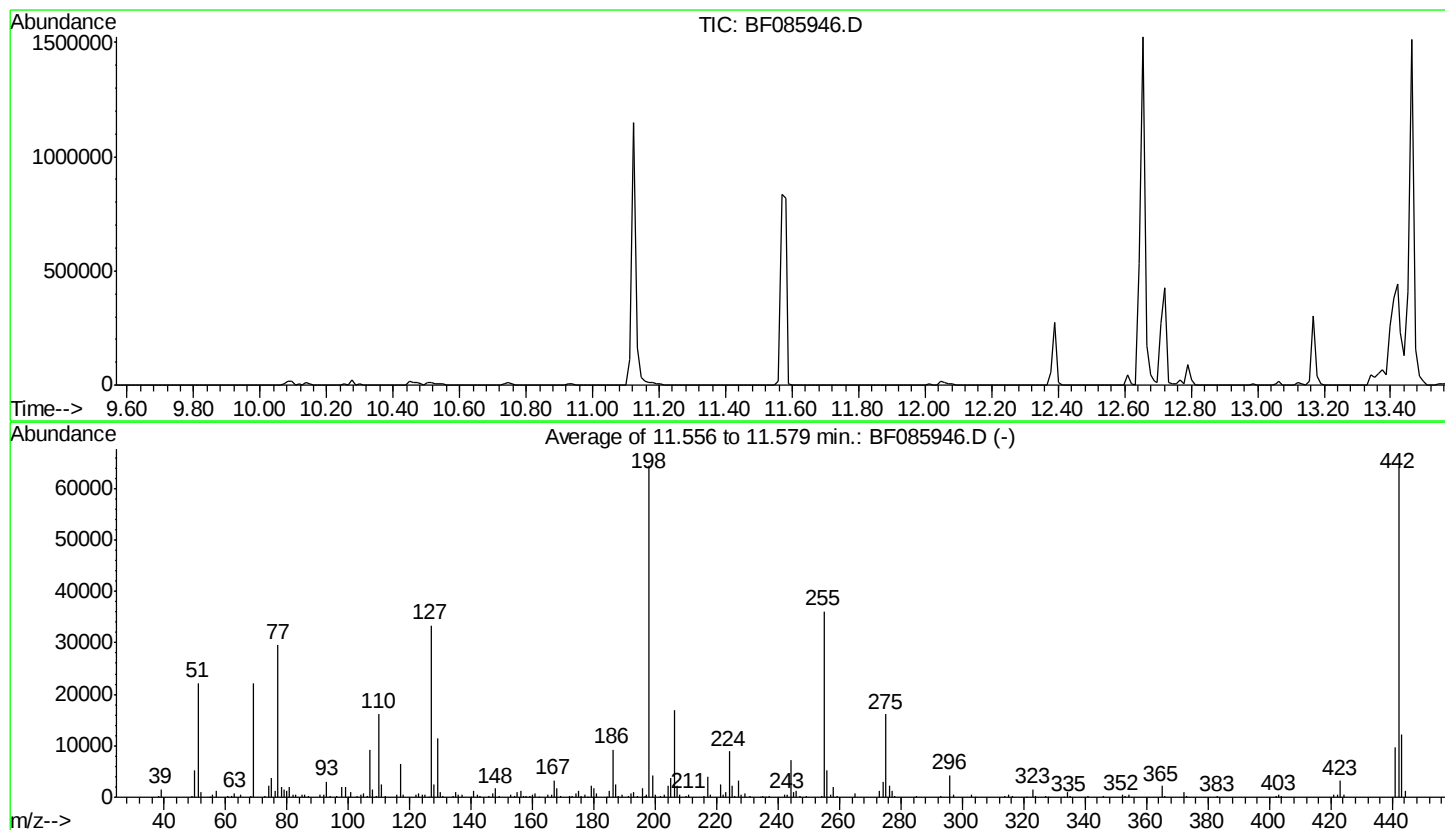

AutoFind: Scans 811, 812, 813; Background Corrected with Scan 808

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	22192	PASS
68	69	0.00	2	1.4	300	PASS
69	198	0.00	100	34.2	22064	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.9	33435	PASS
197	198	0.00	2	0.8	524	PASS
198	198	100	100	100.0	64431	PASS
199	198	5	9	6.6	4267	PASS
275	198	10	60	25.0	16109	PASS
365	198	1	100	3.3	2144	PASS
441	442	0.01	24	15.0	9607	PASS
442	198	50	100	99.4	64064	PASS
443	442	15	24	18.9	12079	PASS