

Data Path : Z:\HPCHEM1\BNA F\DATA\BF033117\
 Data File : BF094102.D
 Acq On : 31 Mar 2017 18:02
 Operator : SJ/MA
 Sample : I2463-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Mar 31 23:09:13 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 14:38:29 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	5.90	152	186370	20.00	ng	0.00
21) Naphthalene-d8	7.40	136	753078	20.00	ng	-0.01
38) Acenaphthene-d10	9.54	164	338208	20.00	ng	-0.01
63) Phenanthrene-d10	11.36	188	564718	20.00	ng	-0.01
75) Chrysene-d12	14.62	240	385423	20.00	ng	-0.01
86) Perylene-d12	16.24	264	284578	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	4.45	112	1441379	130.63	ng	0.01
7) Phenol-d6	5.51	99	1850519	135.56	ng	0.00
23) Nitrobenzene-d5	6.55	82	1190279	90.20	ng	0.00
41) 2,4,6-Tribromophenol	10.52	330	339293	126.95	ng	0.00
44) 2-Fluorobiphenyl	8.73	172	1872716	84.46	ng	0.00
78) Terphenyl-d14	13.35	244	1214901	70.65	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	6.55	70	159790	18.21	ng	# 77
49) Dimethylphthalate	9.22	163	107678	4.48	ng	98
56) 2,4-Dinitrotoluene	9.54	165	44024	6.36	ng	# 33
70) Phenanthrene	11.39	178	90561	2.88	ng	97
74) Fluoranthene	12.86	202	104234	3.24	ng	99
77) Pyrene	13.13	202	98908	3.54	ng	97
82) Chrysene	14.64	228	44466	2.13	ng	# 91
87) Benzo(b)fluoranthene	15.84	252	48576	2.78	ng	# 96
88) Benzo(k)fluoranthene	15.84	252	48576	2.85	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF033117\
Data File : BF094102.D
Acq On : 31 Mar 2017 18:02
Operator : SJ/MA
Sample : I2463-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Mar 31 23:09:13 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 14:38:29 2017
Response via : Initial Calibration

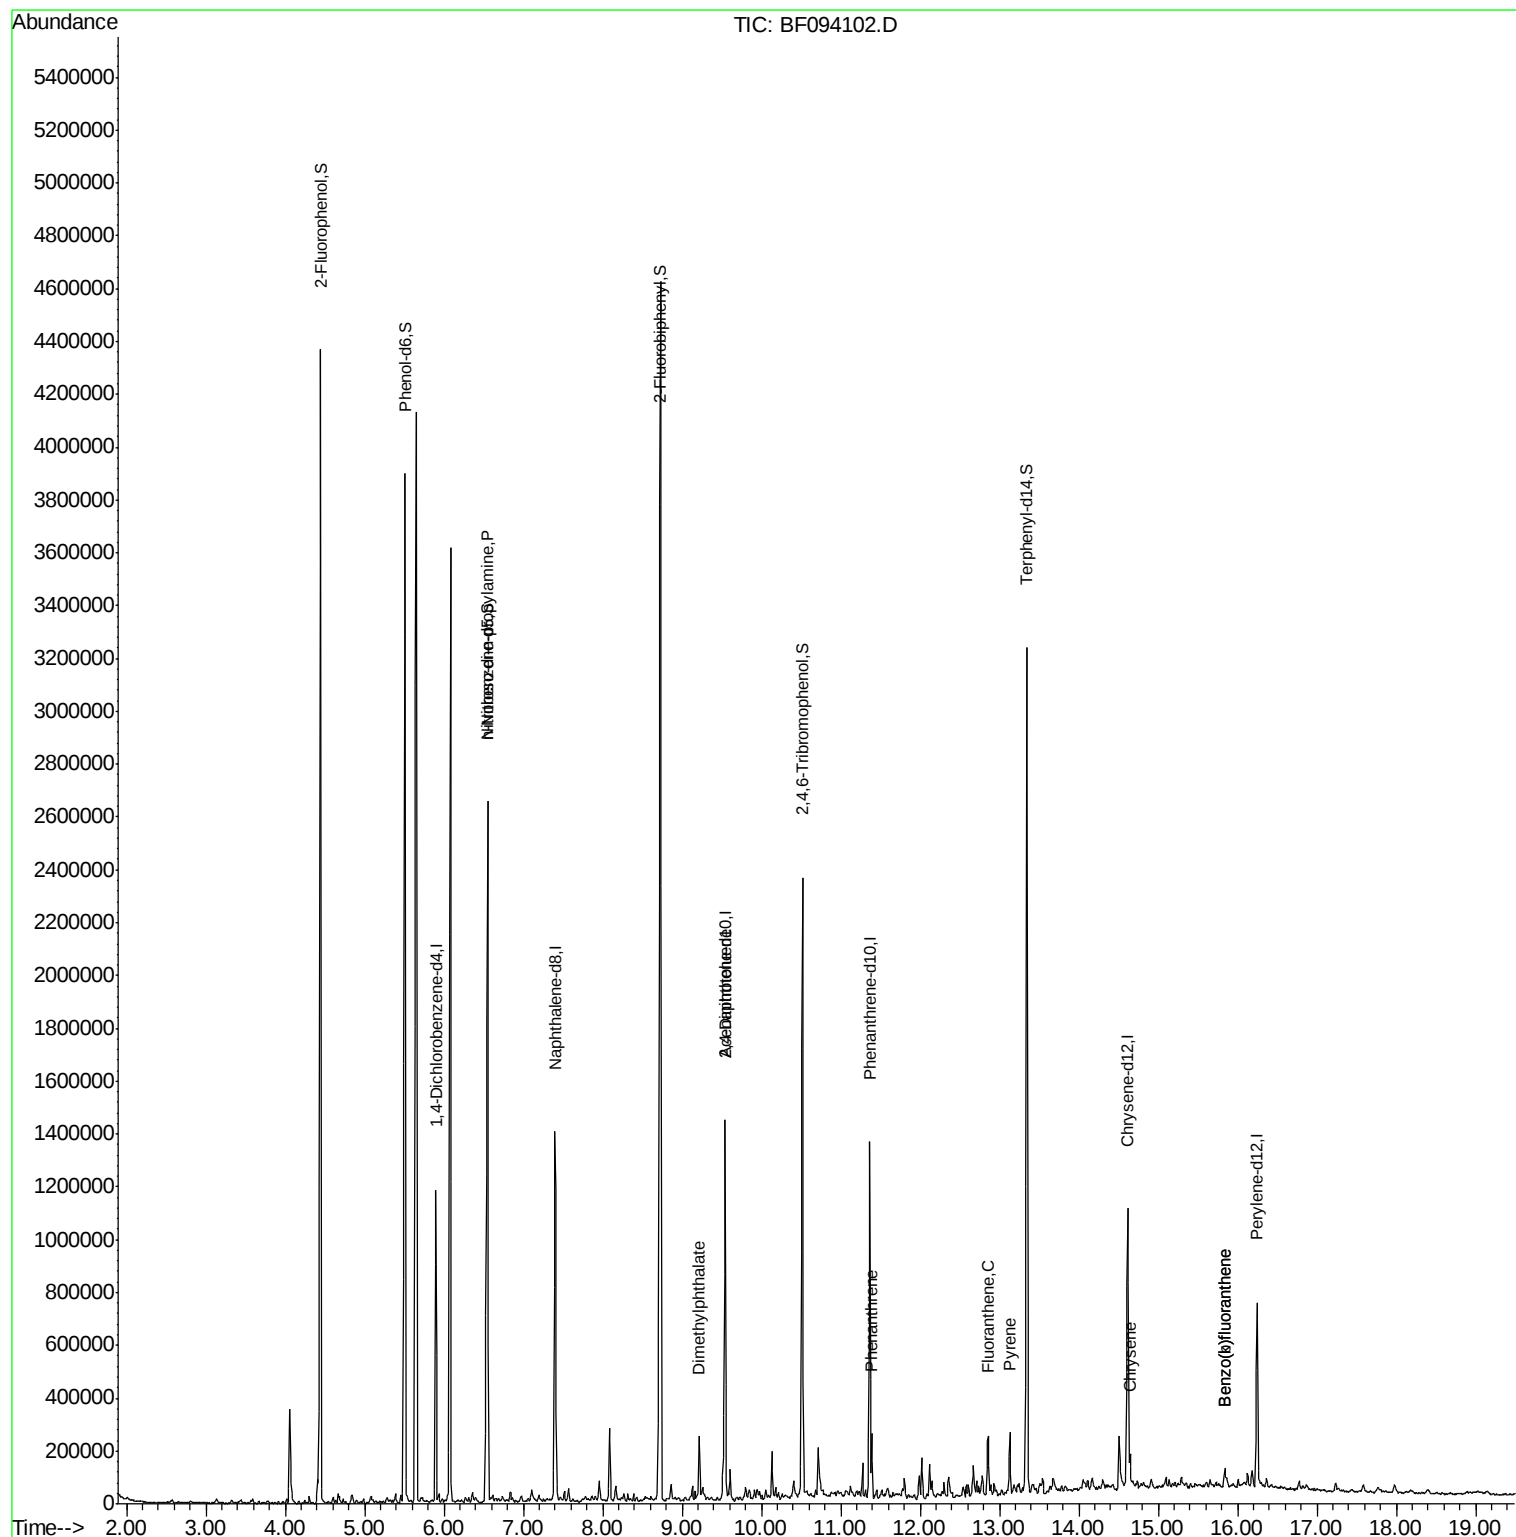

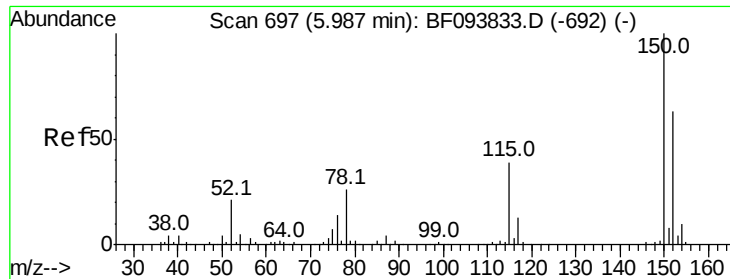

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 5.90 min Scan# 682

Delta R.T. -0.01 min

Lab File: BF094102.D

Acq: 31 Mar 2017 18:02

Instrument :

BNA_F

ClientSampled :


Tot Ion:152 Resp: 186370

Ion Ratio Lower Upper

152 100

150 157.5 126.2 189.2




115 60.6 52.2 78.2

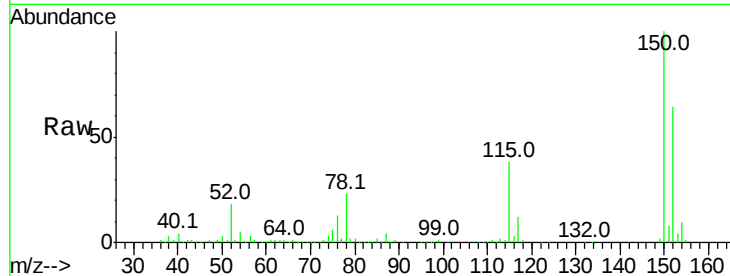

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

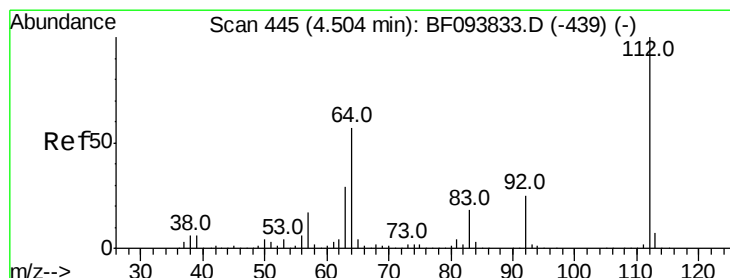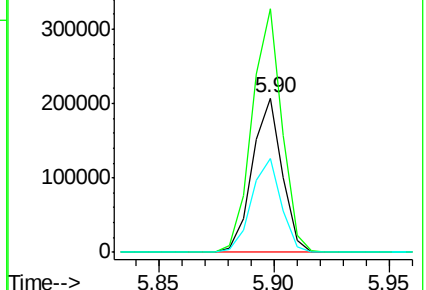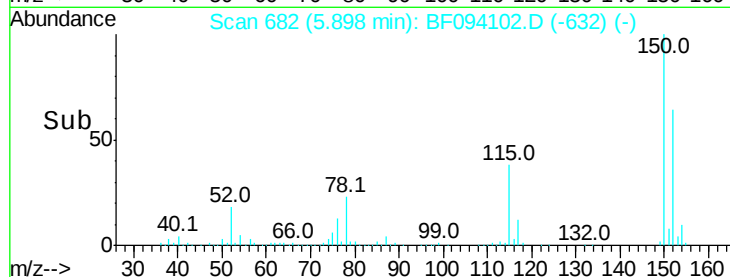

#5

2-Fluorophenol

Concen: 130.63 ng

RT: 4.45 min Scan# 435

Delta R.T. 0.01 min

Lab File: BF094102.D

Acq: 31 Mar 2017 18:02


Tgt Ion:112 Resp: 1441379

Ion Ratio Lower Upper

112 100

64 56.8 46.0 69.0



63 28.5 23.4 35.0



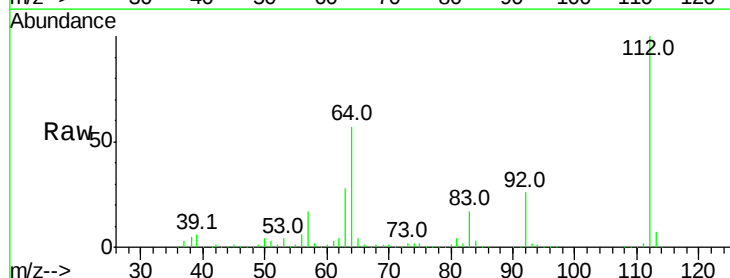


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

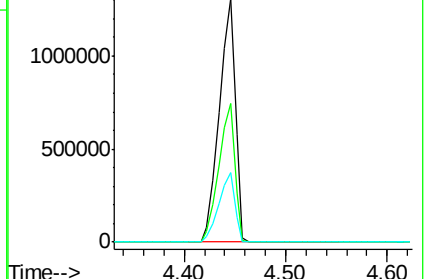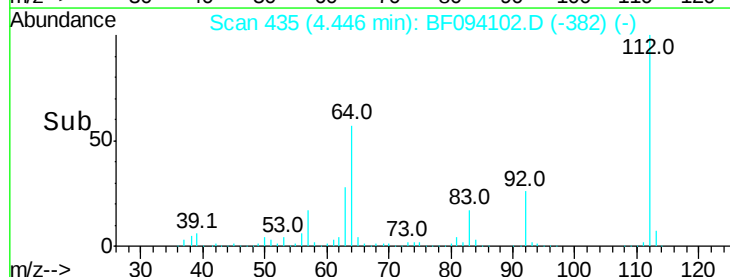

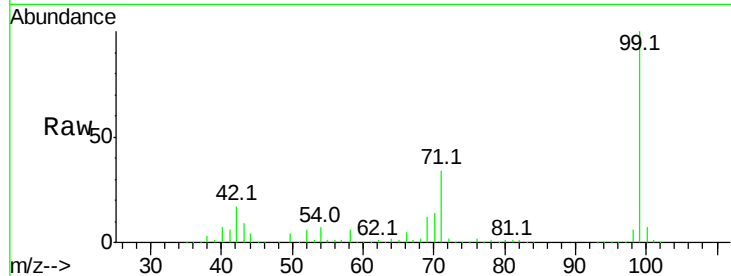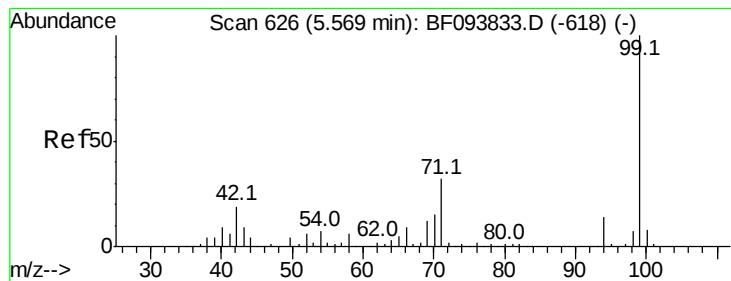

#7

Phenol-d6

Concen: 135.56 ng

RT: 5.51 min Scan# 616

Delta R.T. 0.00 min

Lab File: BF094102.D

Acq: 31 Mar 2017 18:02

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 1850519

Ion Ratio Lower Upper

99 100

42 17.4 13.5 20.3

71 34.3 24.5 36.7

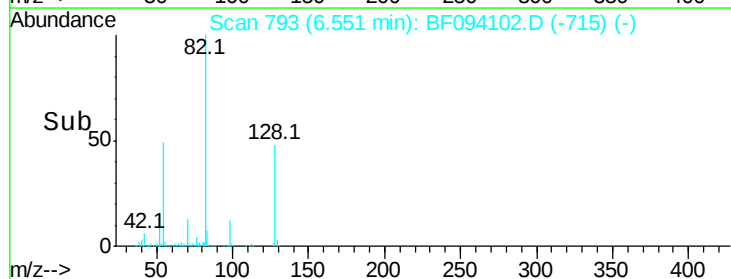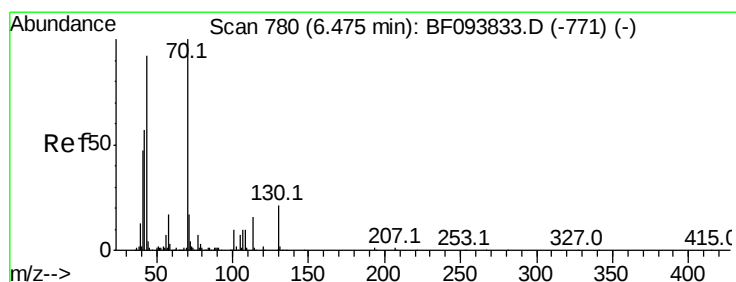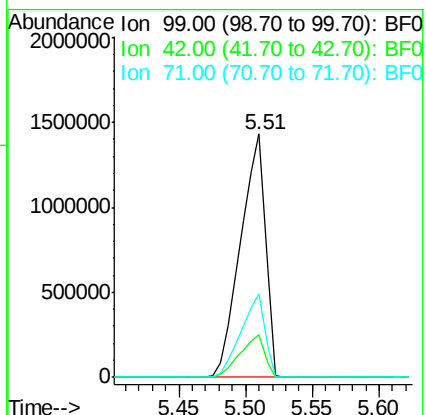

#19

n-Nitroso-di-n-propylamine

Concen: 18.21 ng

RT: 6.55 min Scan# 793

Delta R.T. 0.16 min

Lab File: BF094102.D

Acq: 31 Mar 2017 18:02

Tgt Ion: 70 Resp: 159790


Ion Ratio Lower Upper

70 100

42 45.7 47.2 70.8#

101 0.0 7.2 10.8#

130 2.5 15.9 23.9#

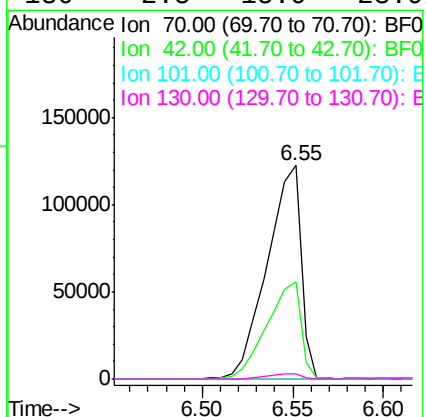



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.40 min Scan# 937

Delta R.T. -0.01 min

Lab File: BF094102.D

Acq: 31 Mar 2017 18:02

Instrument :

BNA_F

ClientSampled :

Tot Ion:136 Resp: 753078



Ion Ratio Lower Upper

136 100

137 11.1 8.5 12.7

54 7.3 4.9 7.3#

68 6.1 4.1 6.1

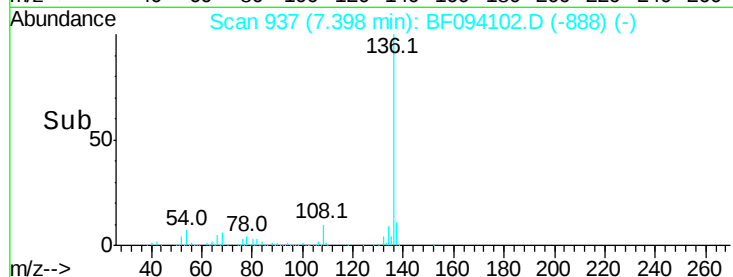
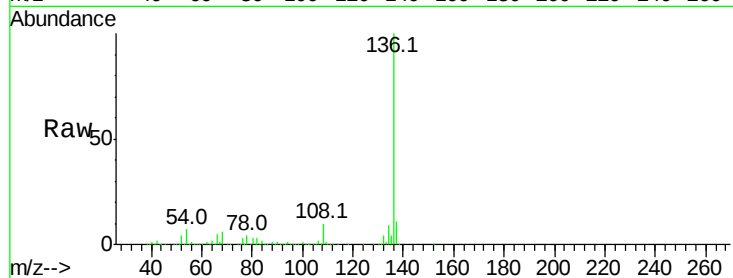


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

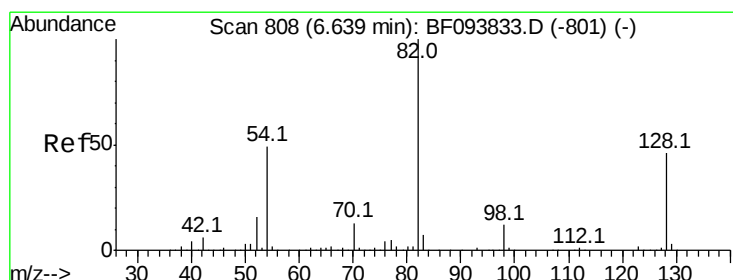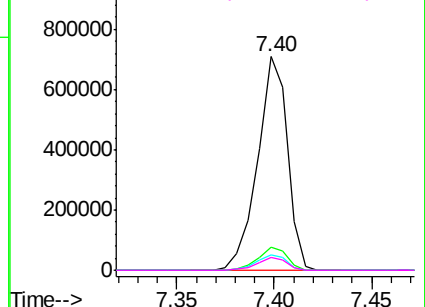

#23

Nitrobenzene-d5

Concen: 90.20 ng

RT: 6.55 min Scan# 793

Delta R.T. -0.01 min

Lab File: BF094102.D

Acq: 31 Mar 2017 18:02



Tgt Ion: 82 Resp: 1190279

Ion Ratio Lower Upper

82 100

128 48.1 34.0 51.0


54 48.7 42.2 63.2

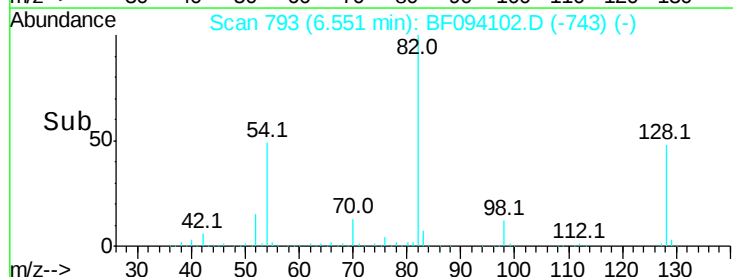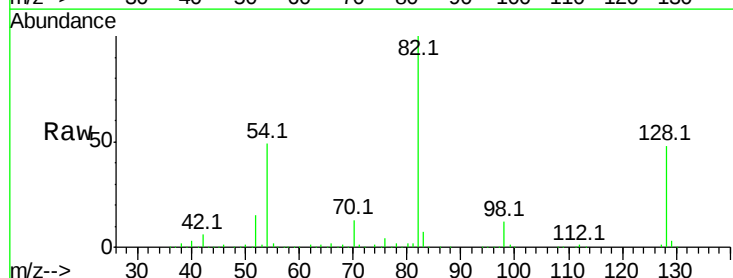


Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

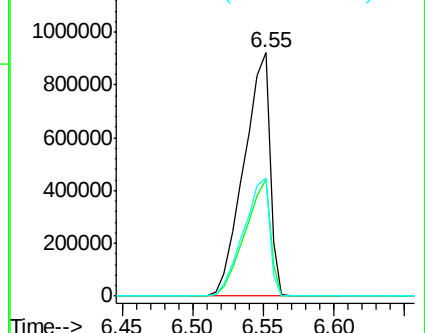


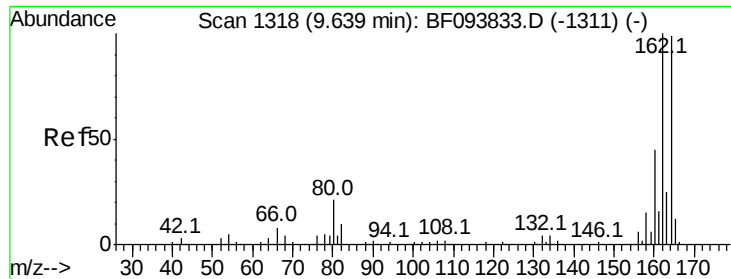



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.54 min Scan# 1301
Delta R.T. -0.01 min
Lab File: BF094102.D
Acq: 31 Mar 2017 18:02

Instrument :
BNA_F
ClientSampleId :

Tot Ion:164 Resp: 338208
Ion Ratio Lower Upper
164 100
162 101.8 82.6 123.8
160 43.8 36.2 54.2




Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E


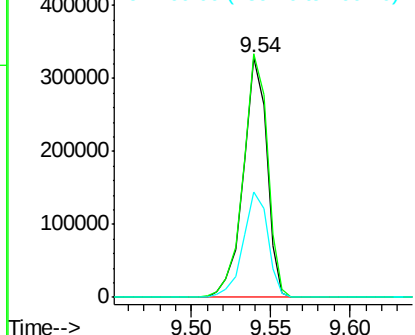


#41
2,4,6-Tribromophenol
Concen: 126.95 ng
RT: 10.52 min Scan# 1468
Delta R.T. 0.00 min
Lab File: BF094102.D
Acq: 31 Mar 2017 18:02

Tgt Ion:330 Resp: 339293
Ion Ratio Lower Upper
330 100
332 96.9 76.6 115.0
141 38.4 31.4 47.2



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

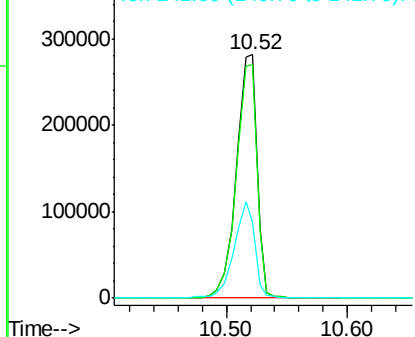







#44
 2-Fluorobiphenyl
 Concen: 84.46 ng
 RT: 8.73 min Scan# 1163
 Delta R.T. -0.01 min
 Lab File: BF094102.D
 Acq: 31 Mar 2017 18:02

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:172 Resp: 1872716




Ion	Ratio	Lower	Upper
172	100		
171	37.0	29.6	44.4
170	24.6	19.8	29.8

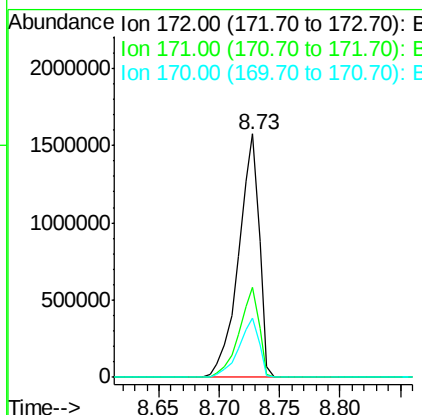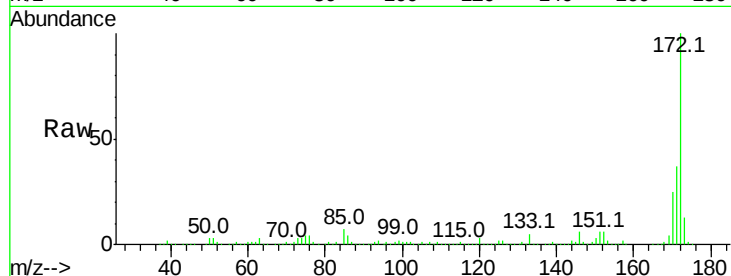

#49
 Dimethylphthalate
 Concen: 4.48 ng
 RT: 9.22 min Scan# 1246
 Delta R.T. -0.03 min
 Lab File: BF094102.D
 Acq: 31 Mar 2017 18:02

Tgt Ion:163 Resp: 107678

Ion	Ratio	Lower	Upper
163	100		
194	3.4	2.6	4.0
164	11.3	8.4	12.6

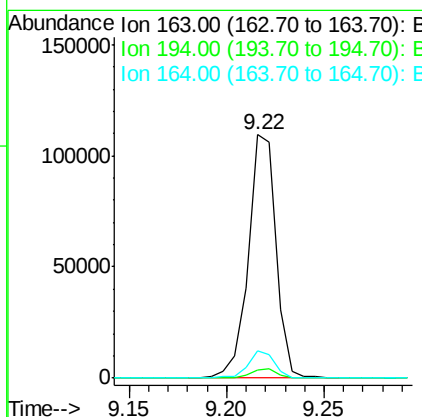







#56
 2,4-Dinitrotoluene
 Concen: 6.36 ng
 RT: 9.54 min Scan# 1301
 Delta R.T. -0.26 min
 Lab File: BF094102.D
 Acq: 31 Mar 2017 18:02

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:165 Resp: 44024
 Ion Ratio Lower Upper
 165 100
 63 1.5 25.4 38.0#
 89 1.3 46.4 69.6#
 182 0.0 1.8 2.6#




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0
 Ion 182.00 (181.70 to 182.70): E

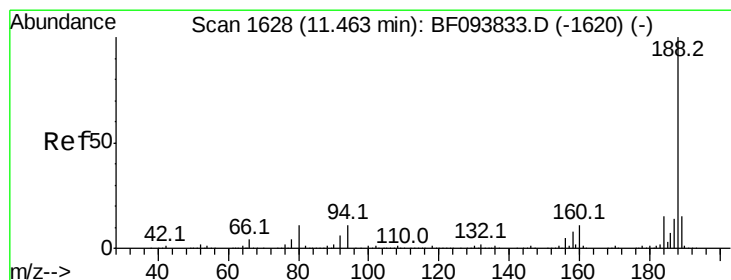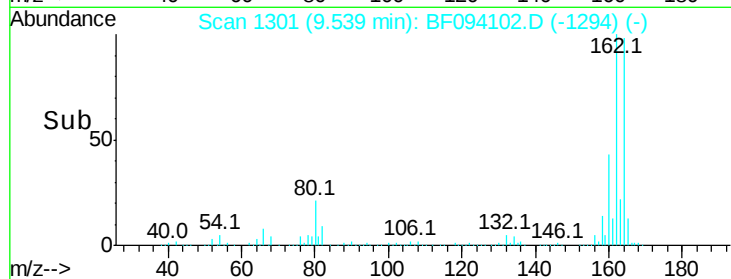
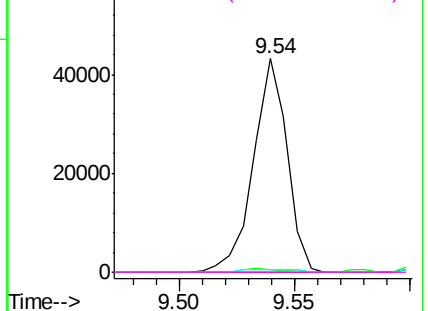



#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.36 min Scan# 1611
 Delta R.T. -0.01 min
 Lab File: BF094102.D
 Acq: 31 Mar 2017 18:02

Tgt Ion:188 Resp: 564718
 Ion Ratio Lower Upper
 188 100
 94 11.7 9.4 14.2
 80 11.8 10.2 15.2

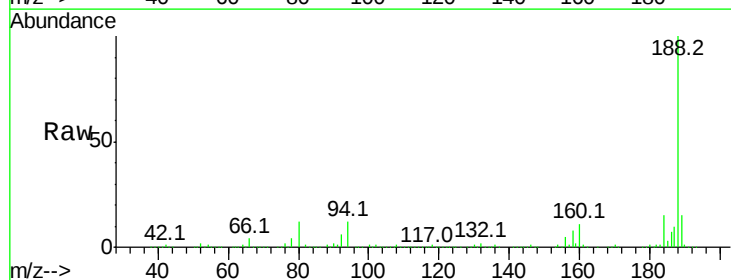

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

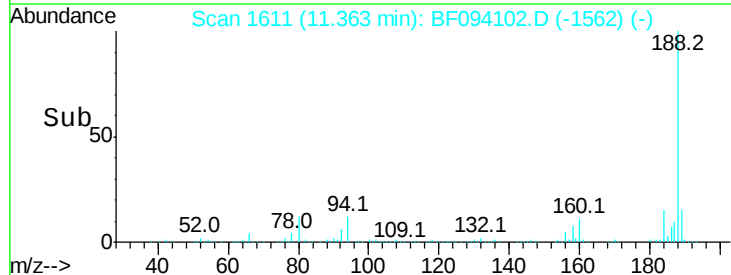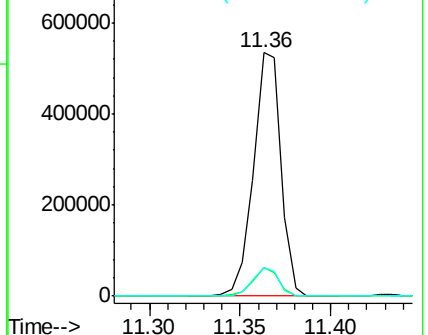



#70

Phenanthrene

Concen: 2.88 ng

RT: 11.39 min Scan# 1616

Delta R.T. -0.01 min

Lab File: BF094102.D

Acq: 31 Mar 2017 18:02

Instrument :

BNA_F

ClientSampleId :


Tot Ion:178 Resp: 90561

Ion Ratio Lower Upper

178 100

176 18.5 16.2 24.4




179 15.1 12.6 19.0



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

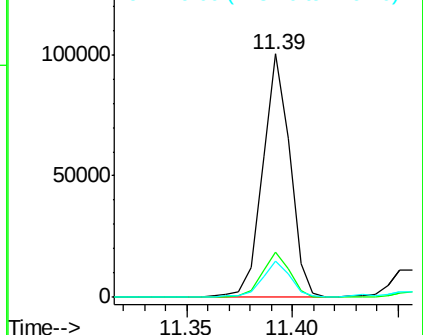

#74

Fluoranthene

Concen: 3.24 ng

RT: 12.86 min Scan# 1865

Delta R.T. -0.01 min

Lab File: BF094102.D

Acq: 31 Mar 2017 18:02


Tgt Ion:202 Resp: 104234

Ion Ratio Lower Upper

202 100

101 12.6 0.0 33.2



203 17.5 0.0 38.1




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

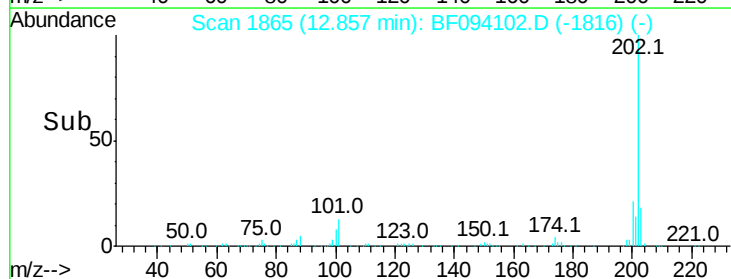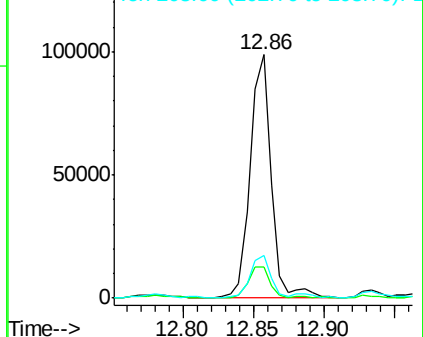



#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.62 min Scan# 2164

Delta R.T. -0.01 min

Lab File: BF094102.D

Acq: 31 Mar 2017 18:02

Instrument :

BNA_F

ClientSampled :


Tot Ion:240 Resp: 385423

Ion Ratio Lower Upper

240 100

120 14.6 5.8 8.8#




236 26.0 20.5 30.7



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

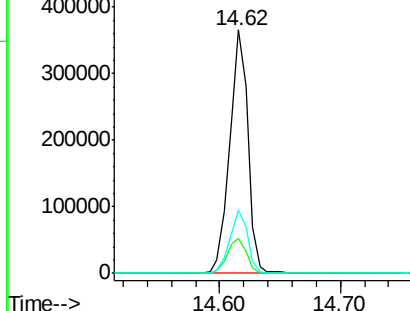

#77

Pyrene

Concen: 3.54 ng

RT: 13.13 min Scan# 1912

Delta R.T. -0.01 min

Lab File: BF094102.D

Acq: 31 Mar 2017 18:02


Tgt Ion:202 Resp: 98908

Ion Ratio Lower Upper

202 100

200 19.9 17.6 26.4



203 18.7 14.4 21.6




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E



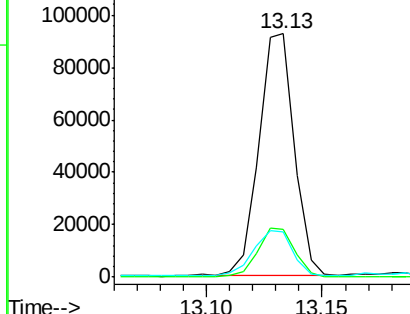





#78
 Terphenyl-d14
 Concen: 70.65 ng
 RT: 13.35 min Scan# 1948
 Delta R.T. -0.01 min
 Lab File: BF094102.D
 Acq: 31 Mar 2017 18:02




Instrument :
 BNA_F
 ClientSampled :


Tot Ion:244 Resp: 1214901
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.0 9.0
 122 14.3 10.3 15.5

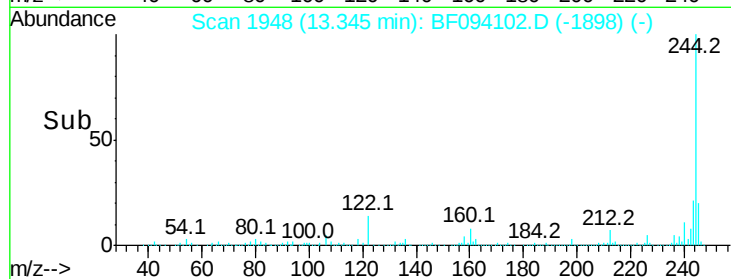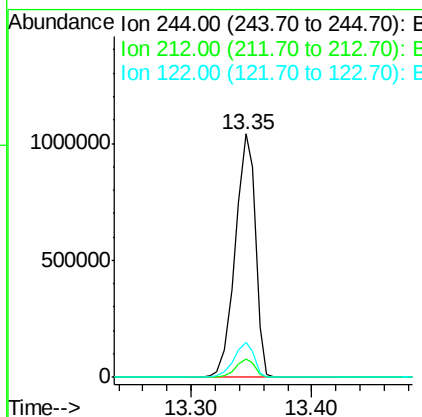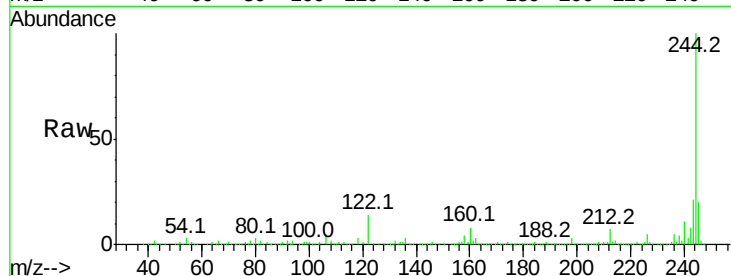

#82
 Chrysene
 Concen: 2.13 ng
 RT: 14.64 min Scan# 2169
 Delta R.T. -0.02 min
 Lab File: BF094102.D
 Acq: 31 Mar 2017 18:02

Tgt Ion:228 Resp: 44466
 Ion Ratio Lower Upper
 228 100
 226 33.6 24.9 37.3
 229 27.1 15.8 23.6#

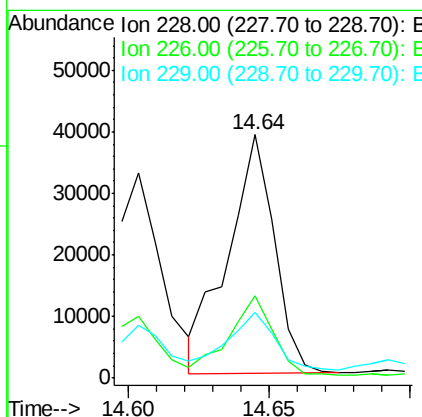


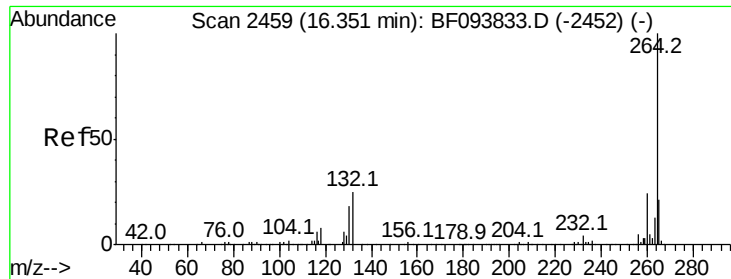




#86
Pervlene-d12
Concen: 20.00 ng
RT: 16.24 min Scan# 2441
Delta R.T. -0.01 min
Lab File: BF094102.D
Acq: 31 Mar 2017 18:02

Instrument :
BNA_F
ClientSampleId :

Tot Ion:264 Resp: 284578
Ion Ratio Lower Upper
264 100
260 23.4 19.5 29.3
265 22.6 17.2 25.8

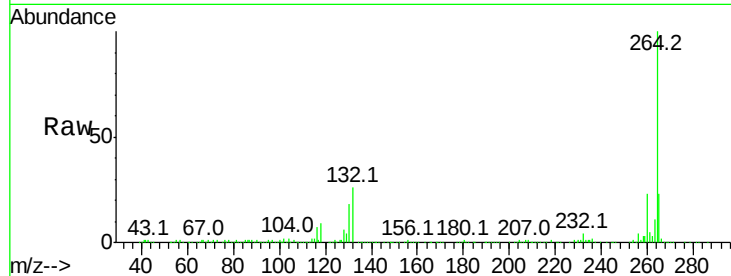


Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E


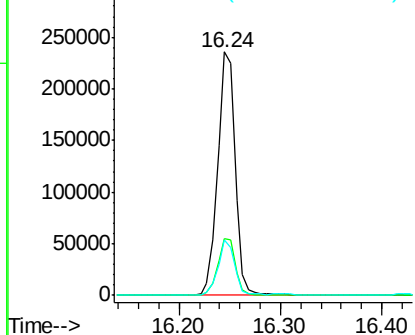



#87
Benzo(b)fluoranthene
Concen: 2.78 ng
RT: 15.84 min Scan# 2372
Delta R.T. -0.01 min
Lab File: BF094102.D
Acq: 31 Mar 2017 18:02

Tgt Ion:252 Resp: 48576
Ion Ratio Lower Upper
252 100
253 22.5 18.1 27.1
125 17.2 9.8 14.8#



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

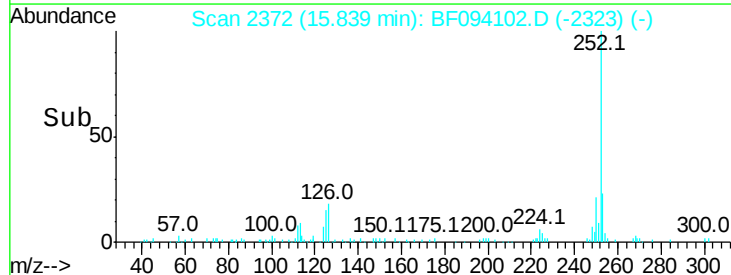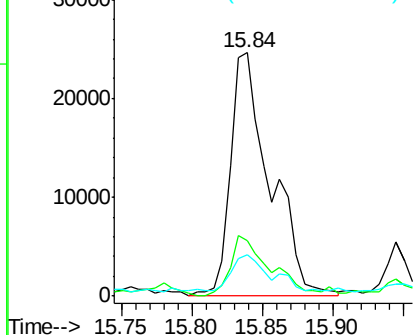

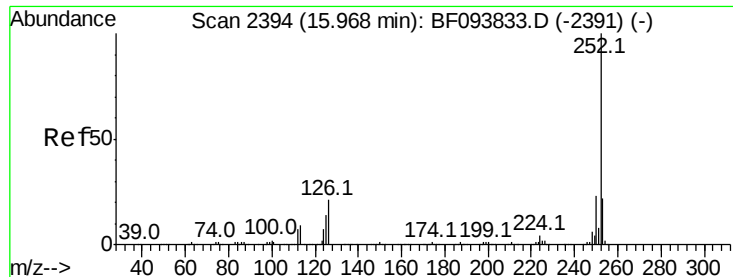

#88

Benzo(k)fluoranthene

Concen: 2.85 ng

RT: 15.84 min Scan# 2372

Delta R.T. -0.04 min

Lab File: BF094102.D

Acq: 31 Mar 2017 18:02

Instrument :

BNA_F

ClientSampleId :


Tot Ion:252 Resp: 48576

Ion Ratio Lower Upper

252 100

253 22.5 18.4 27.6

125 17.2 13.1 19.7

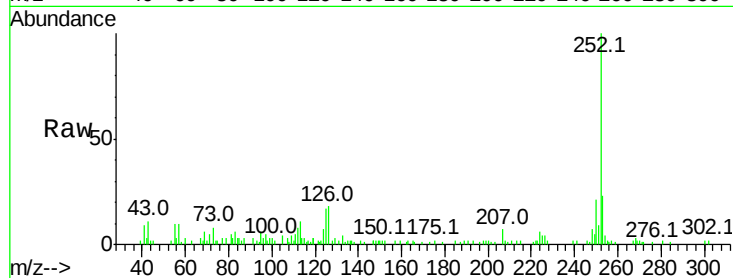

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

