
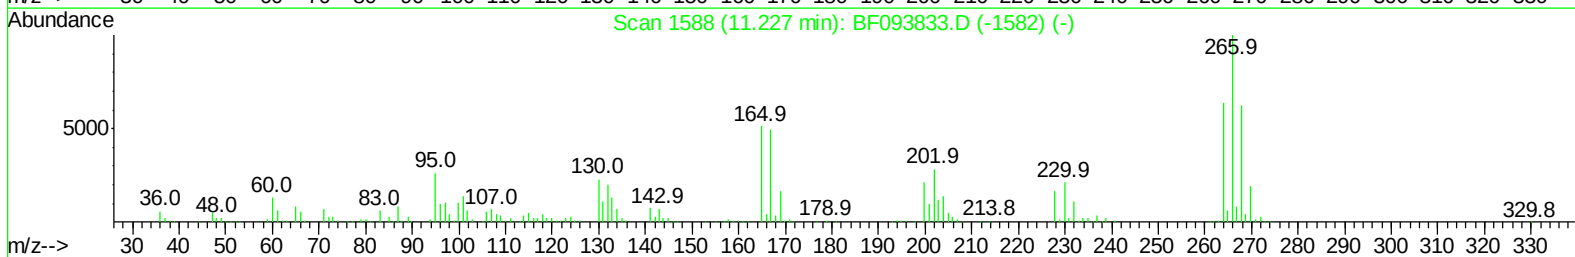
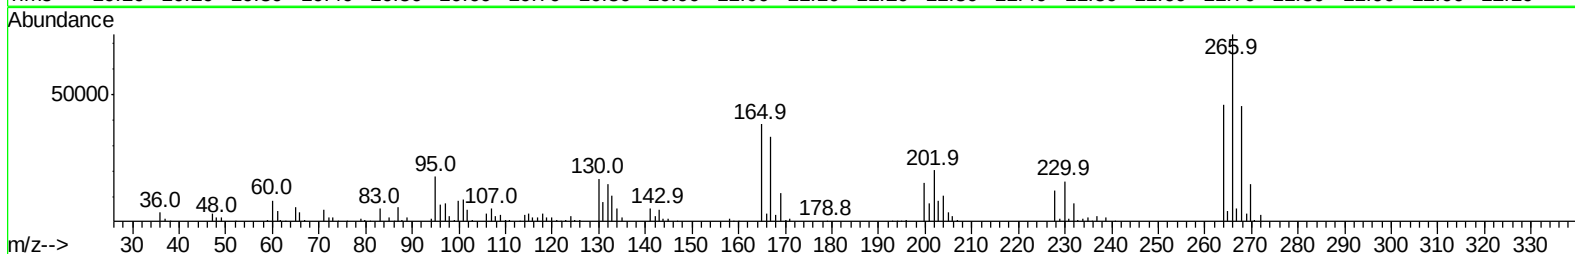


Data Path : Z:\HPCHEM1\BNA F\Data\BF033117\
Data File : BF094086.D
Acq On : 31 Mar 2017 10:15
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 18:11:26 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 14:38:29 2017
Response via : Initial Calibration

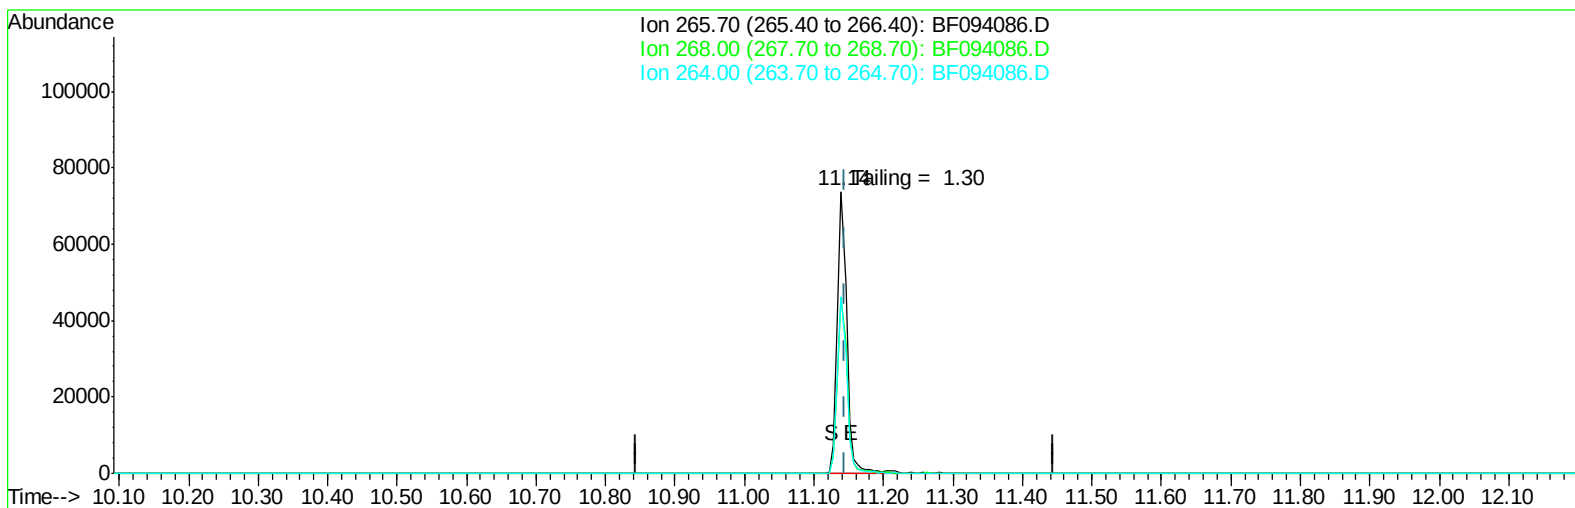

TIC: BF094086.D

(69) Pentachlorophenol (C)




11.139min (-0.006) 0.00ng

response 68732

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.07
264.00	64.60	62.60
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF033117\
Data File : BF094086.D
Acq On : 31 Mar 2017 10:15
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 18:11:26 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 14:38:29 2017
Response via : Initial Calibration

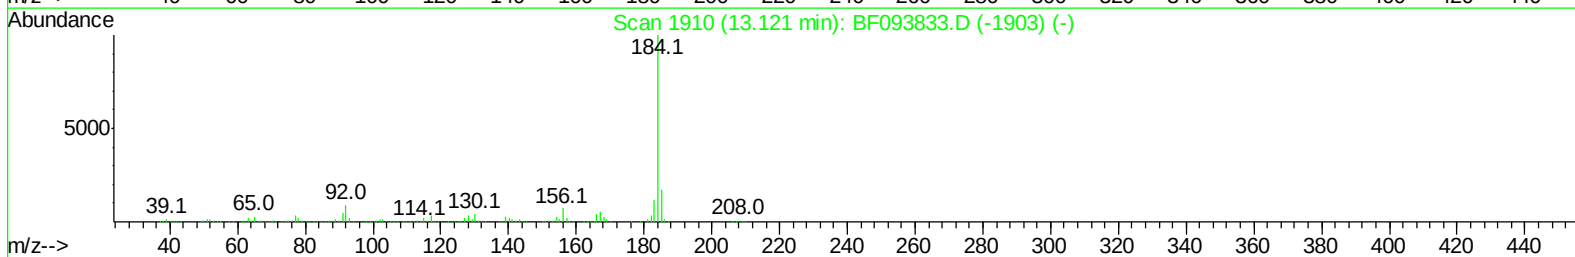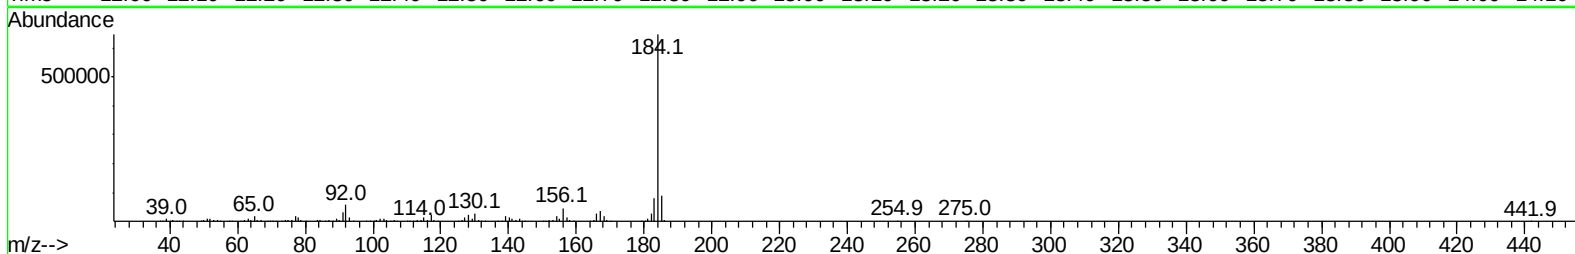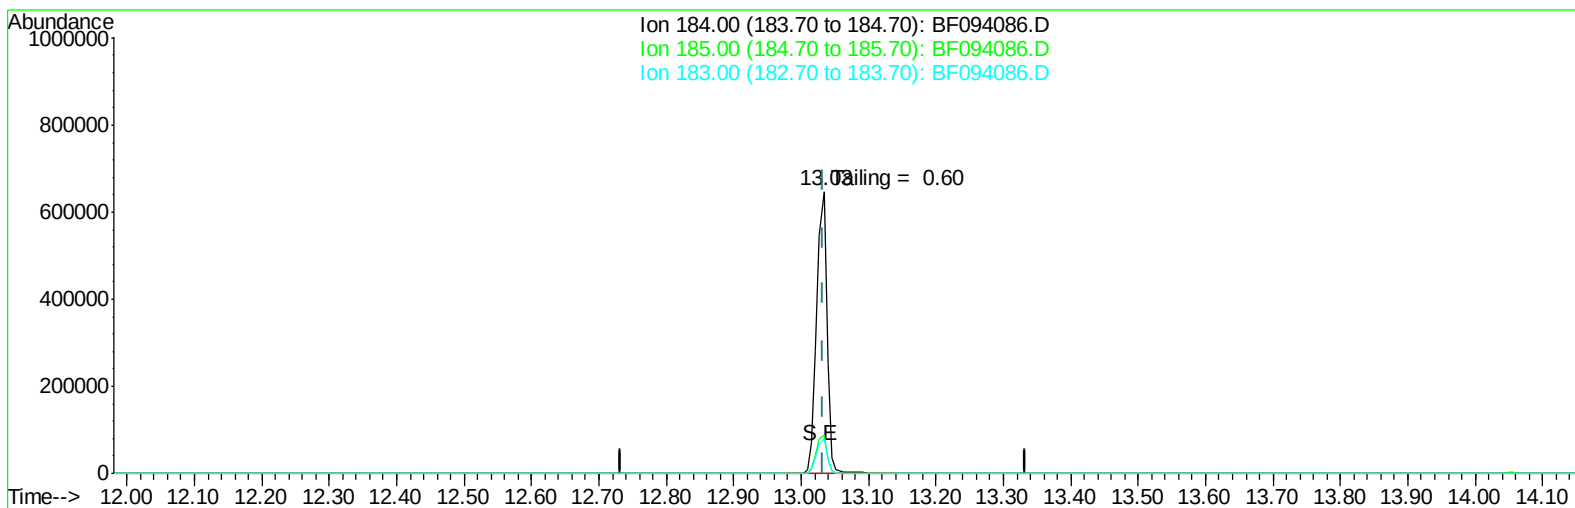

TIC: BF094086.D

(76) Benzidine

13.033min (-0.000) 0.00ng

response 665775

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.81#
183.00	12.20	12.10
0.00	0.00	0.00