
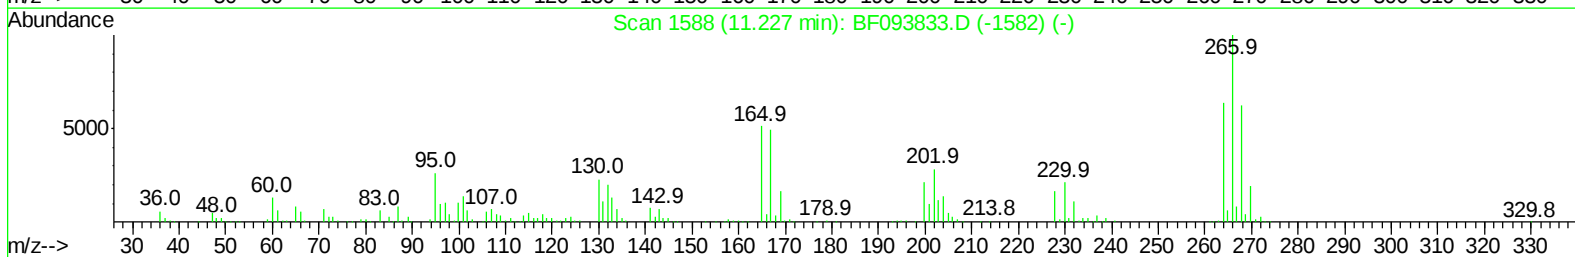
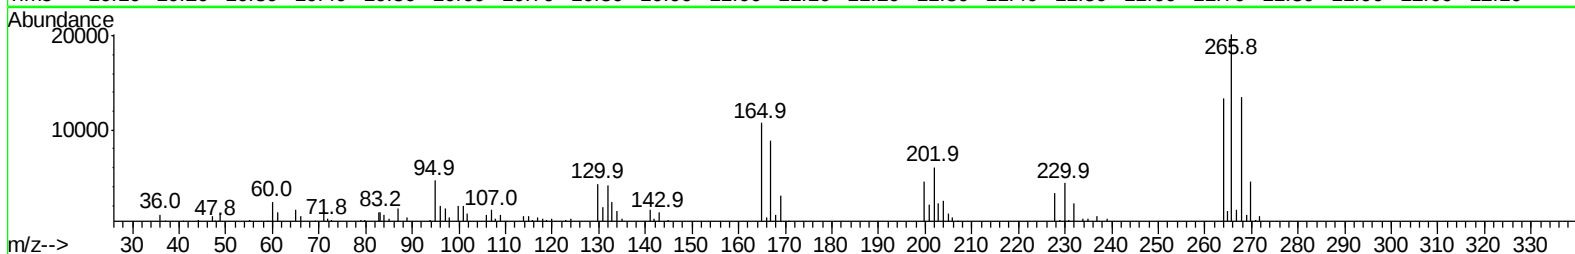


Data Path : Z:\HPCHEM1\BNA F\DATA\BF033117\
Data File : BF094111.D
Acq On : 1 Apr 2017 00:27
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 04:50:25 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 14:38:29 2017
Response via : Initial Calibration

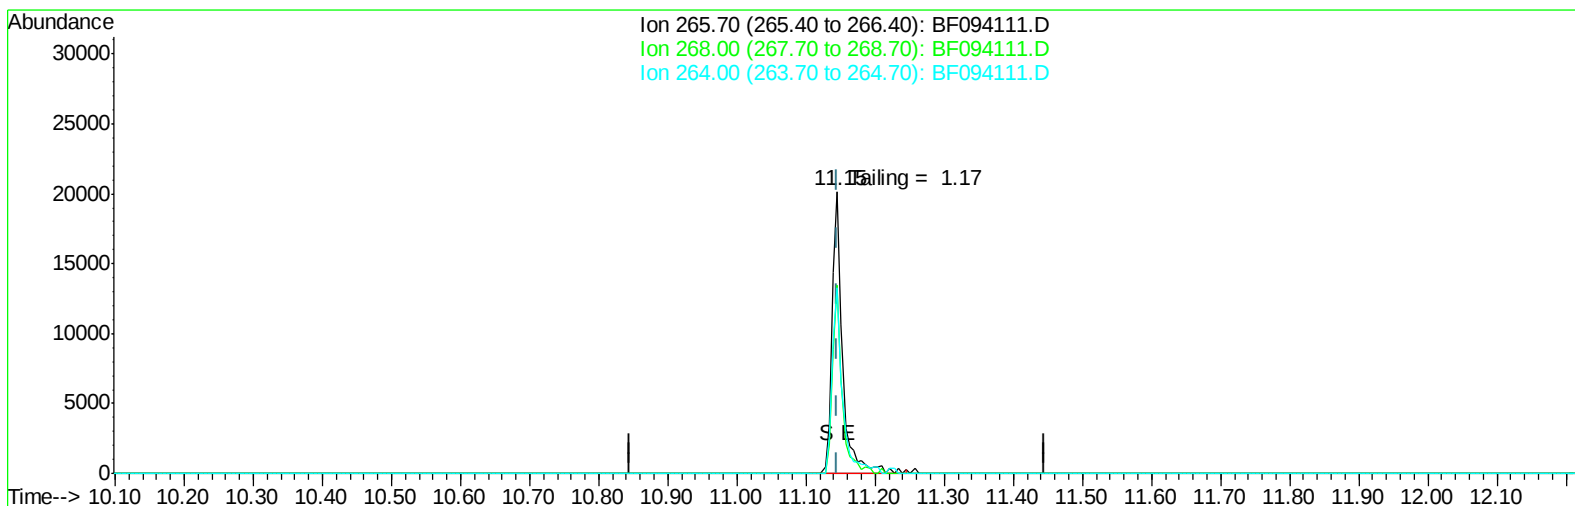

TIC: BF094111.D

(69) Pentachlorophenol (C)




11.145min (-0.000) 0.00ng

response 21219

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.81
264.00	64.60	66.12
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF033117\
Data File : BF094111.D
Acq On : 1 Apr 2017 00:27
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 04:50:25 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 14:38:29 2017
Response via : Initial Calibration

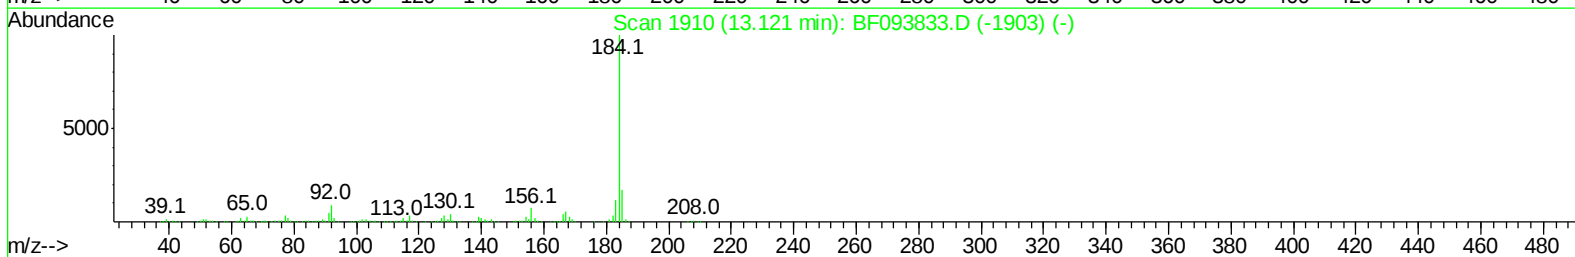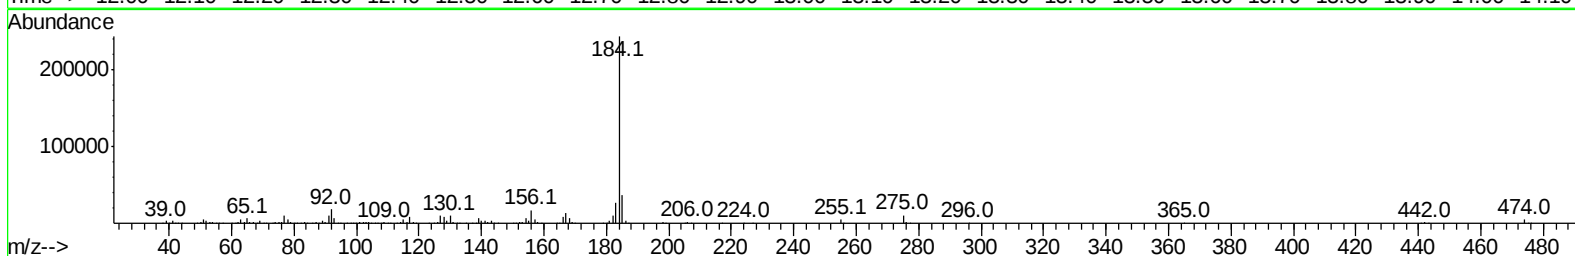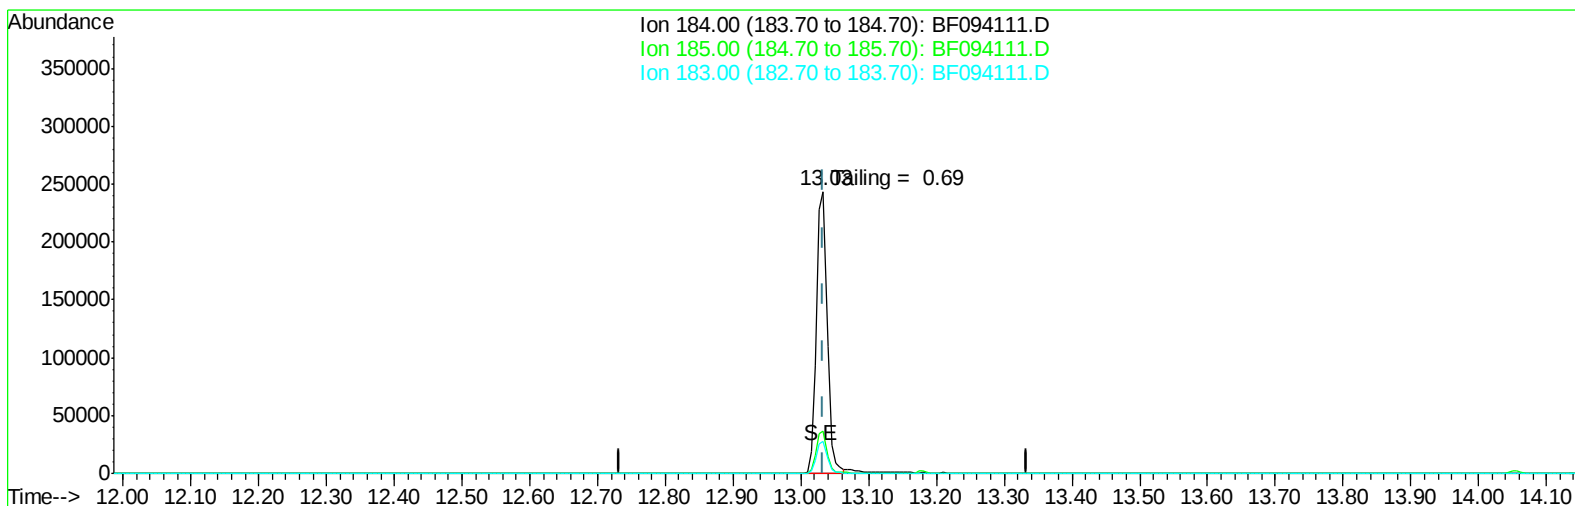

TIC: BF094111.D

(76) Benzidine

13.033min (-0.000) 0.00ng

response 267578

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	15.10#
183.00	12.20	11.31
0.00	0.00	0.00