


Data Path : Z:\HPCHEM1\BNA F\Data\BF033117\
 Data File : BF094086.D
 Acq On : 31 Mar 2017 10:15
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 31 14:38:29 2017

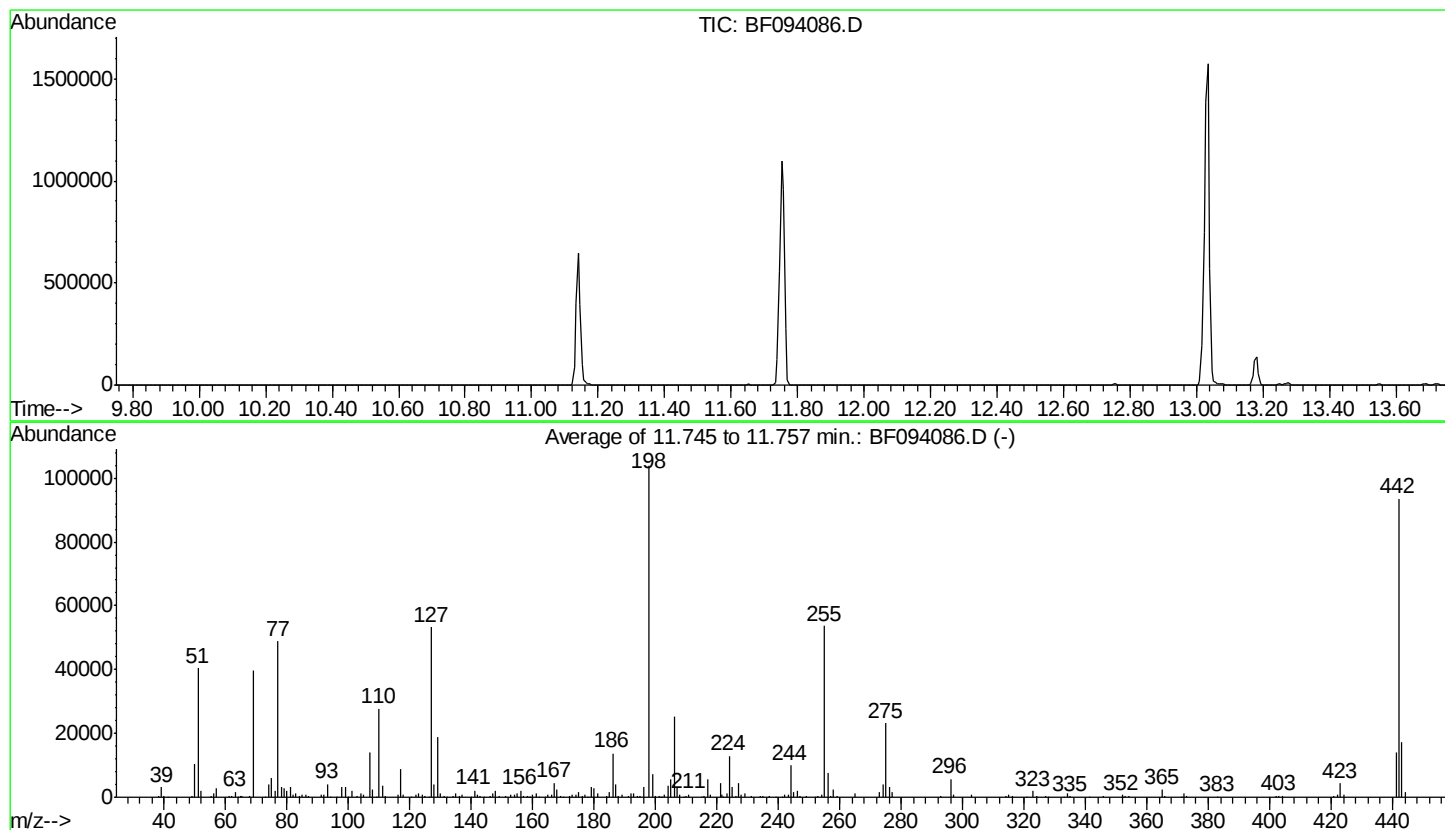

AutoFind: Scans 1676, 1677, 1678; Background Corrected with Scan 1670

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	40480	PASS
68	69	0.00	2	1.5	584	PASS
69	198	0.00	100	38.1	39632	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.3	53293	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	103901	PASS
199	198	5	9	6.8	7089	PASS
275	198	10	60	22.4	23226	PASS
365	198	1	100	2.3	2400	PASS
441	442	0.01	24	15.2	14241	PASS
442	198	50	100	90.1	93634	PASS
443	442	15	24	18.3	17114	PASS