


Data Path : Z:\HPCHEM1\BNA F\Data\BF033117\
 Data File : BF094111.D
 Acq On : 1 Apr 2017 00:27
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 31 14:38:29 2017

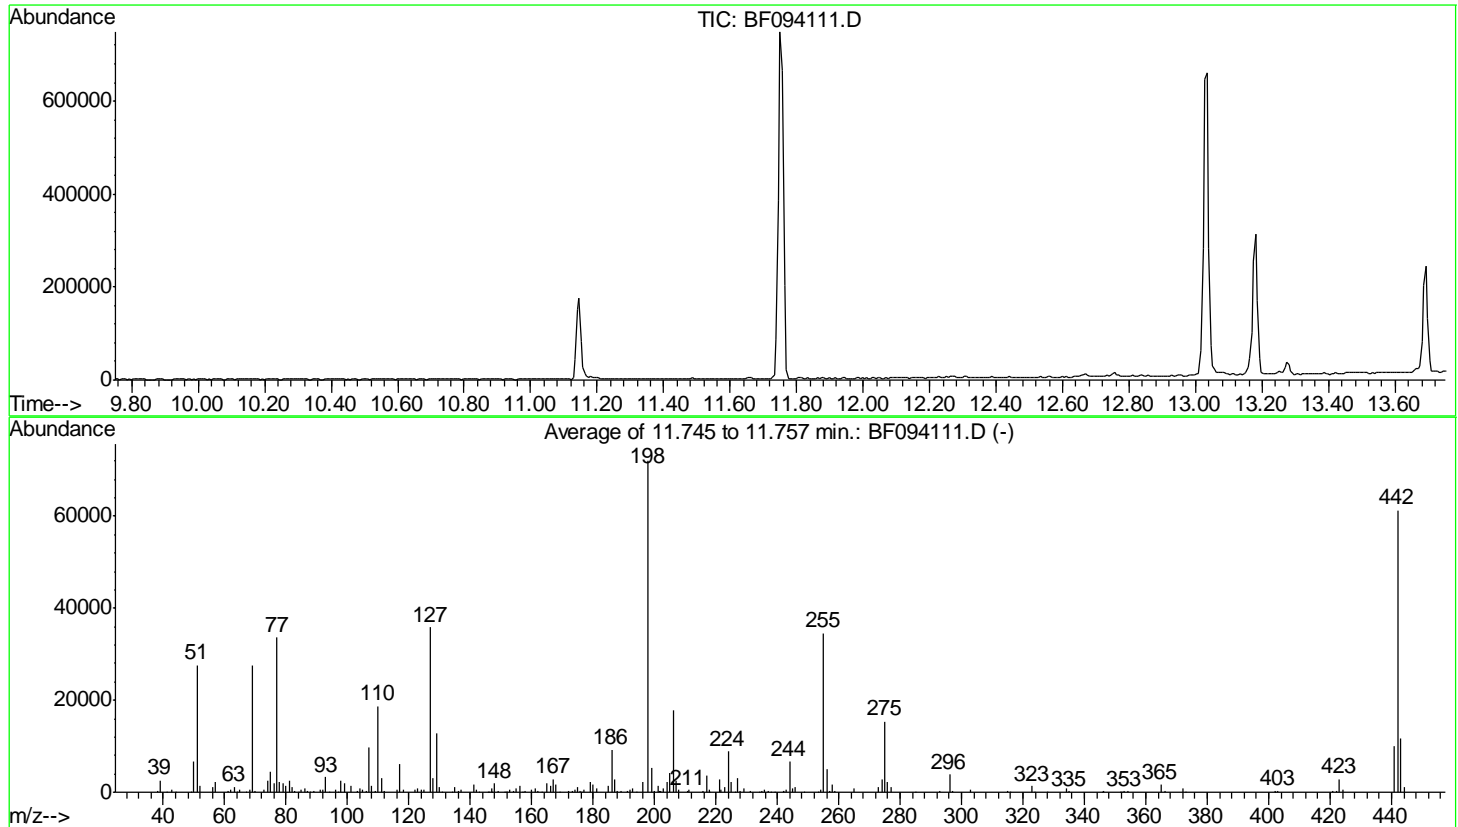

AutoFind: Scans 1676, 1677, 1678; Background Corrected with Scan 1671

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	27648	PASS
68	69	0.00	2	2.0	559	PASS
69	198	0.00	100	38.2	27533	PASS
70	69	0.00	2	0.5	150	PASS
127	198	10	80	49.7	35800	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72082	PASS
199	198	5	9	7.2	5220	PASS
275	198	10	60	21.4	15446	PASS
365	198	1	100	2.3	1663	PASS
441	442	0.01	24	16.4	10049	PASS
442	198	50	100	85.0	61272	PASS
443	442	15	24	19.0	11648	PASS