


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033125\
Data File : BF142174.D
Acq On : 31 Mar 2025 11:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

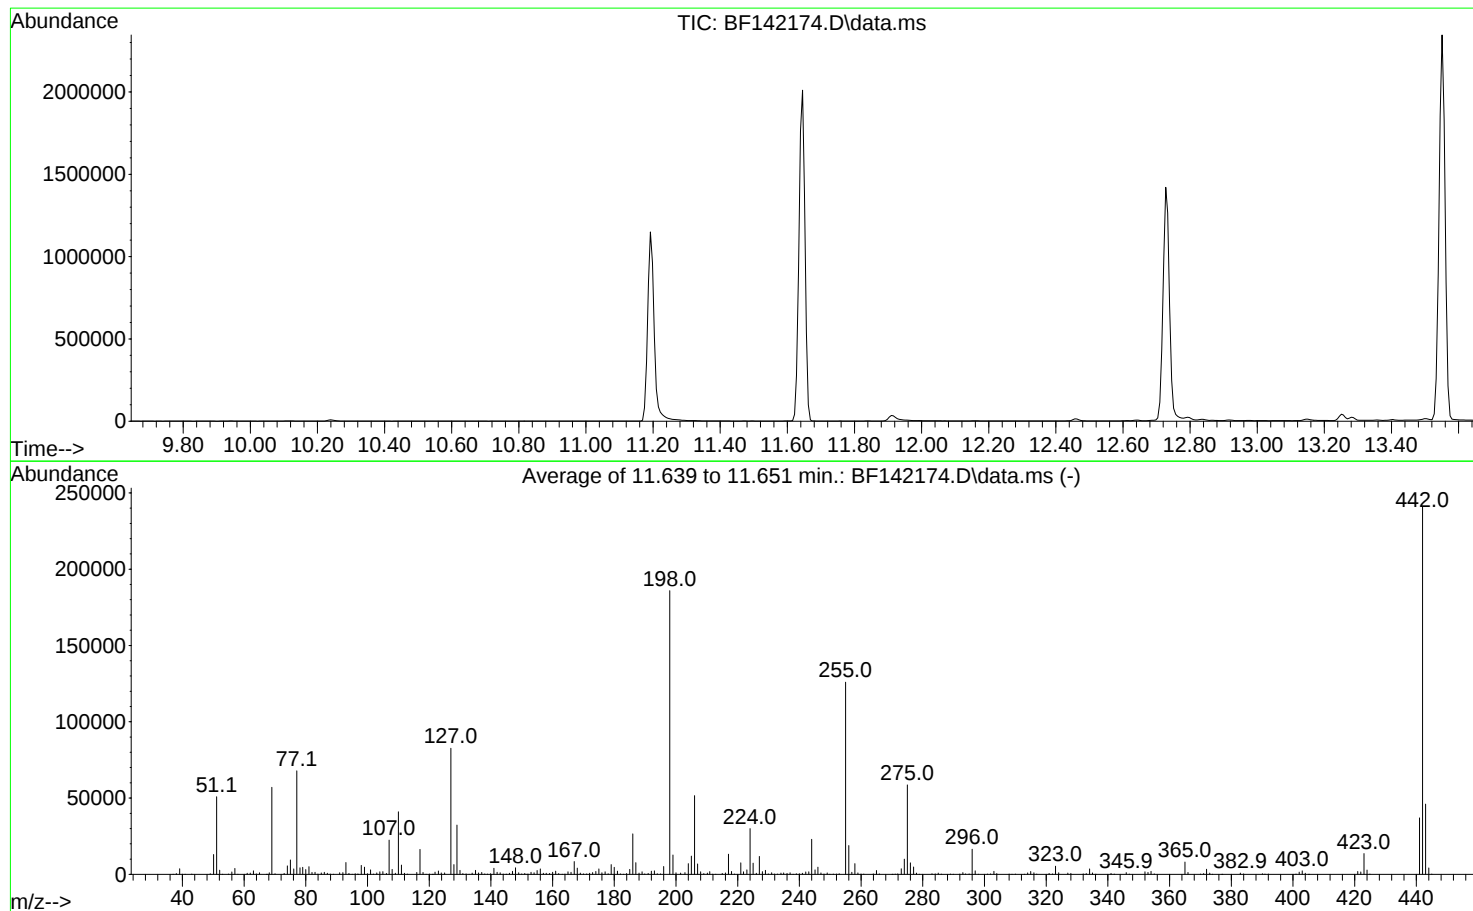

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	50853	PASS
68	69	0.00	2	1.8	1026	PASS
69	198	0.00	100	30.7	57003	PASS
70	69	0.00	2	0.7	402	PASS
127	198	10	80	44.4	82605	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	185877	PASS
199	198	5	9	6.8	12724	PASS
275	198	10	60	31.5	58629	PASS
365	198	1	100	4.3	8063	PASS
441	198	0.01	100	19.9	36995	PASS
442	442	50	100	100.0	241088	PASS
443	442	15	24	19.1	46021	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/31/2025	BNA_F	<u>BF142174.D</u>
Compound Name	Response	Retention Time
DDT	776493	13.557
DDD	16504	13.251
DDE	1369	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17873	794366	2.25

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033125\
Data File : BF142174.D
Acq On : 31 Mar 2025 11:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 31 13:27:35 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

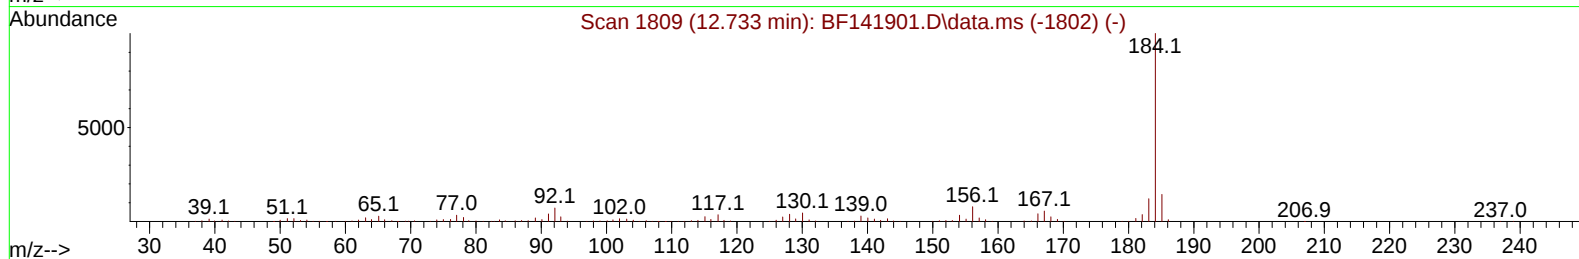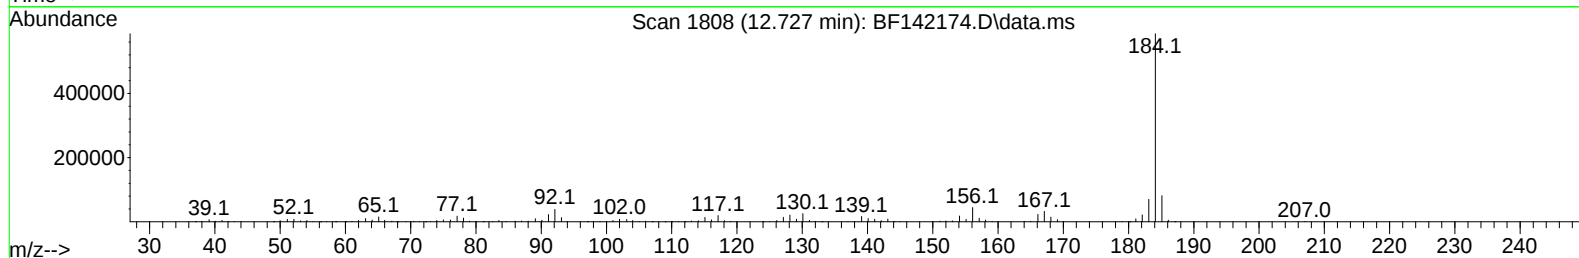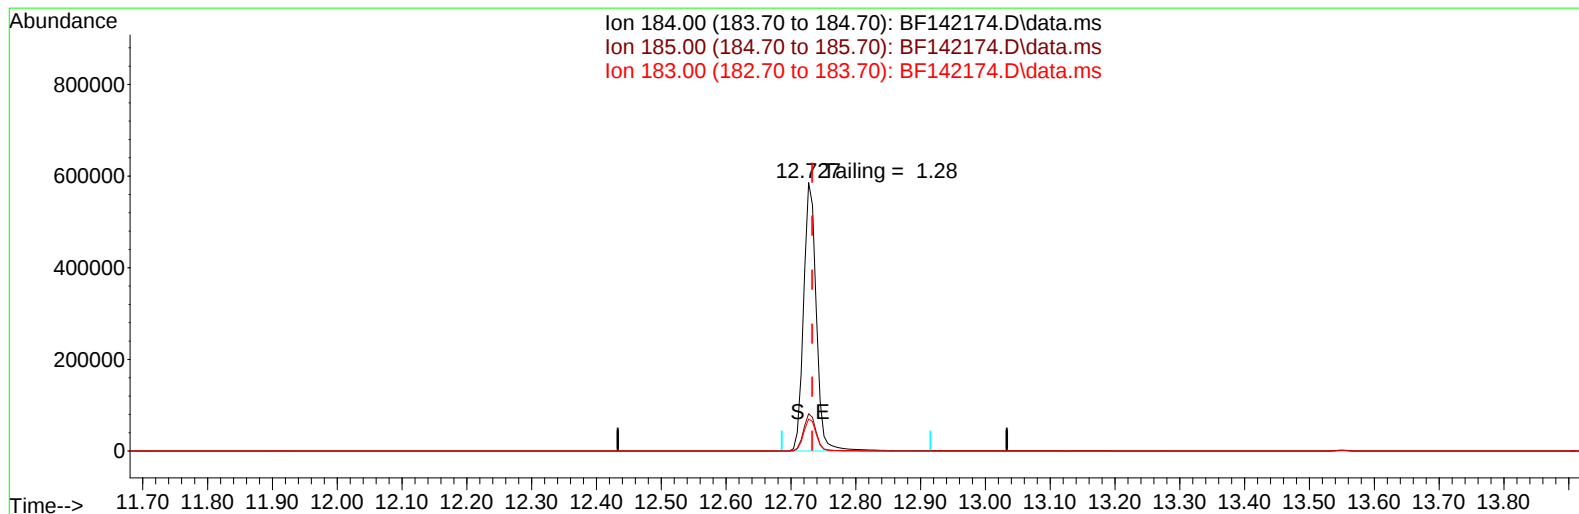

TIC: BF142174.D\data.ms

(77) Benzidine

12.727min (-0.006) 153700.47 ng

response 802010

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.89
183.00	12.10	11.96
0.00	0.00	0.00