

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040115\
 Data File : BF078168.D
 Acq On : 1 Apr 2015 22:55
 Operator : TP/IZ
 Sample : PB82441BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB82441BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.196	24	27	29	rBV	256366	289812	20.74%	3.022%
2	1.298	32	36	39	rVB	22231	50028	3.58%	0.522%
3	1.710	70	72	82	rVB	14951	27433	1.96%	0.286%
4	4.739	336	337	344	rBV	63420	98048	7.02%	1.022%
5	5.299	383	386	396	rBV	776316	863109	61.75%	8.999%
6	6.602	498	500	503	rBV	900498	834678	59.72%	8.702%
7	6.728	509	511	514	rBV	884498	900586	64.44%	9.389%
8	7.013	534	536	539	rBV	218258	230612	16.50%	2.404%
9	7.208	550	553	555	rBV	517331	722623	51.70%	7.534%
10	7.710	595	597	600	rBV	499930	509791	36.47%	5.315%
11	8.591	672	674	677	rBV	337536	314518	22.50%	3.279%
12	9.939	790	792	795	rBV	1217427	1166307	83.45%	12.160%
13	10.762	861	864	866	rBV	343070	364125	26.05%	3.796%
14	11.734	947	949	952	rBV	597275	608617	43.55%	6.345%
15	12.591	1022	1024	1027	rBV	427678	395785	28.32%	4.126%
16	14.591	1196	1199	1201	rBV	1157598	1397656	100.00%	14.572%
17	15.860	1307	1310	1313	rBV	408139	416566	29.80%	4.343%
18	17.540	1455	1457	1460	rBV	298997	401298	28.71%	4.184%


Sum of corrected areas: 9591592

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040115\
Data File : BF078168.D
Acq On : 1 Apr 2015 22:55
Operator : TP/IZ
Sample : PB82441BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB82441BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

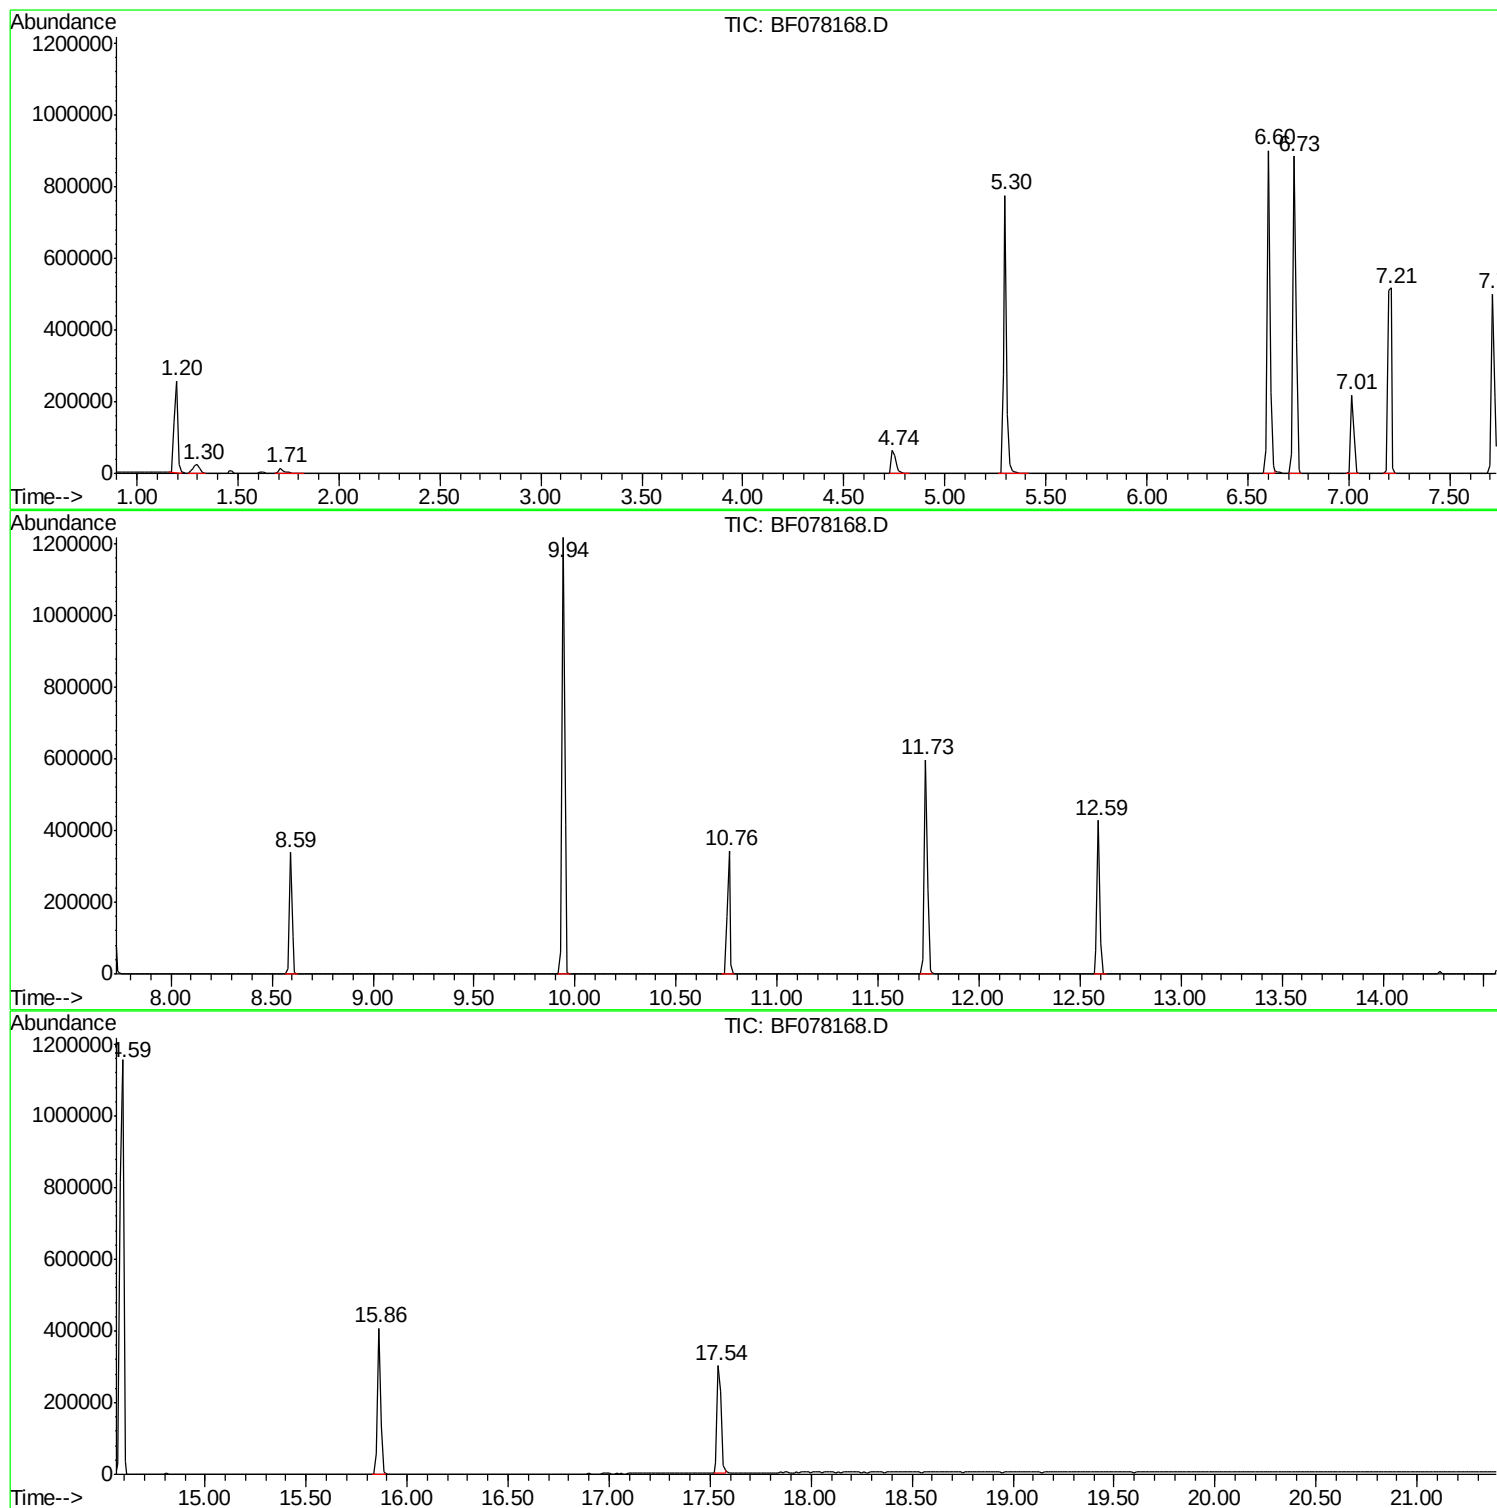

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040115\
Data File : BF078168.D
Acq On : 1 Apr 2015 22:55
Operator : TP/IZ
Sample : PB82441BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleID :
PB82441BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.74	8.50 ng	98048	1,4-Dichlorobenzene-d4	7.01

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59	
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9	
3	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9	
4	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9	
5	Acetone	58	C3H6O	000067-64-1	9	

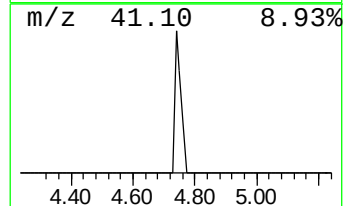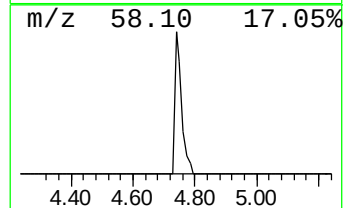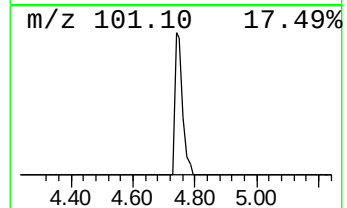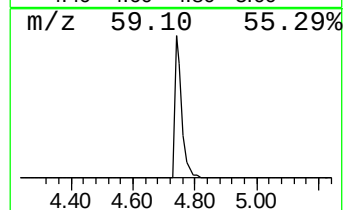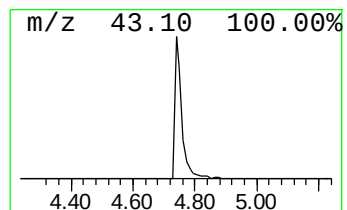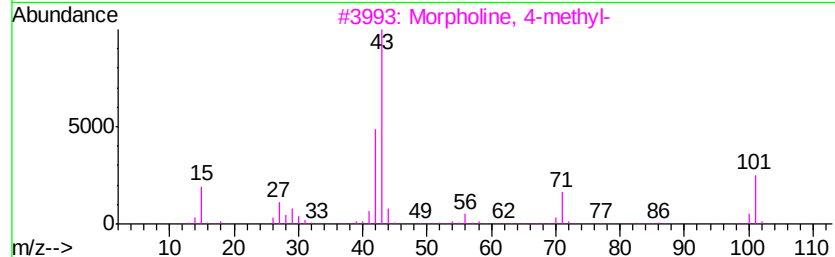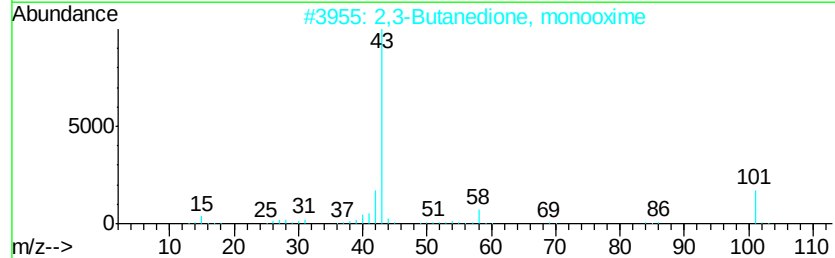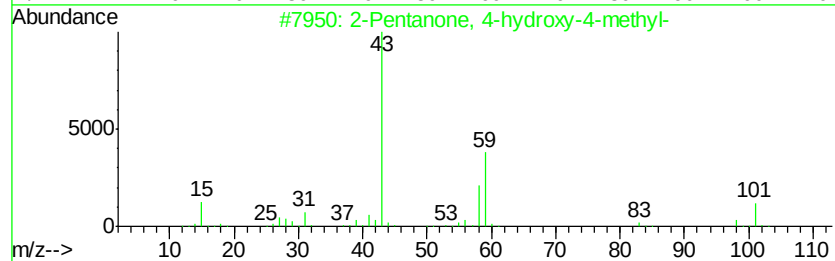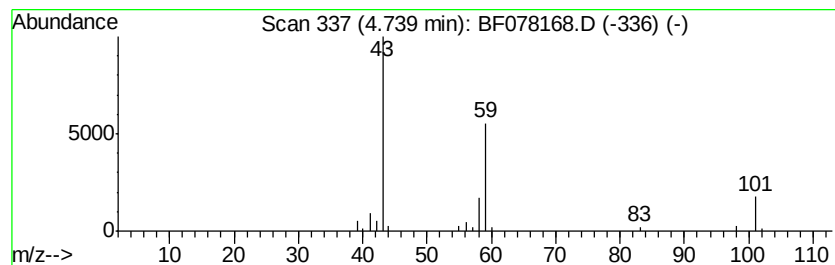

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040115\
Data File : BF078168.D
Acq On : 1 Apr 2015 22:55
Operator : TP/IZ
Sample : PB82441BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB82441BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 unknown6.73 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.73	78.10 ng	900586	1,4-Dichlorobenzene-d4	7.01

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27	
2	5-Aminoindole	132	C8H8N2	005192-03-0	12	
3	Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	10	
4	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9	
5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9	

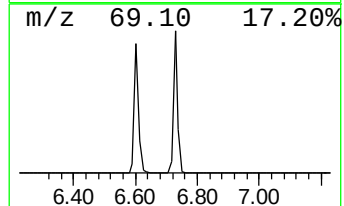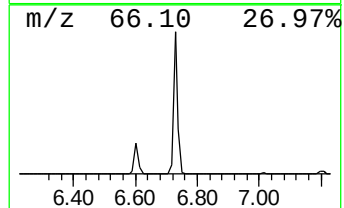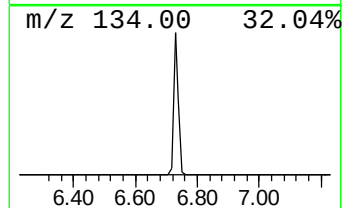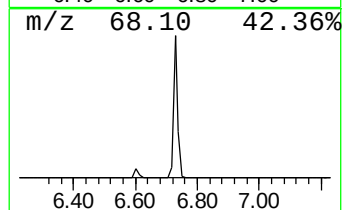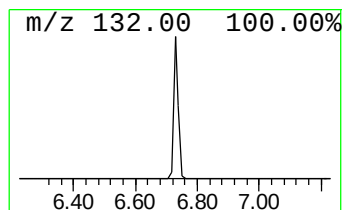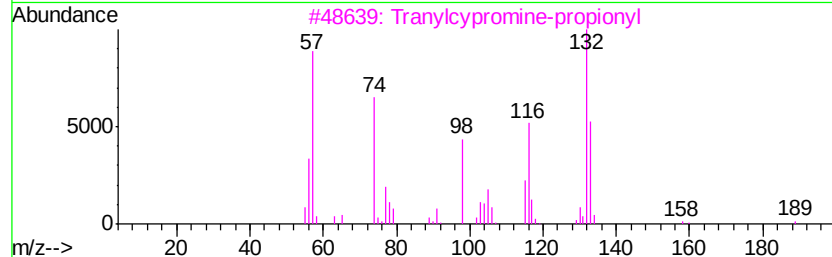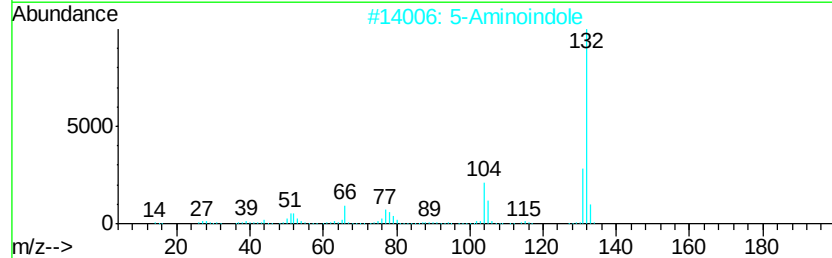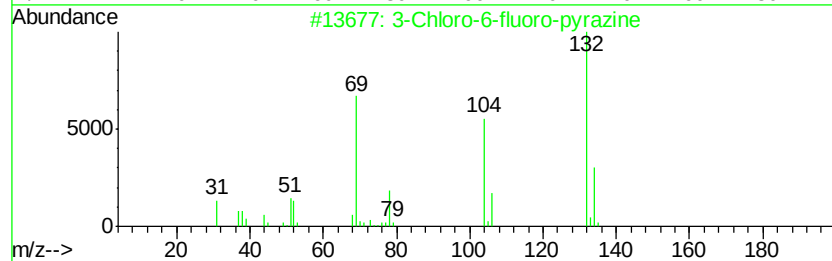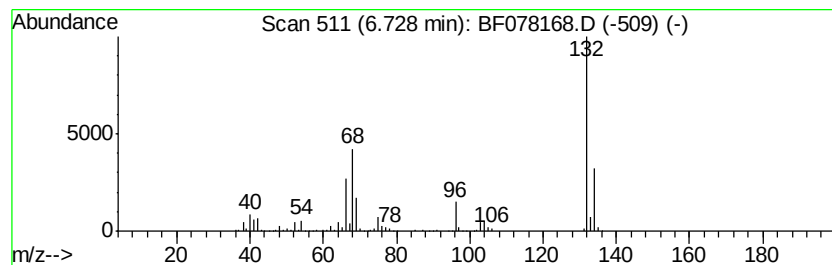

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040115\
Data File : BF078168.D
Acq On : 1 Apr 2015 22:55
Operator : TP/IZ
Sample : PB82441BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB82441BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.74	8.5	ng	98048	1	7.01	230612	20.0
unknown6.73	6.73	78.1	ng	900586	1	7.01	230612	20.0