


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040115\
 Data File : BF078154.D
 Acq On : 1 Apr 2015 15:30
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 02 13:21:29 2015

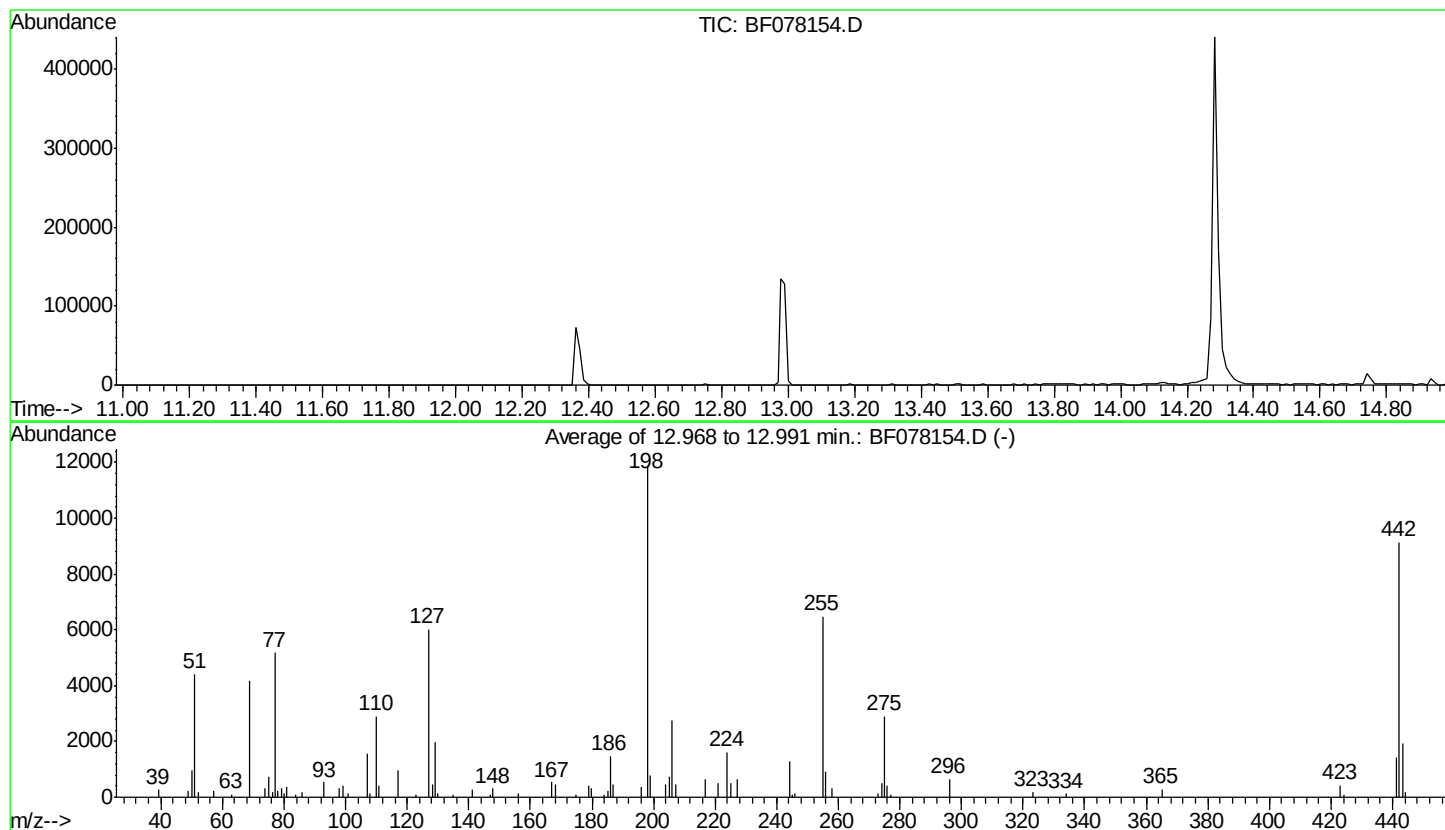

AutoFind: Scans 1057, 1058, 1059; Background Corrected with Scan 1054

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	4408	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.3	4191	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.6	6011	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11881	PASS
199	198	5	9	6.6	784	PASS
275	198	10	60	24.5	2907	PASS
365	198	1	100	2.4	288	PASS
441	442	0.01	24	15.8	1446	PASS
442	198	50	100	76.9	9138	PASS
443	442	15	24	20.9	1909	PASS