
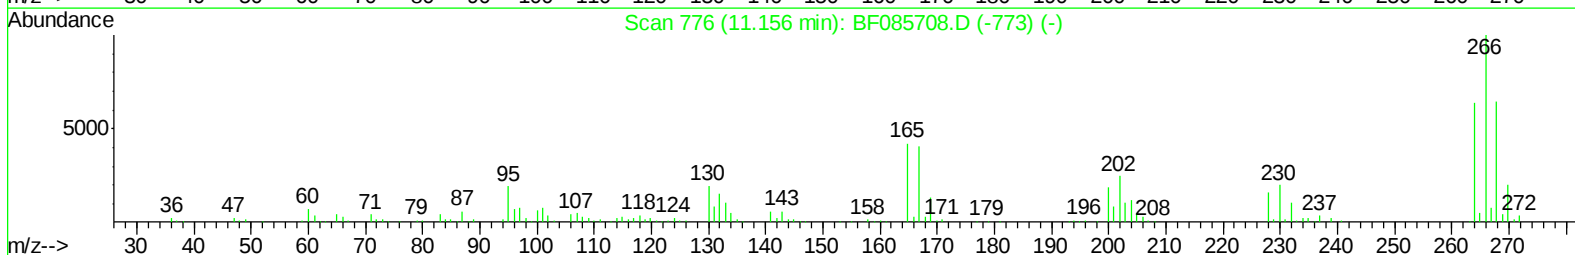
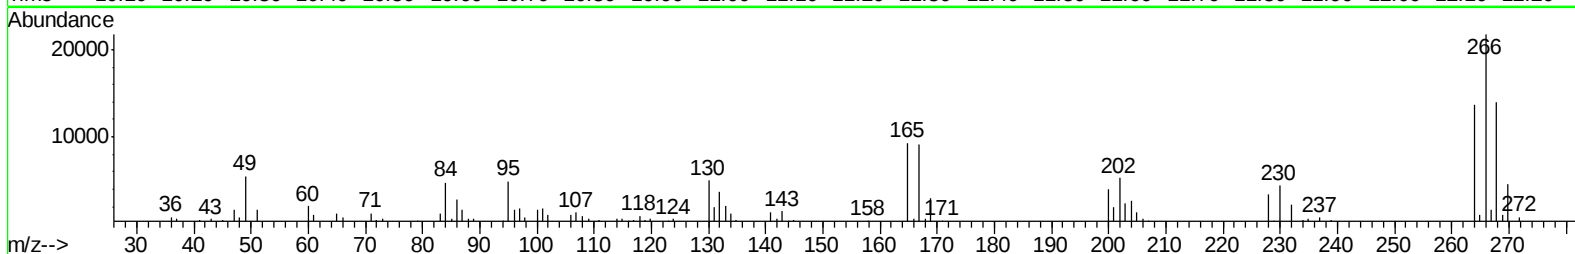


Data Path : Z:\HPCHEM1\BNA F\DATA\BF040116\
Data File : BF085958.D
Acq On : 1 Apr 2016 10:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 12:04:04 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 30 12:31:18 2016
Response via : Initial Calibration

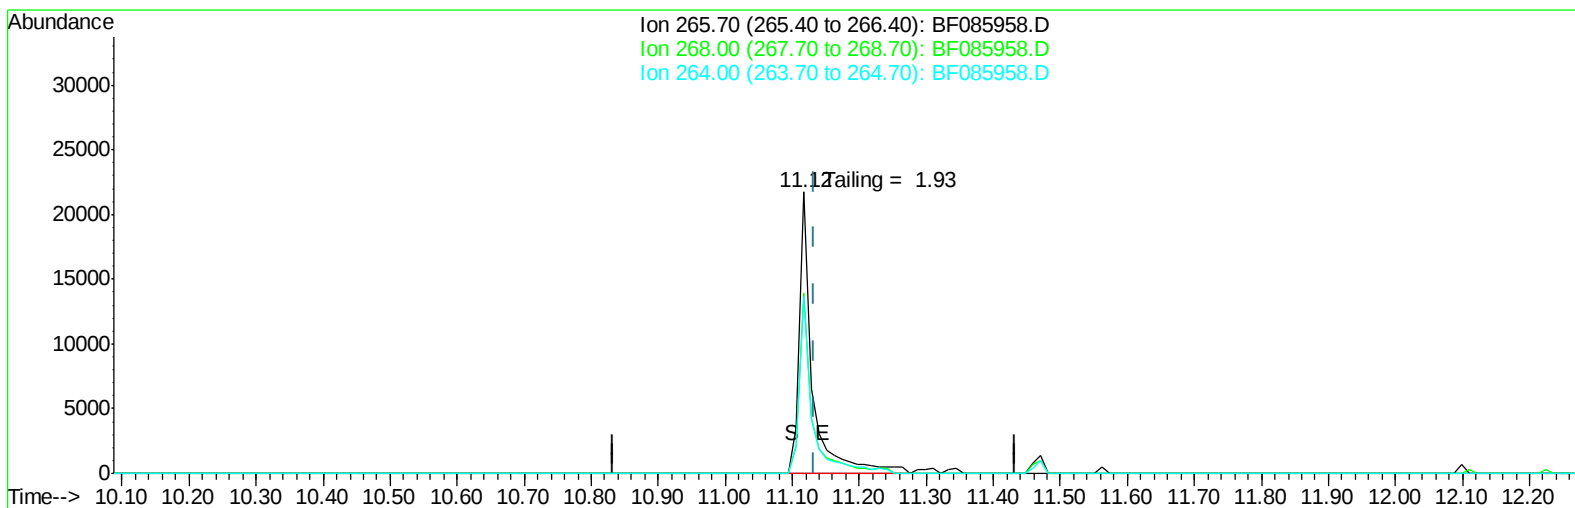

TIC: BF085958.D

(69) Pentachlorophenol (C)




11.116min (-0.017) 23481.25ng

response 30218

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.27
264.00	63.30	62.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040116\
Data File : BF085958.D
Acq On : 1 Apr 2016 10:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 12:04:04 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 30 12:31:18 2016
Response via : Initial Calibration

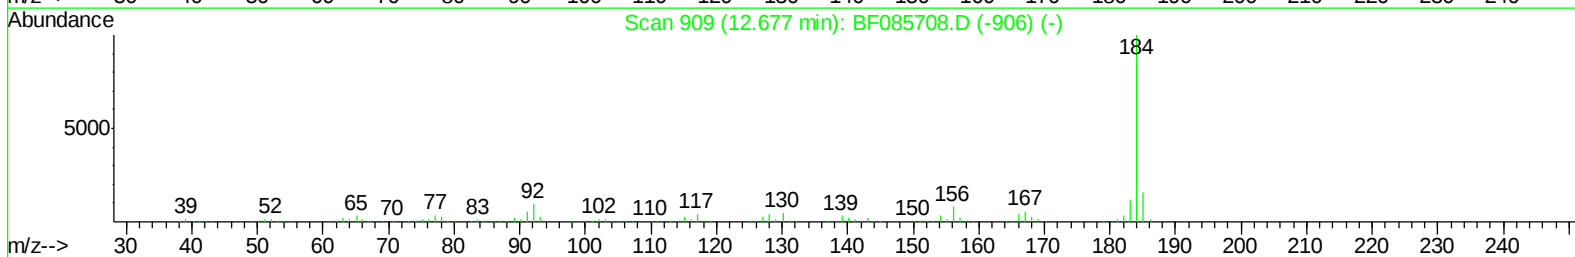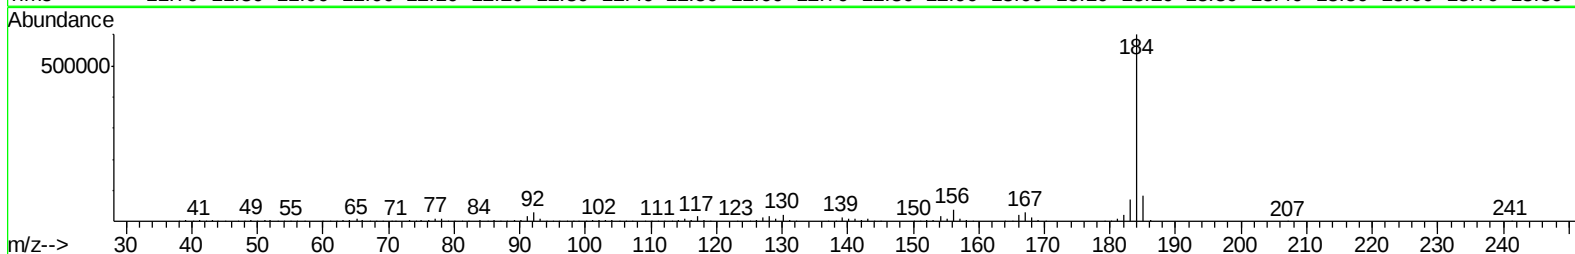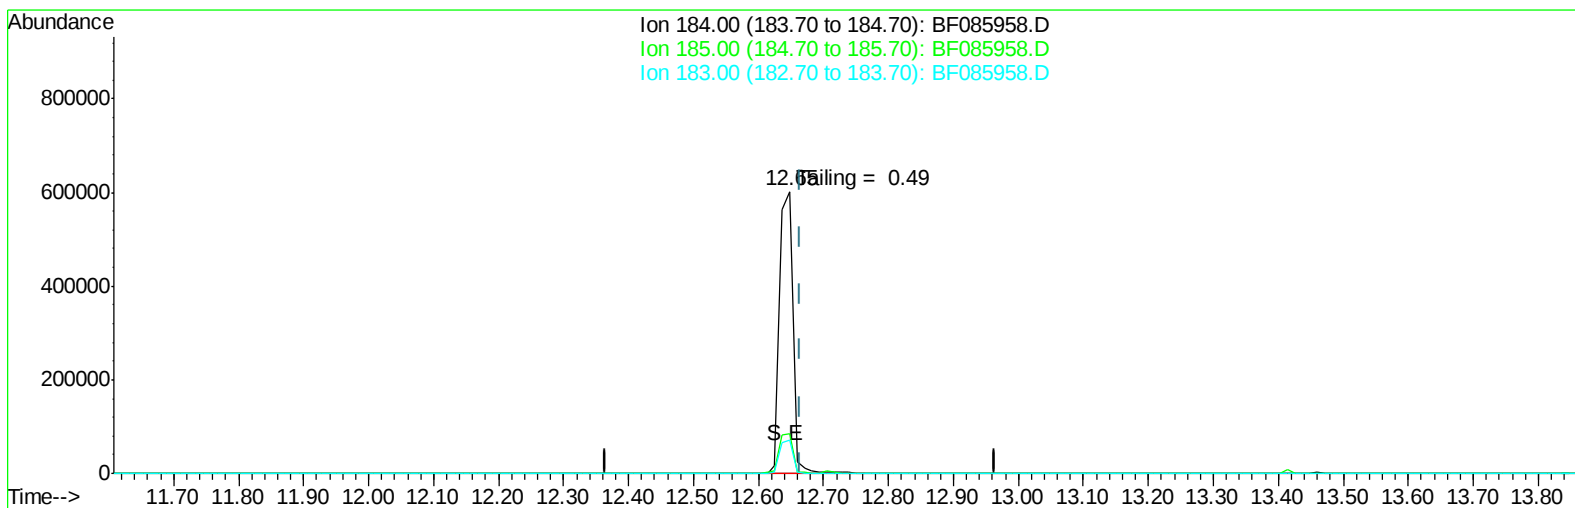

TIC: BF085958.D

(76) Benzidine

12.648min (-0.017) 52418.55ng

response 851033

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.04
183.00	11.80	11.73
0.00	0.00	0.00