


Data Path : Z:\HPCHEM1\BNA F\DATA\BF040116\
 Data File : BF085958.D
 Acq On : 1 Apr 2016 10:11
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 30 12:31:18 2016

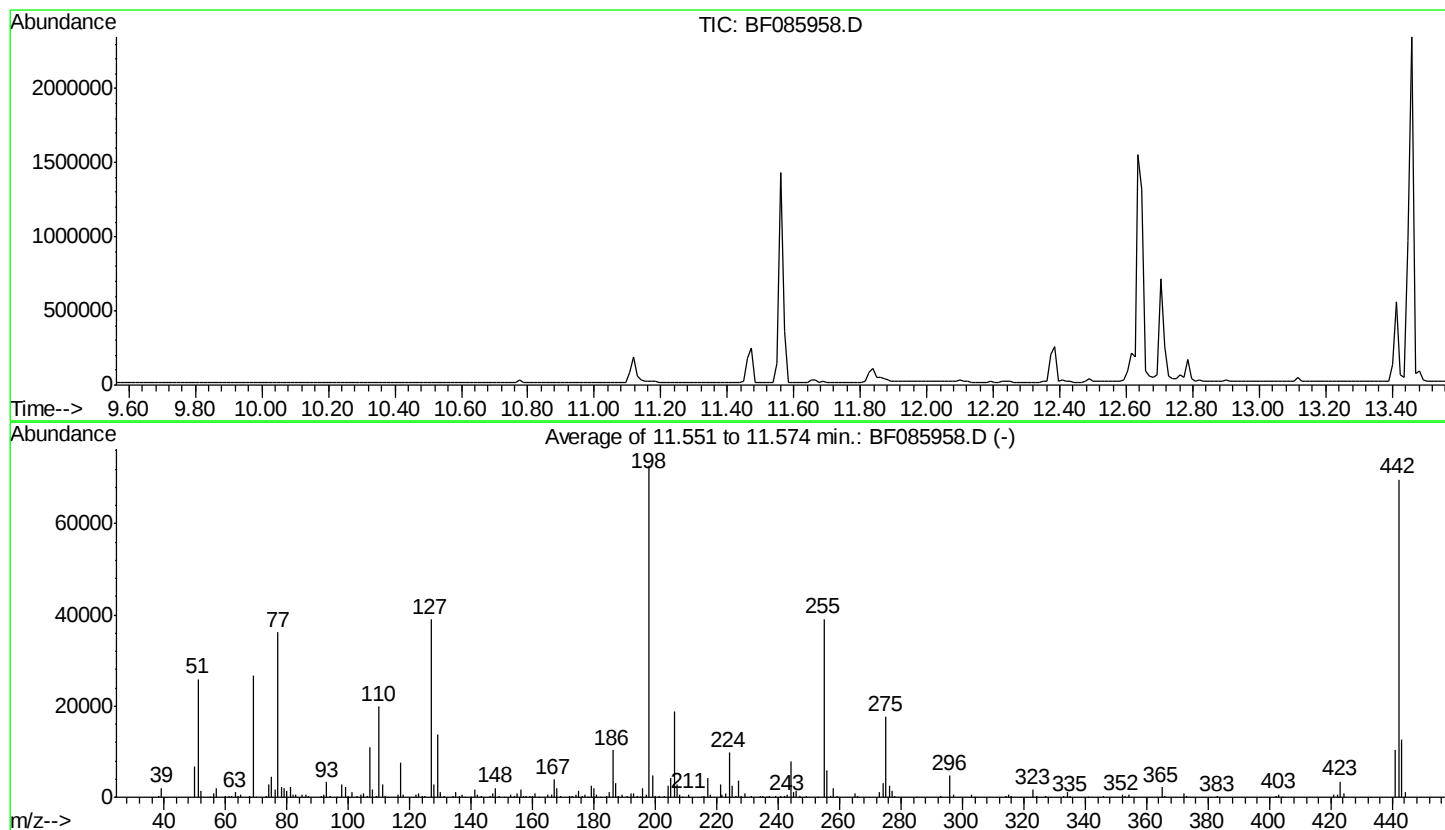

AutoFind: Scans 828, 829, 830; Background Corrected with Scan 825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	25933	PASS
68	69	0.00	2	1.4	368	PASS
69	198	0.00	100	36.8	26789	PASS
70	69	0.00	2	0.5	147	PASS
127	198	10	80	53.6	38992	PASS
197	198	0.00	2	0.6	451	PASS
198	198	100	100	100.0	72753	PASS
199	198	5	9	6.6	4791	PASS
275	198	10	60	24.3	17653	PASS
365	198	1	100	2.9	2131	PASS
441	442	0.01	24	15.1	10503	PASS
442	198	50	100	95.9	69785	PASS
443	442	15	24	18.2	12698	PASS