
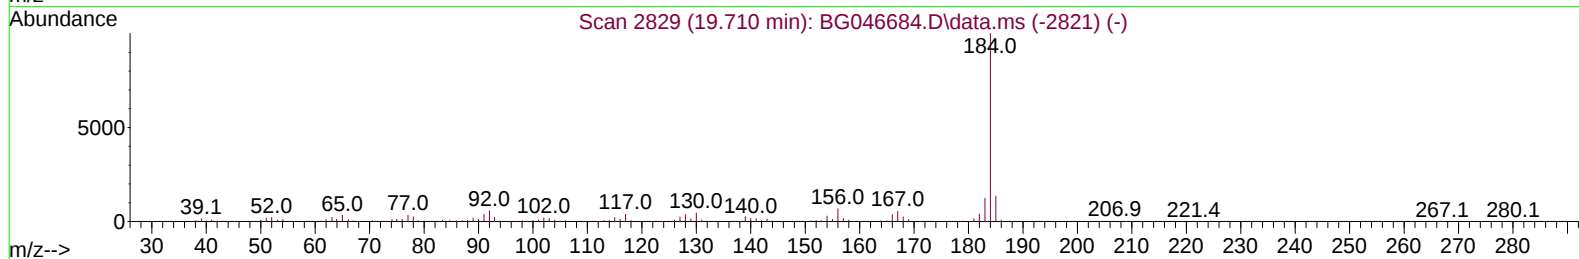
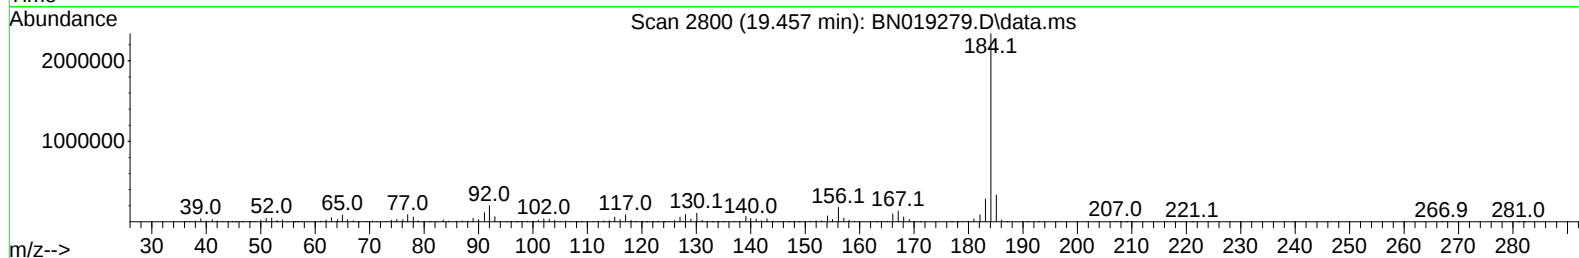


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033122\
Data File : BN019279.D
Acq On : 01 Apr 2022 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 16:37:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

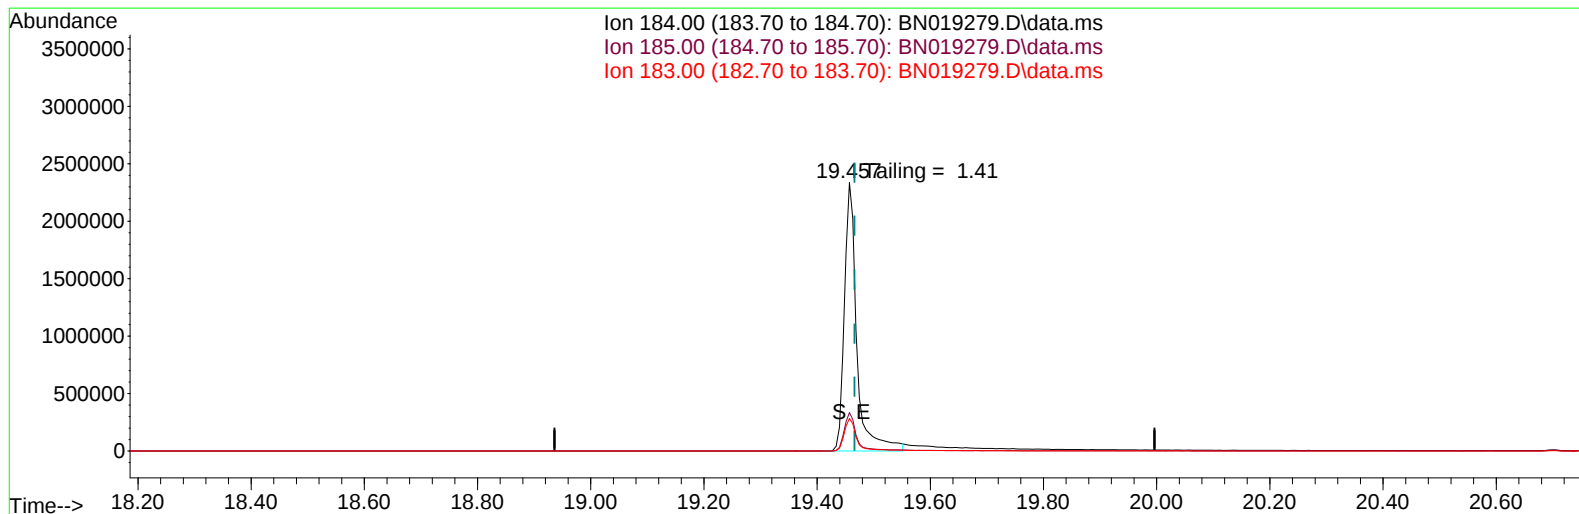

TIC: BN019279.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 3907303

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.31
183.00	13.20	12.09
0.00	0.00	0.00