

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040122\
 Data File : BF127620.D
 Acq On : 01 Apr 2022 19:03
 Operator : CG\JU
 Sample : N2202-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MHF

Quant Time: Apr 01 23:49:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 29 07:13:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.834	152	99721	20.000	ng	0.00
21) Naphthalene-d8	8.116	136	381018	20.000	ng	0.00
39) Acenaphthene-d10	9.869	164	219686	20.000	ng	0.00
64) Phenanthrene-d10	11.363	188	401944	20.000	ng	0.00
76) Chrysene-d12	14.016	240	261169	20.000	ng	0.00
86) Perylene-d12	15.498	264	189816	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.475	112	815241	130.494	ng	0.02
7) Phenol-d6	6.481	99	1040076	121.794	ng	0.00
23) Nitrobenzene-d5	7.404	82	802475	90.028	ng	0.00
42) 2,4,6-Tribromophenol	10.669	330	322280	137.714	ng	0.00
45) 2-Fluorobiphenyl	9.192	172	1331851	88.527	ng	0.00
79) Terphenyl-d14	12.951	244	1560299	97.800	ng	0.00
Target Compounds						
52) Acenaphthene	9.904	154	33481	2.905	ng	99
71) Phenanthrene	11.386	178	47536	2.268	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040122\
Data File : BF127620.D
Acq On : 01 Apr 2022 19:03
Operator : CG\JU
Sample : N2202-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MHF

Quant Time: Apr 01 23:49:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 29 07:13:31 2022
Response via : Initial Calibration




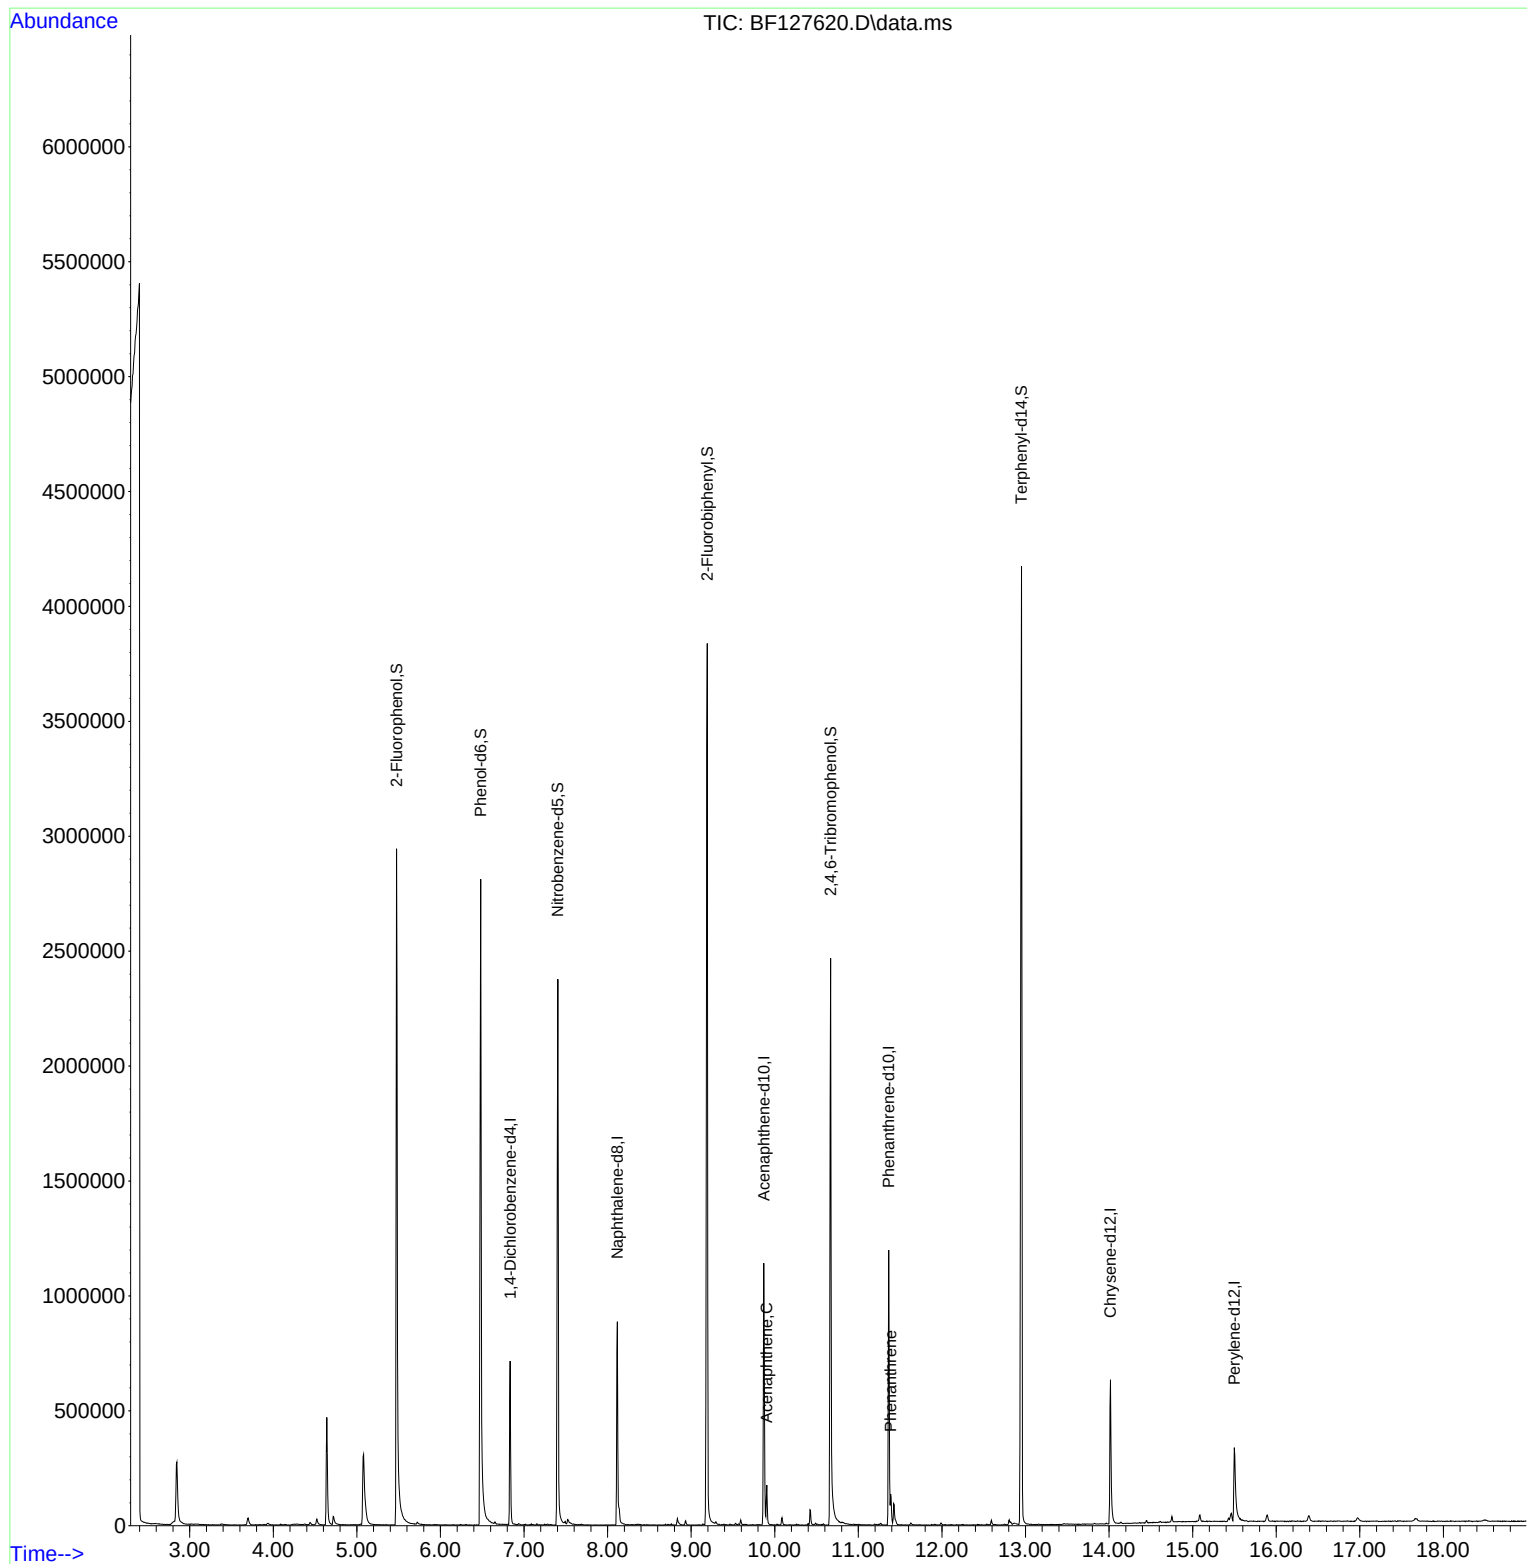


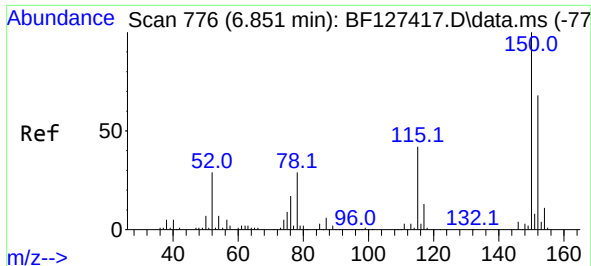

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.834 min Scan# 71
Delta R.T. 0.001 min
Lab File: BF127620.D
Acq: 01 Apr 2022 19:03




Instrument :
BNA_F
ClientSampleId :
MHF


Tgt Ion:152 Resp: 99721
Ion Ratio Lower Upper
152 100
150 145.7 117.2 175.8
115 61.9 49.8 74.6

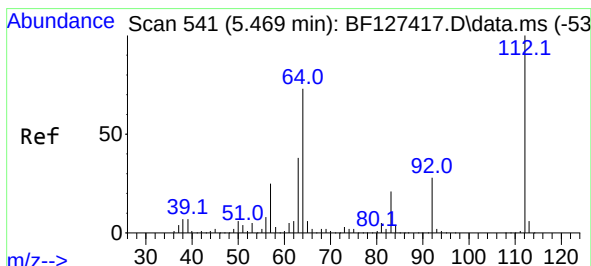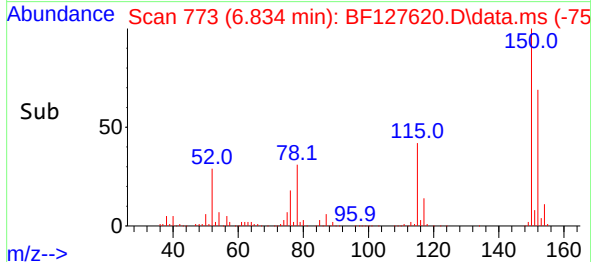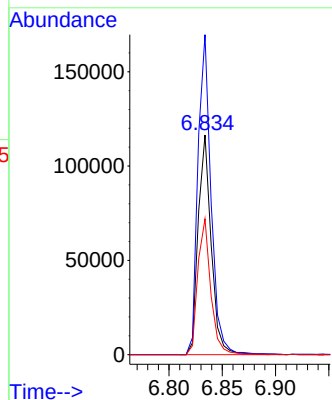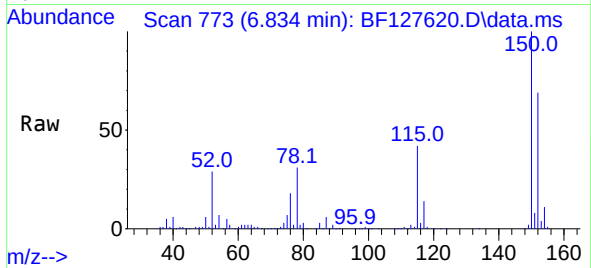

#5
2-Fluorophenol
Concen: 130.494 ng
RT: 5.475 min Scan# 542
Delta R.T. 0.018 min
Lab File: BF127620.D
Acq: 01 Apr 2022 19:03

Tgt Ion:112 Resp: 815241
Ion Ratio Lower Upper
112 100
64 76.4 58.4 87.6
63 39.6 30.1 45.1


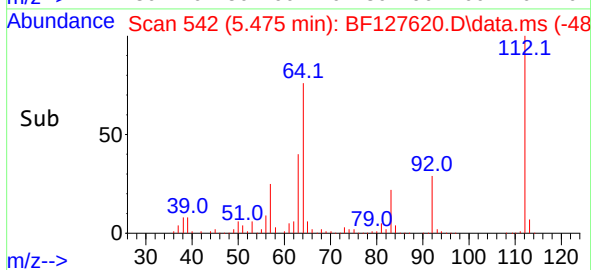
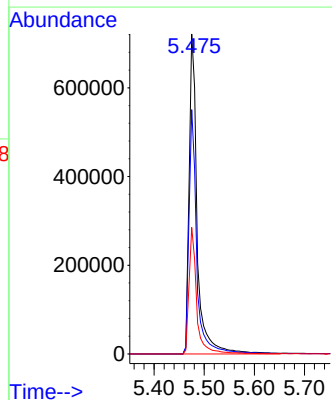
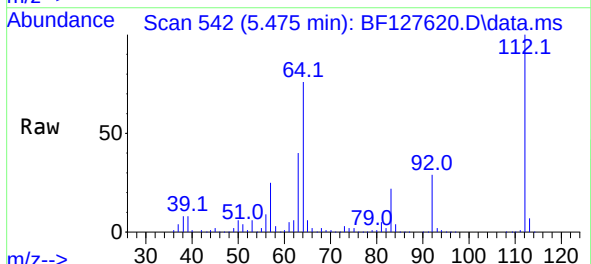


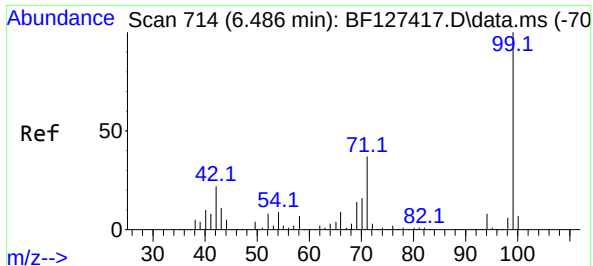

#7
Phenol-d6
Concen: 121.794 ng
RT: 6.481 min Scan# 714
Delta R.T. 0.000 min
Lab File: BF127620.D
Acq: 01 Apr 2022 19:03




Instrument :
BNA_F
ClientSampleId :
MHF


Tgt Ion: 99 Resp: 1040076
Ion Ratio Lower Upper
99 100
42 21.7 17.8 26.6
71 36.7 29.6 44.4

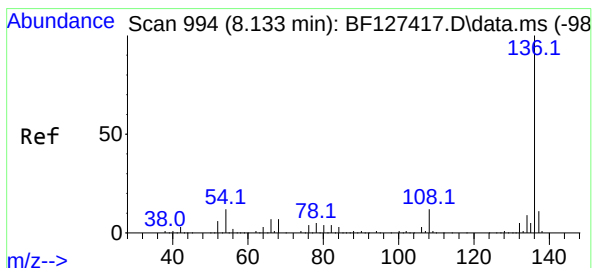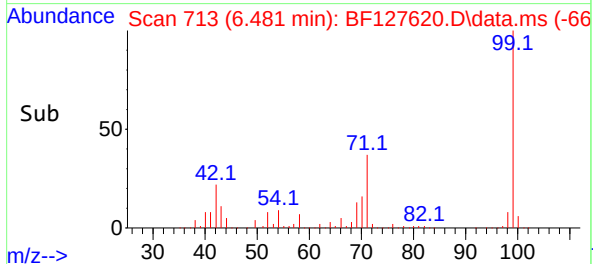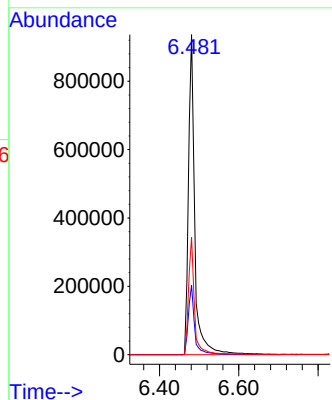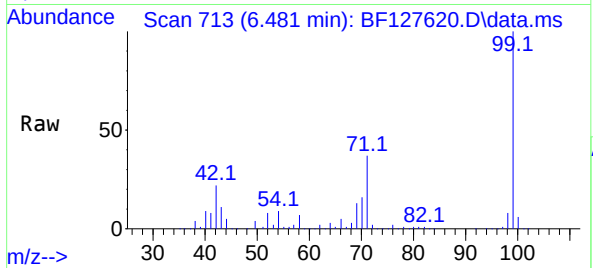

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.116 min Scan# 991
Delta R.T. 0.000 min
Lab File: BF127620.D
Acq: 01 Apr 2022 19:03

Tgt Ion: 136 Resp: 381018
Ion Ratio Lower Upper
136 100
137 10.3 8.6 13.0
54 11.2 9.2 13.8
68 7.1 5.4 8.0


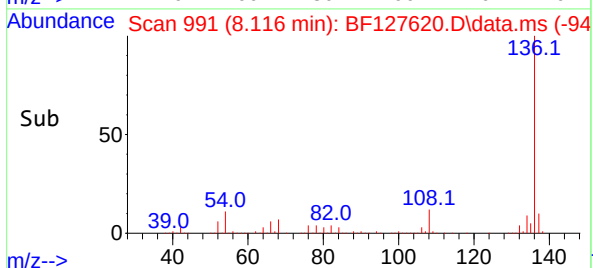
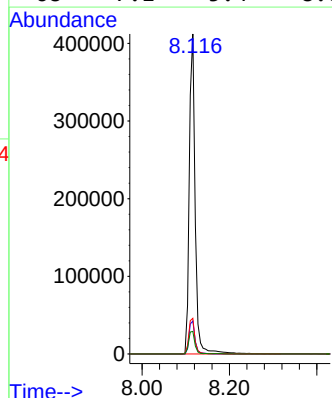
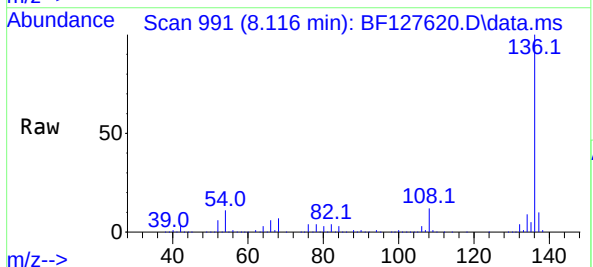


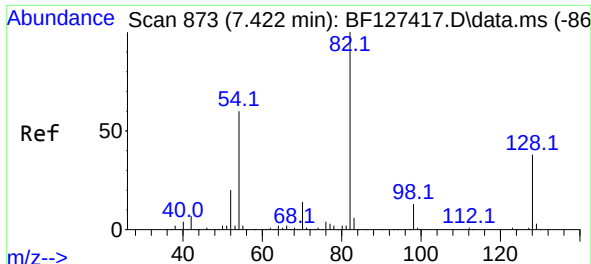

#23
Nitrobenzene-d5
Concen: 90.028 ng
RT: 7.404 min Scan# 81
Delta R.T. -0.006 min
Lab File: BF127620.D
Acq: 01 Apr 2022 19:03




Instrument :
BNA_F
ClientSampleId :
MHF


Tgt Ion: 82 Resp: 802475
Ion Ratio Lower Upper
82 100
128 38.5 30.6 45.8
54 61.3 48.2 72.2

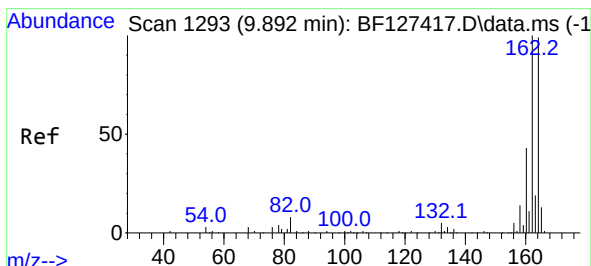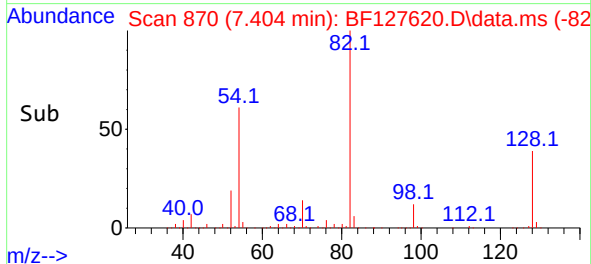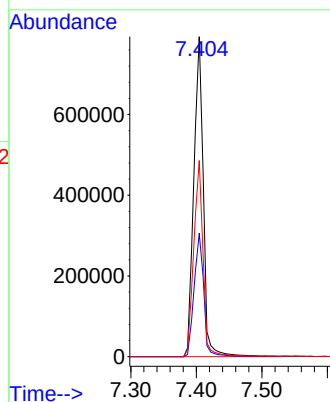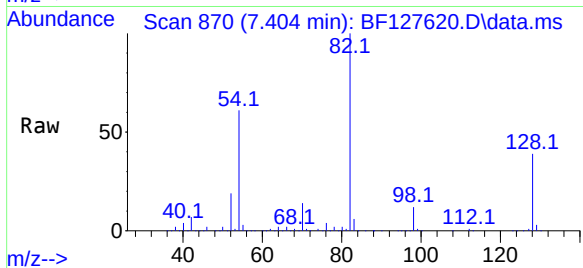

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.869 min Scan# 1289
Delta R.T. -0.006 min
Lab File: BF127620.D
Acq: 01 Apr 2022 19:03

Tgt Ion:164 Resp: 219686
Ion Ratio Lower Upper
164 100
162 104.3 81.2 121.8
160 45.1 34.6 52.0

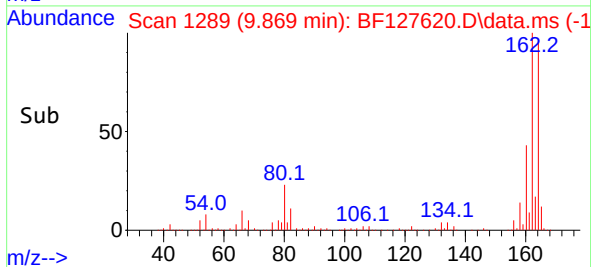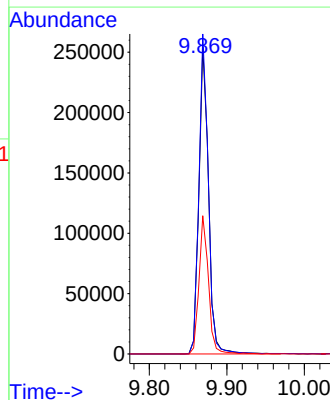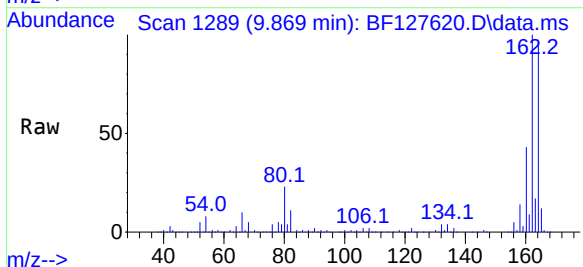

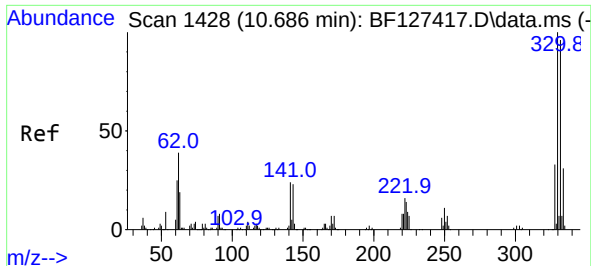

#42

2,4,6-Tribromophenol

Concen: 137.714 ng

RT: 10.669 min Scan# 1425

Delta R.T. 0.000 min

Lab File: BF127620.D

Acq: 01 Apr 2022 19:03

Instrument :

BNA_F

ClientSampleId :

MHF





Tgt Ion:330 Resp: 322280

Ion Ratio Lower Upper

330 100

332 97.1 79.1 118.7

141 32.0 26.2 39.4

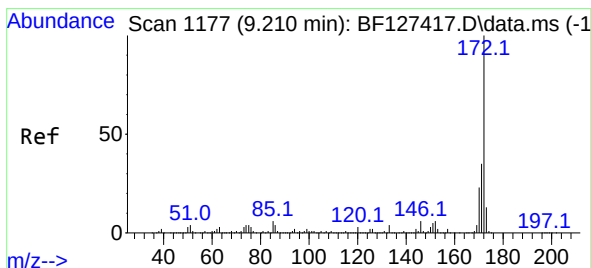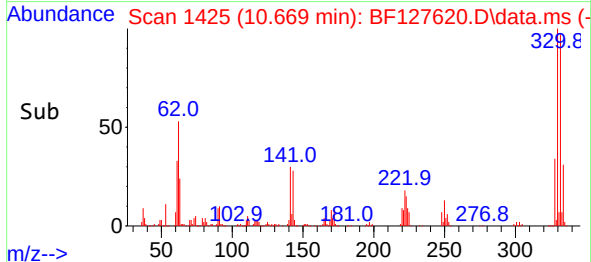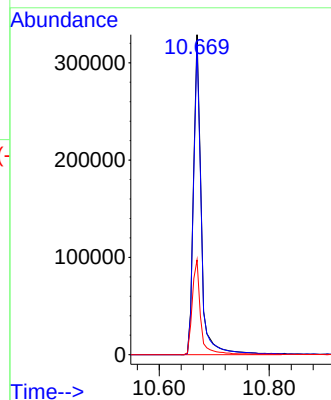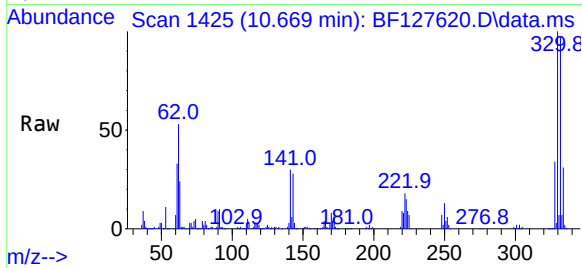

#45

2-Fluorobiphenyl

Concen: 88.527 ng

RT: 9.192 min Scan# 1174

Delta R.T. 0.000 min

Lab File: BF127620.D

Acq: 01 Apr 2022 19:03




Tgt Ion:172 Resp: 1331851


Ion Ratio Lower Upper

172 100

171 34.7 28.4 42.6

170 23.8 18.6 27.8


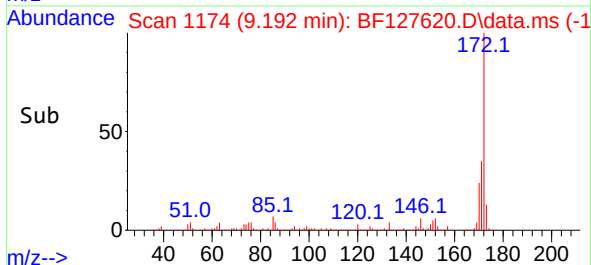
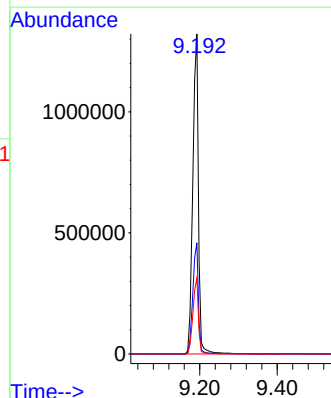
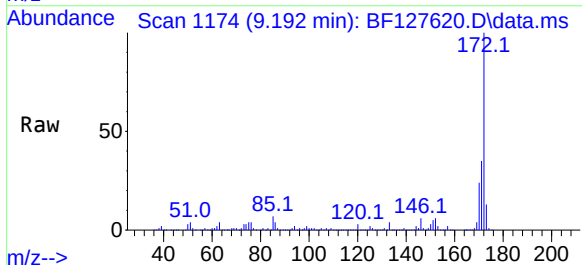


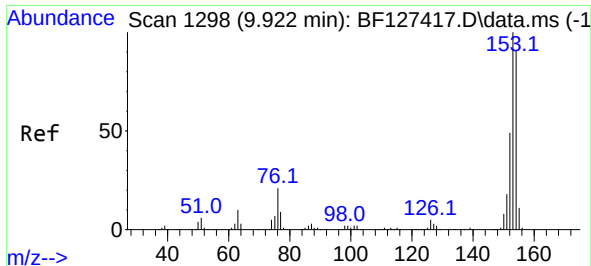

#52
Acenaphthene
Concen: 2.905 ng
RT: 9.904 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF127620.D
Acq: 01 Apr 2022 19:03




Instrument :
BNA_F
ClientSampleId :
MHF


Tgt Ion:154 Resp: 33481
Ion Ratio Lower Upper
154 100
153 110.3 87.6 131.4
152 51.7 42.9 64.3

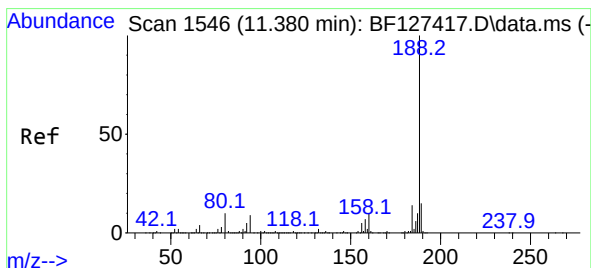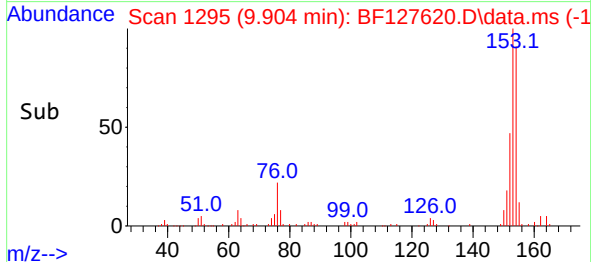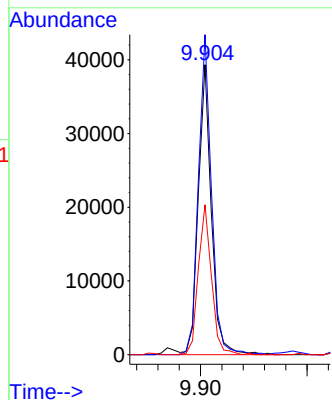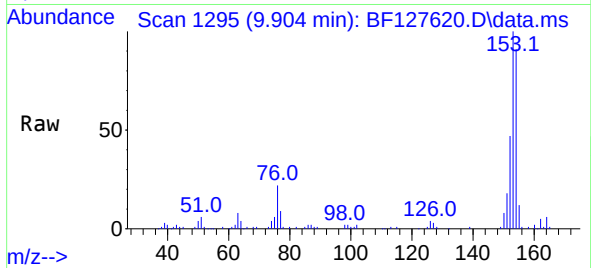

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.363 min Scan# 1543
Delta R.T. 0.000 min
Lab File: BF127620.D
Acq: 01 Apr 2022 19:03

Tgt Ion:188 Resp: 401944
Ion Ratio Lower Upper
188 100
94 10.8 7.4 11.0
80 11.6 8.0 12.0


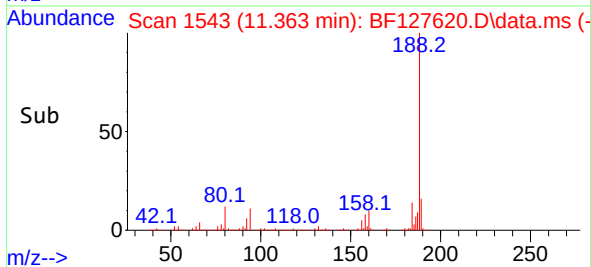
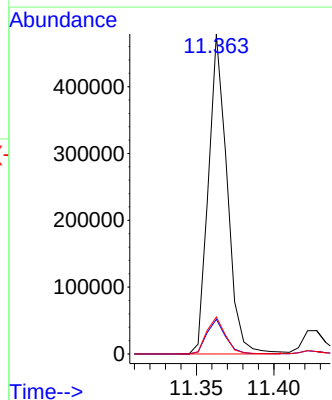
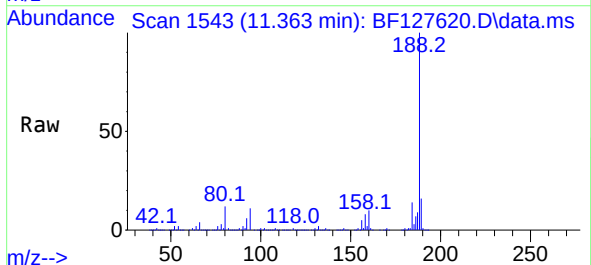


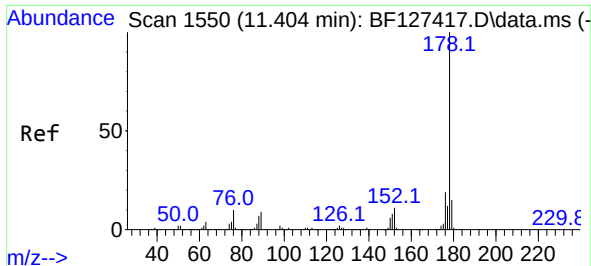

#71
Phenanthrene
Concen: 2.268 ng
RT: 11.386 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF127620.D
Acq: 01 Apr 2022 19:03




Instrument :
BNA_F
ClientSampleId :
MHF


Tgt Ion:178 Resp: 47536
Ion Ratio Lower Upper
178 100
176 16.9 15.4 23.2
179 14.7 12.4 18.6

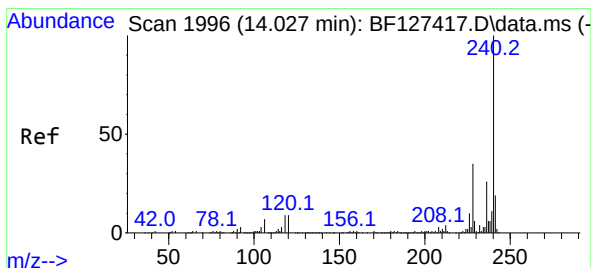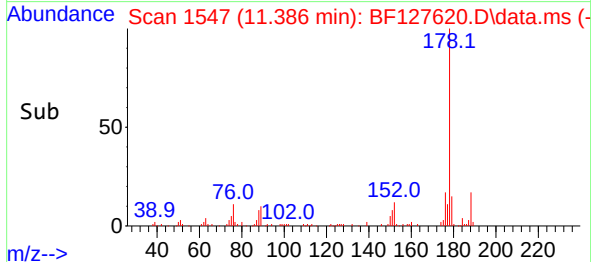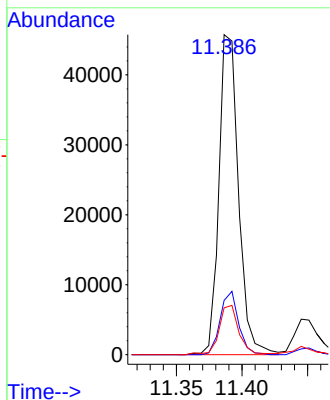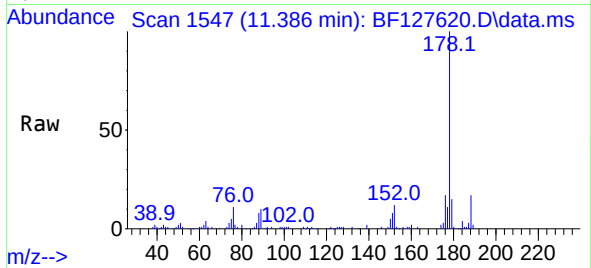

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.016 min Scan# 1994
Delta R.T. 0.000 min
Lab File: BF127620.D
Acq: 01 Apr 2022 19:03


Tgt Ion:240 Resp: 261169
Ion Ratio Lower Upper
240 100
120 9.5 7.1 10.7
236 25.1 20.7 31.1

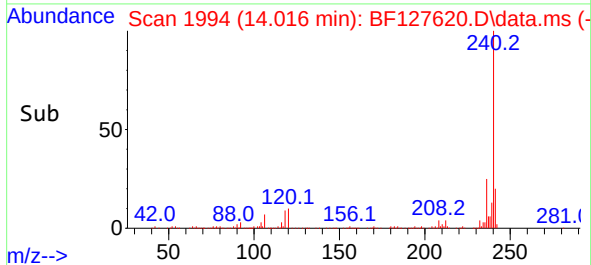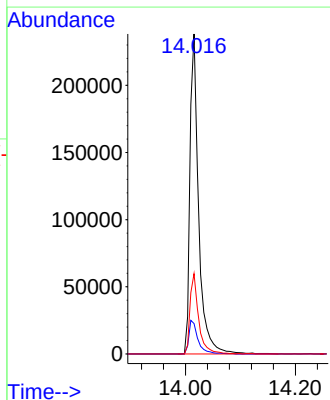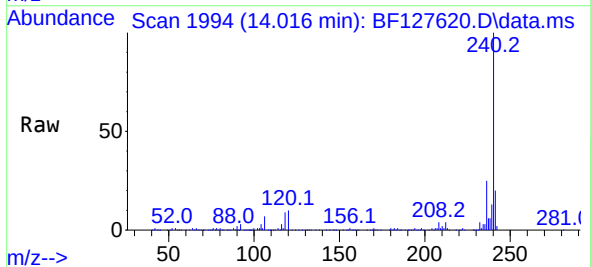



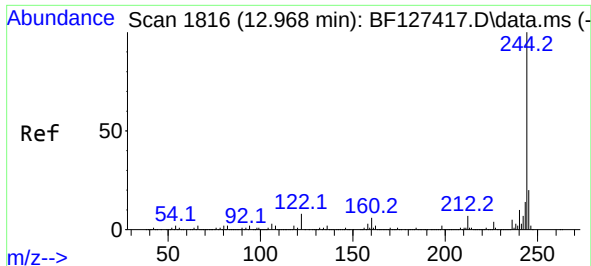


#79
 Terphenyl-d14
 Concen: 97.800 ng
 RT: 12.951 min Scan# 1813
 Delta R.T. 0.000 min
 Lab File: BF127620.D
 Acq: 01 Apr 2022 19:03

Instrument :
 BNA_F
 ClientSampleId :
 MHF

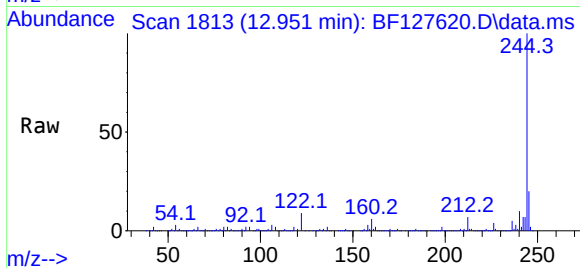

Tgt Ion:244 Resp: 1560299
 Ion Ratio Lower Upper
 244 100
 212 7.3 5.7 8.5
 122 9.5 6.2 9.2#

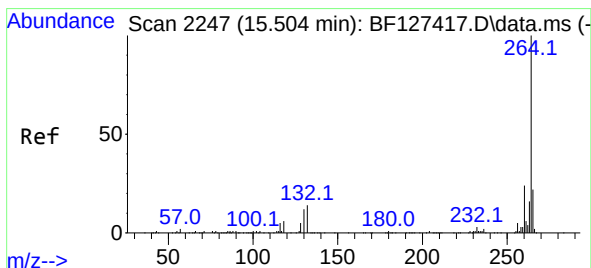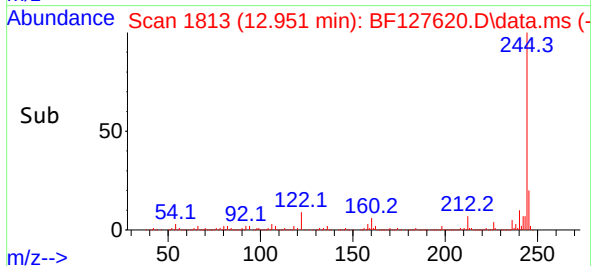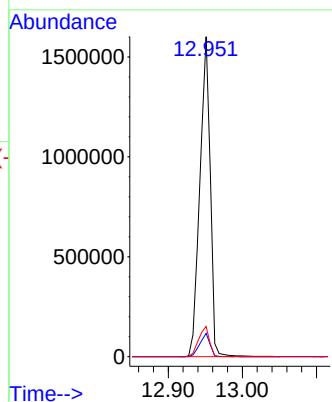

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.498 min Scan# 2246
 Delta R.T. 0.006 min
 Lab File: BF127620.D
 Acq: 01 Apr 2022 19:03

Tgt Ion:264 Resp: 189816
 Ion Ratio Lower Upper
 264 100
 260 24.8 19.1 28.7
 265 21.5 17.4 26.2

