

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040215\
 Data File : BF078215.D
 Acq On : 2 Apr 2015 22:35
 Operator : TP/IZ
 Sample : G1736-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-11

Quant Time: Apr 03 01:19:19 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 03 00:57:15 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.01	152	34194	20.00	ng	0.00
21) Naphthalene-d8	8.59	136	141241	20.00	ng	0.00
38) Acenaphthene-d10	10.76	164	66792	20.00	ng	0.00
63) Phenanthrene-d10	12.59	188	133760	20.00	ng	0.00
75) Chrysene-d12	15.86	240	135917	20.00	ng	-0.02
86) Perylene-d12	17.56	264	126730	20.00	ng	-0.10
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	117328	56.57	ng	0.01
7) Phenol-d6	6.60	99	92002	35.40	ng	0.00
23) Nitrobenzene-d5	7.71	82	206807	88.75	ng	-0.01
41) 2,4,6-Tribromophenol	11.75	330	85054	153.54	ng	0.00
44) 2-Fluorobiphenyl	9.94	172	457709	97.95	ng	0.00
78) Terphenyl-d14	14.59	244	550494	91.52	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040215\
Data File : BF078215.D
Acq On : 2 Apr 2015 22:35
Operator : TP/IZ
Sample : G1736-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-11

Quant Time: Apr 03 01:19:19 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 03 00:57:15 2015
Response via : Initial Calibration

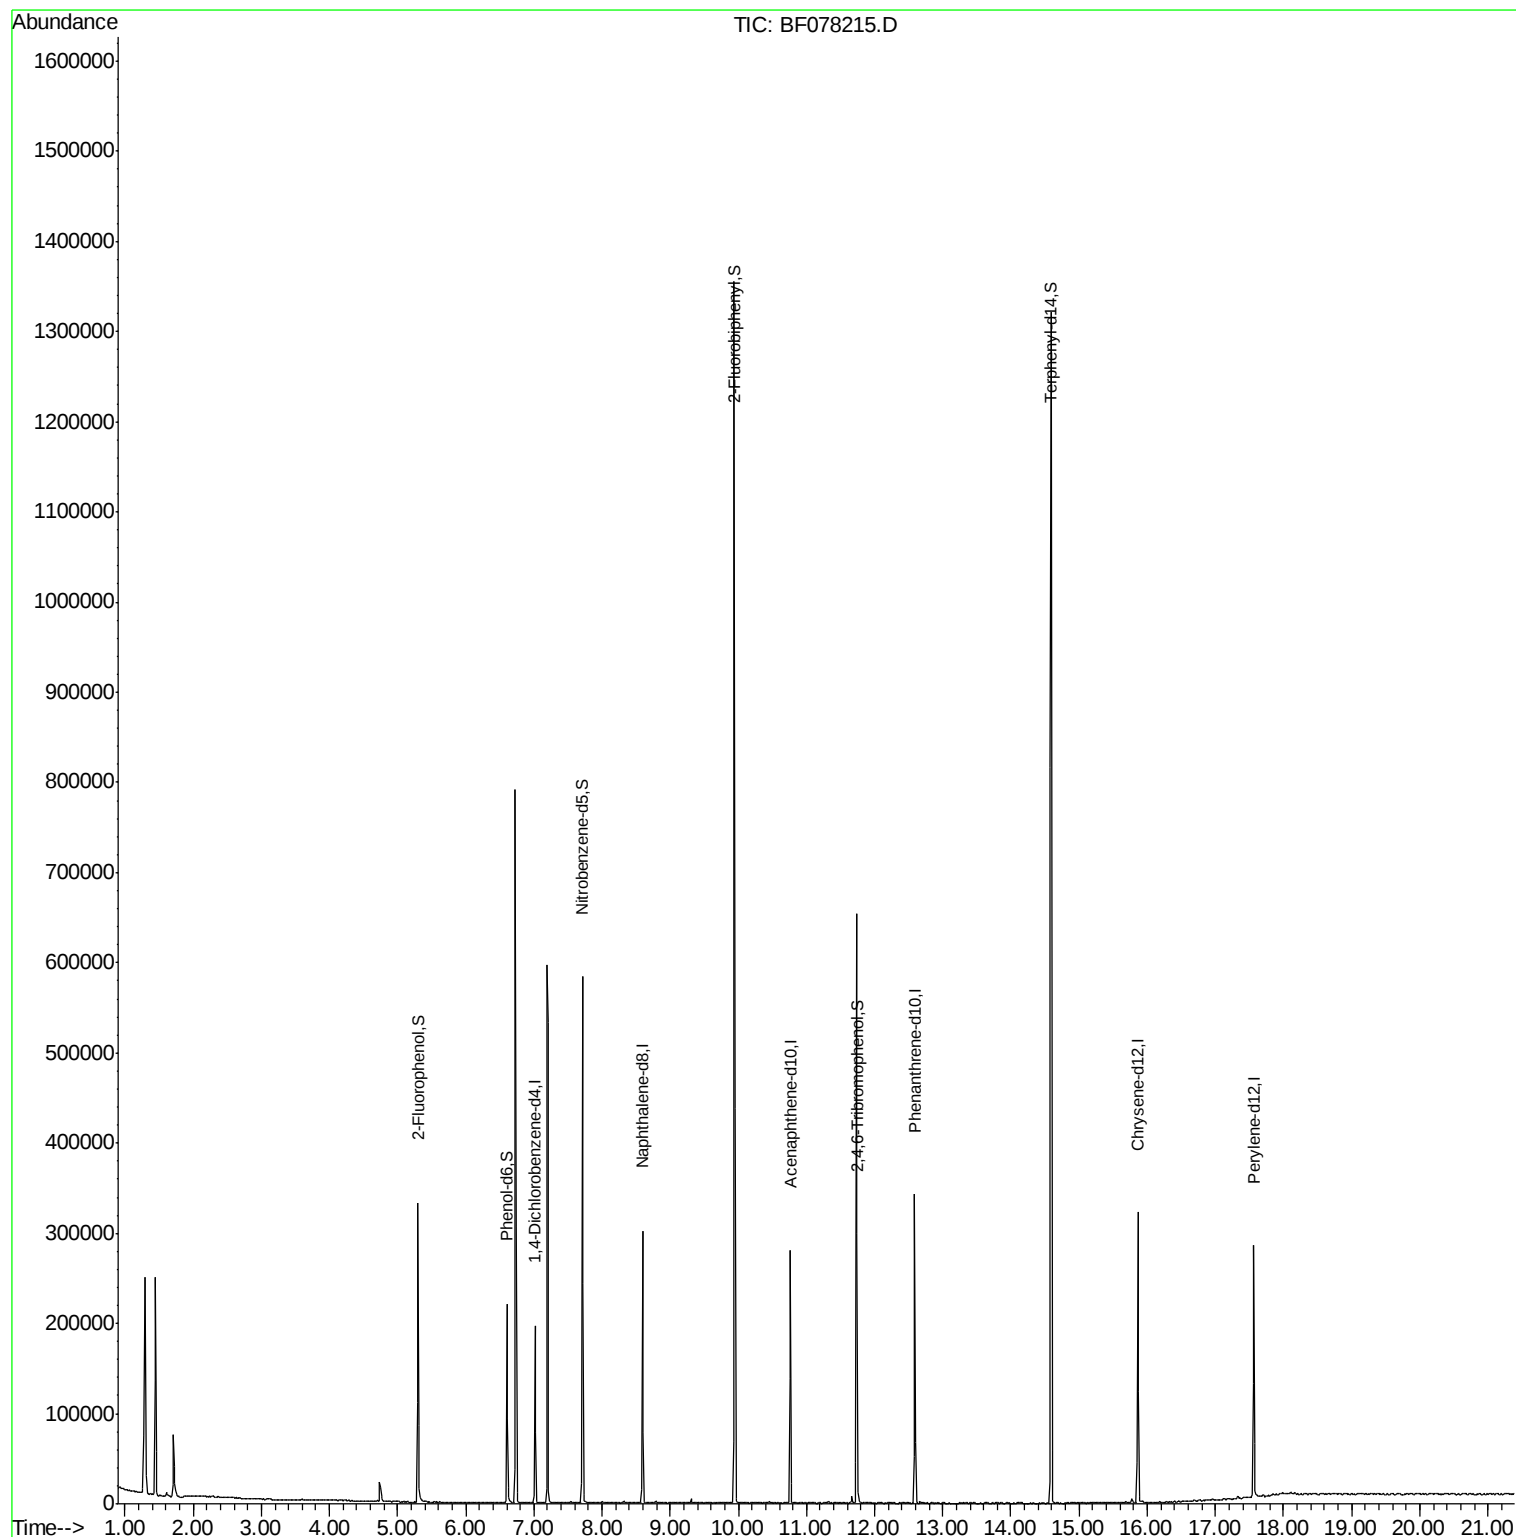




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.01 min Scan# 536
Delta R.T. 0.00 min
Lab File: BF078215.D
Acq: 2 Apr 2015 22:35

Instrument :
BNA_F
ClientSampleId :
MW-11

Tot Ion:152 Resp: 34194
Ion Ratio Lower Upper
152 100
150 165.3 125.9 188.9
115 67.5 52.7 79.1

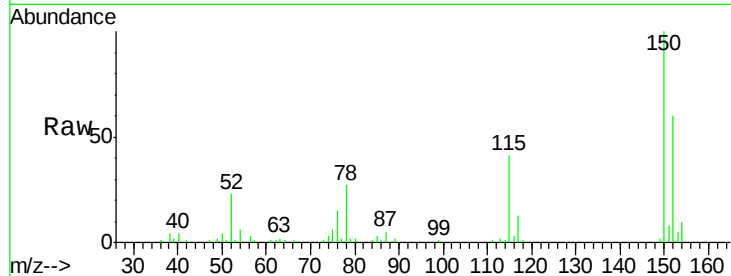


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

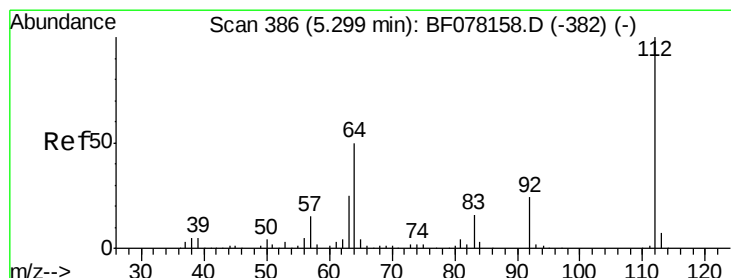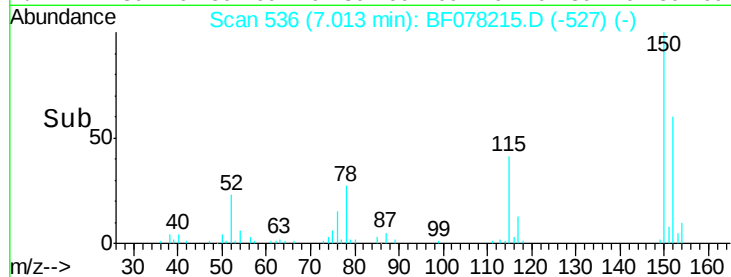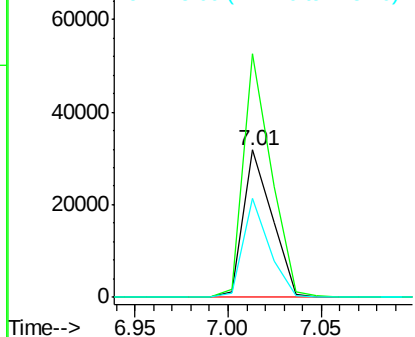



#5


2-Fluorophenol
Concen: 56.57 ng
RT: 5.30 min Scan# 386
Delta R.T. 0.01 min
Lab File: BF078215.D
Acq: 2 Apr 2015 22:35

Tgt Ion:112 Resp: 117328
Ion Ratio Lower Upper
112 100
64 53.1 39.9 59.9
63 26.3 20.2 30.4



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

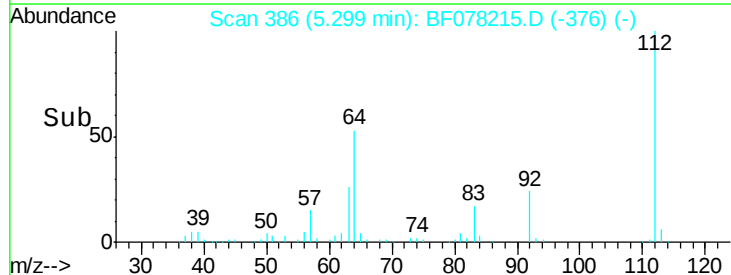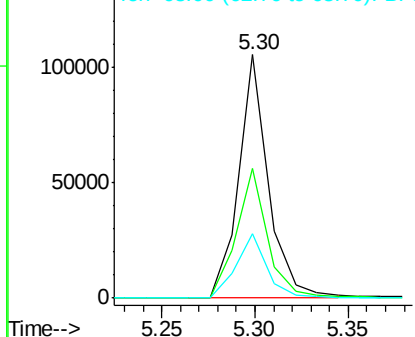

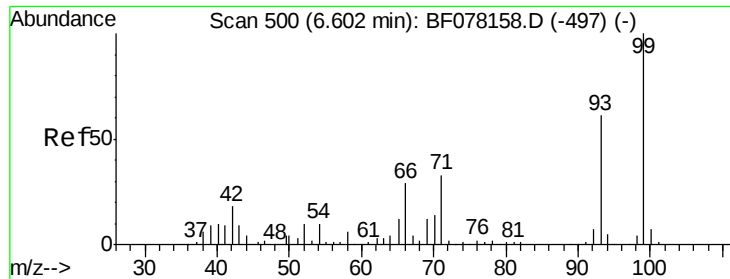

#7

Phenol-d6

Concen: 35.40 ng

RT: 6.60 min Scan# 500

Delta R.T. 0.00 min

Lab File: BF078215.D

Acq: 2 Apr 2015 22:35

Instrument :

BNA_F

ClientSampled :

MW-11


Tot Ion: 99 Resp: 92002

Ion Ratio Lower Upper

99 100

42 17.1 14.8 22.2




71 32.4 26.6 39.8

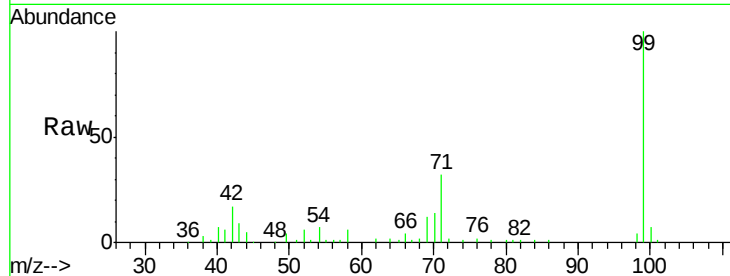

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

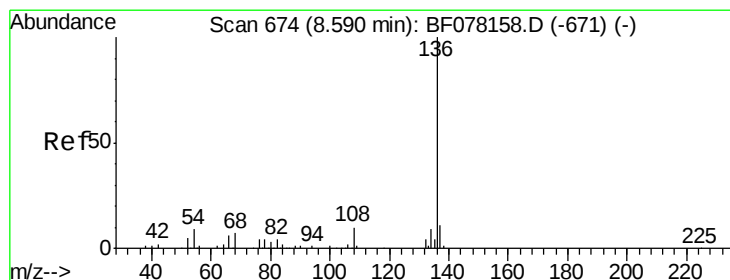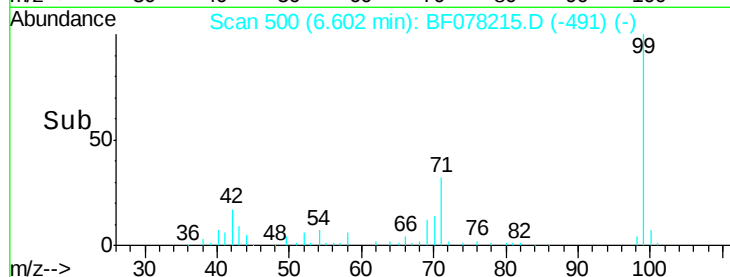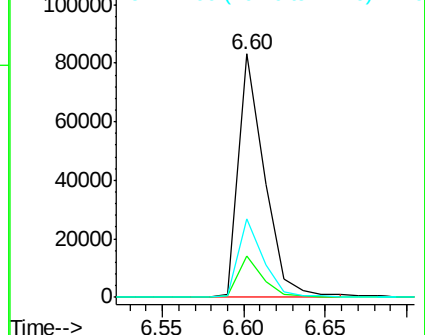

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.59 min Scan# 674

Delta R.T. 0.00 min

Lab File: BF078215.D

Acq: 2 Apr 2015 22:35

Tgt Ion: 136 Resp: 141241


Ion Ratio Lower Upper

136 100

137 11.2 9.0 13.4

54 8.2 7.0 10.6

68 6.7 5.4 8.2


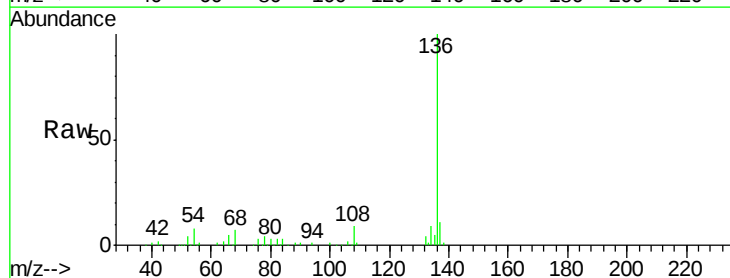


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



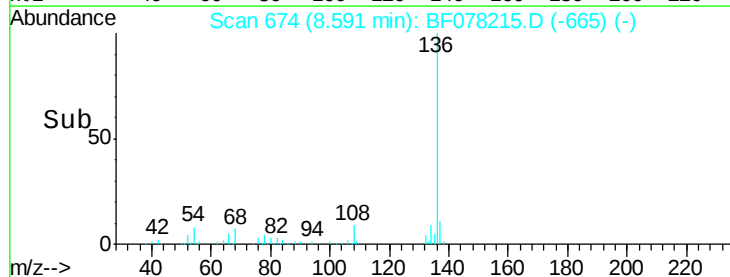
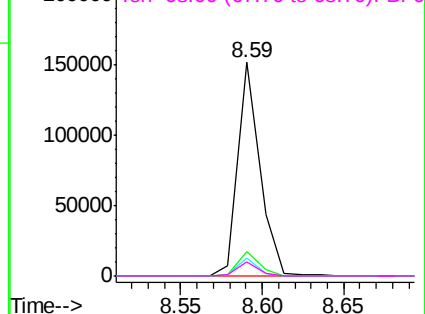




#23
 Nitrobenzene-d5
 Concen: 88.75 ng
 RT: 7.71 min Scan# 597
 Delta R.T. -0.01 min
 Lab File: BF078215.D
 Acq: 2 Apr 2015 22:35




Instrument :
 BNA_F
 ClientSampleId :
 MW-11


Tot Ion	82	Resp	206807
Ion Ratio	100	Lower	Upper
128	41.2	31.8	47.8
54	52.3	41.5	62.3

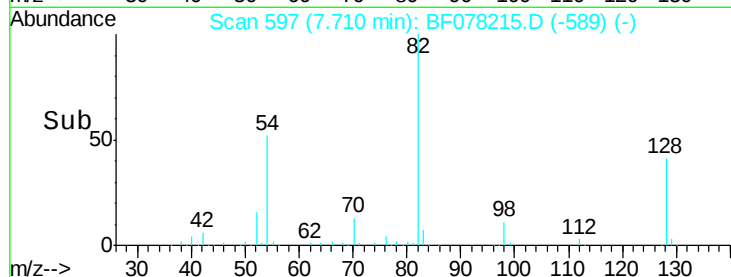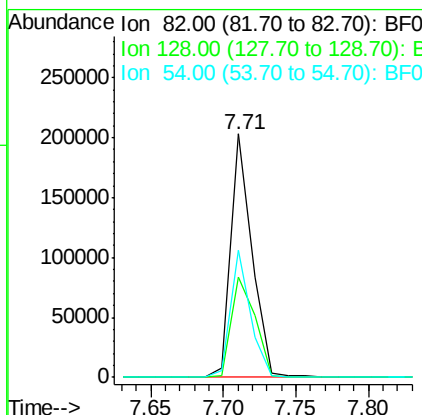

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.76 min Scan# 864
 Delta R.T. 0.00 min
 Lab File: BF078215.D
 Acq: 2 Apr 2015 22:35

Tgt Ion	164	Resp	66792
Ion Ratio	100	Lower	Upper
162	106.2	82.2	123.2
160	45.8	34.7	52.1


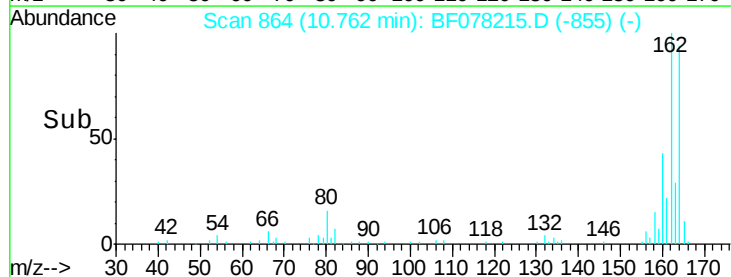
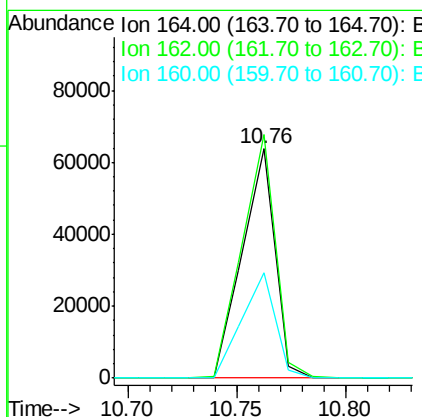



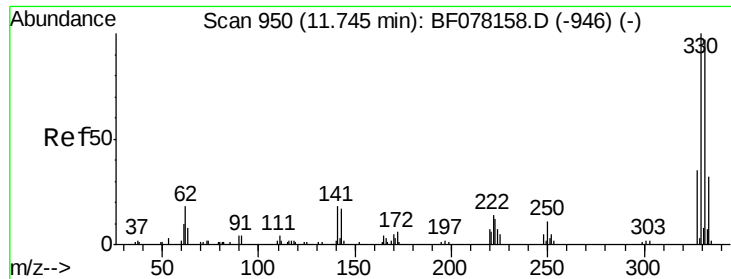

#41
 2,4,6-Tribromophenol
 Concen: 153.54 ng
 RT: 11.75 min Scan# 950
 Delta R.T. 0.00 min
 Lab File: BF078215.D
 Acq: 2 Apr 2015 22:35




Instrument :
 BNA_F
 ClientSampleId :
 MW-11

Tot Ion:330 Resp: 85054
 Ion Ratio Lower Upper
 330 100
 332 97.6 78.6 117.8
 141 39.0 31.2 46.8

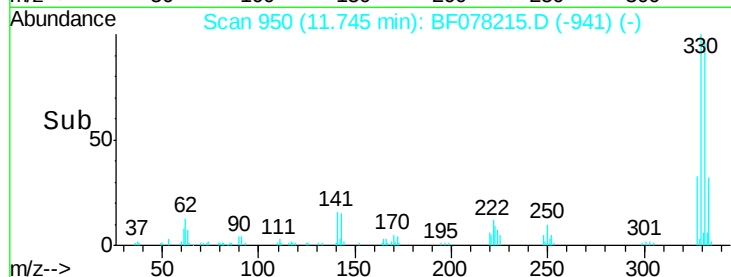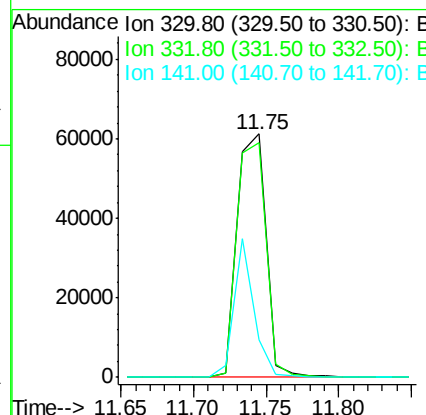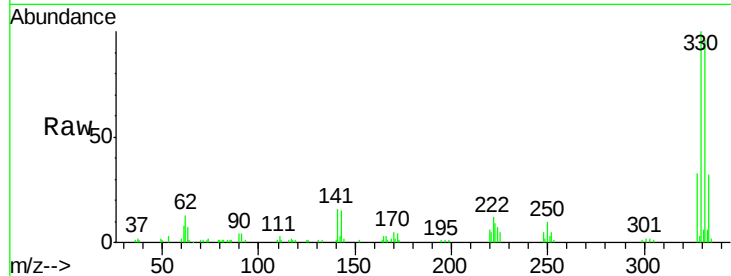

#44
 2-Fluorobiphenyl
 Concen: 97.95 ng
 RT: 9.94 min Scan# 792
 Delta R.T. 0.00 min
 Lab File: BF078215.D
 Acq: 2 Apr 2015 22:35

Tgt Ion:172 Resp: 457709
 Ion Ratio Lower Upper
 172 100
 171 35.4 28.6 42.8
 170 23.4 18.5 27.7

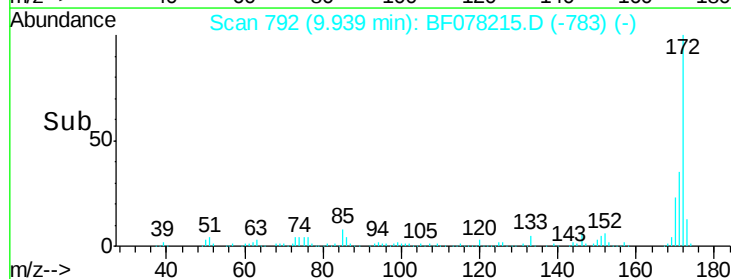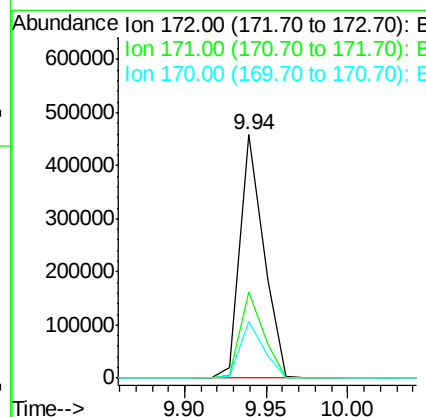







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.59 min Scan# 1024
Delta R.T. 0.00 min
Lab File: BF078215.D
Acq: 2 Apr 2015 22:35

Instrument :
BNA_F
ClientSampleId :
MW-11

Tot Ion:188 Resp: 133760
Ion Ratio Lower Upper
188 100
94 9.6 9.0 13.4
80 10.6 9.5 14.3

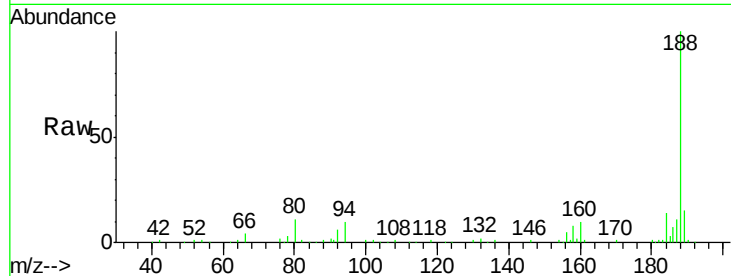


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

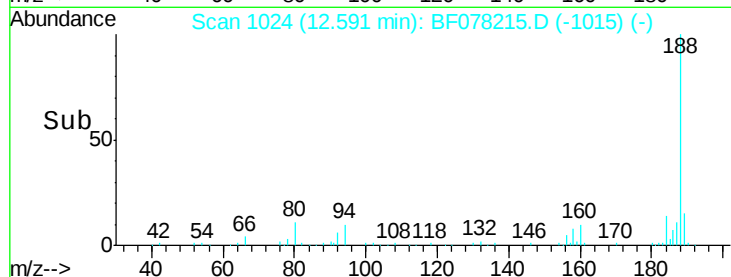
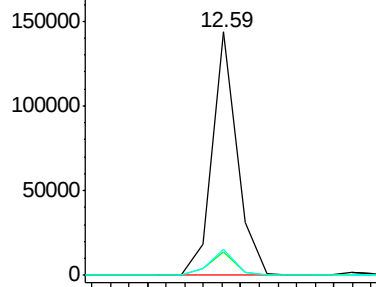


#75
Chrysene-d12
Concen: 20.00 ng
RT: 15.86 min Scan# 1310
Delta R.T. -0.02 min
Lab File: BF078215.D
Acq: 2 Apr 2015 22:35

Tgt Ion:240 Resp: 135917
Ion Ratio Lower Upper
240 100
120 13.8 7.1 10.7#
236 24.9 21.4 32.2



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

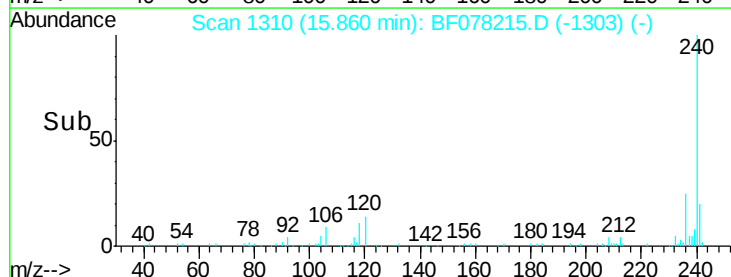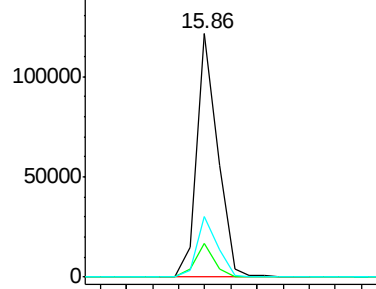







#78
 Terphenyl-d14
 Concen: 91.52 ng
 RT: 14.59 min Scan# 1199
 Delta R.T. 0.00 min
 Lab File: BF078215.D
 Acq: 2 Apr 2015 22:35

Instrument :
 BNA_F
 ClientSampleId :
 MW-11

Tot Ion:244 Resp: 550494
 Ion Ratio Lower Upper
 244 100
 212 6.6 5.0 7.4
 122 9.4 7.1 10.7




Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

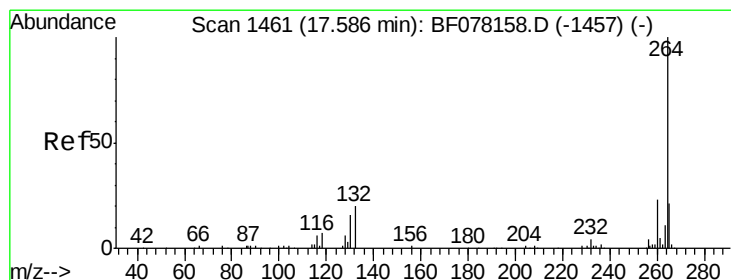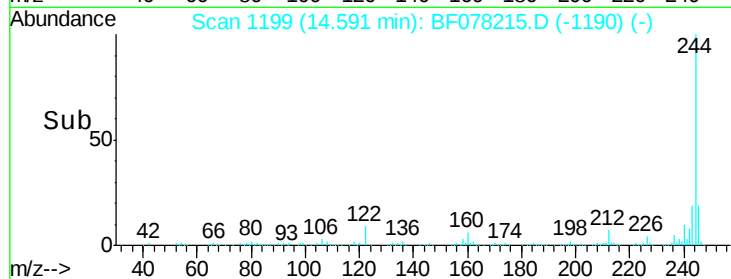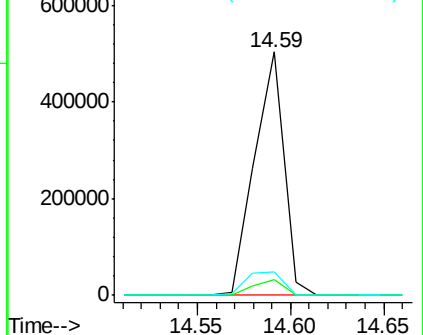

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 17.56 min Scan# 1459
 Delta R.T. -0.10 min
 Lab File: BF078215.D
 Acq: 2 Apr 2015 22:35

Tgt Ion:264 Resp: 126730
 Ion Ratio Lower Upper
 264 100
 260 22.9 18.6 27.8
 265 22.0 17.0 25.6

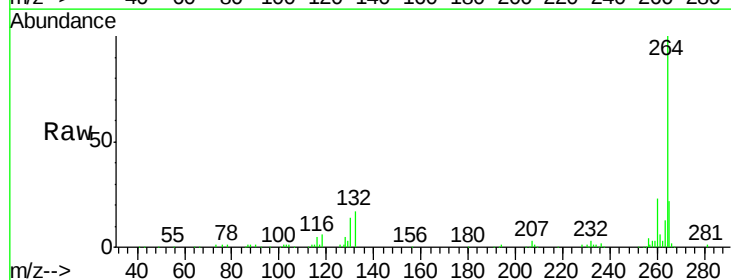

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

