

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040215\
 Data File : BF078203.D
 Acq On : 2 Apr 2015 16:53
 Operator : TP/IZ
 Sample : G1653-06RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FD2RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.184	24	26	28	rBV	250869	275344	18.61%	0.893%
2	1.298	32	36	38	rVB	75713	137564	9.30%	0.446%
3	1.447	47	49	52	rVB	76644	100265	6.77%	0.325%
4	1.710	70	72	83	rVB	42087	64543	4.36%	0.209%
5	4.739	335	337	350	rVB	88290	116640	7.88%	0.378%
6	5.299	383	386	397	rBV	779995	968196	65.42%	3.139%
7	6.464	486	488	492	rBB	20890	22342	1.51%	0.072%
8	6.602	498	500	503	rBV	850630	949913	64.19%	3.080%
9	6.727	509	511	514	rBV	912489	1024428	69.22%	3.321%
10	7.013	534	536	539	rBV	241038	252315	17.05%	0.818%
11	7.196	550	552	555	rBV	605967	820553	55.45%	2.660%
12	7.287	557	560	561	rBV2	14371	28609	1.93%	0.093%
13	7.333	563	564	568	rBV4	48213	118309	7.99%	0.384%
14	7.447	571	574	575	rBV	27592	43502	2.94%	0.141%
15	7.493	575	578	580	rVV4	95625	181347	12.25%	0.588%
16	7.539	580	582	584	rVV2	122466	223406	15.10%	0.724%
17	7.585	584	586	587	rVV2	83306	151516	10.24%	0.491%
18	7.619	587	589	590	rVV2	96516	181036	12.23%	0.587%
19	7.665	590	593	594	rVV3	155310	329126	22.24%	1.067%
20	7.710	594	597	599	rVV	652768	938840	63.44%	3.044%
21	7.756	599	601	604	rVV4	160381	469829	31.75%	1.523%
22	7.825	604	607	609	rVV2	218684	516262	34.88%	1.674%
23	7.870	609	611	612	rVV2	172660	268352	18.13%	0.870%
24	7.905	612	614	615	rVV2	192106	335059	22.64%	1.086%
25	7.939	615	617	620	rVV3	195633	560788	37.89%	1.818%
26	8.007	620	623	628	rVV2	621361	1479929	100.00%	4.798%
27	8.087	628	630	631	rVV2	267500	468033	31.63%	1.517%
28	8.122	631	633	634	rVV	227606	435197	29.41%	1.411%
29	8.145	634	635	639	rVV2	843189	1129413	76.32%	3.662%
30	8.213	639	641	643	rVV2	279852	635910	42.97%	2.062%
31	8.259	643	645	648	rVV3	258489	757329	51.17%	2.455%
32	8.305	648	649	655	rVV5	271568	1097739	74.18%	3.559%
33	8.396	655	657	659	rVV2	264793	602699	40.72%	1.954%
34	8.430	659	660	661	rVV	271353	301619	20.38%	0.978%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040215\
 Data File : BF078203.D
 Acq On : 2 Apr 2015 16:53
 Operator : TP/IZ
 Sample : G1653-06RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FD2RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	8.488	663	665	666	rVV2	398160	639884	43.24%	2.075%
36	8.510	666	667	671	rVV2	203606	546347	36.92%	1.771%
37	8.590	671	674	677	rVV2	496188	1029856	69.59%	3.339%
38	8.648	677	679	682	rVV4	171978	407840	27.56%	1.322%
39	8.728	684	686	689	rVV	118928	267531	18.08%	0.867%
40	8.773	689	690	691	rVV	113288	101907	6.89%	0.330%
41	8.808	691	693	694	rVV2	61012	85790	5.80%	0.278%
42	8.865	694	698	701	rVV5	45043	155073	10.48%	0.503%
43	8.956	703	706	707	rVV2	49556	77339	5.23%	0.251%
44	8.990	707	709	711	rVB3	37919	58669	3.96%	0.190%
45	9.093	717	718	720	rVB2	29001	28056	1.90%	0.091%
46	9.162	721	724	726	rVV2	55041	86379	5.84%	0.280%
47	9.219	727	729	731	rVB2	26984	32350	2.19%	0.105%
48	9.379	740	743	746	rBV4	27790	64624	4.37%	0.210%
49	9.436	746	748	749	rVV	30332	42990	2.90%	0.139%
50	9.482	749	752	756	rVV5	31986	79501	5.37%	0.258%
51	9.539	756	757	759	rVV2	22528	29916	2.02%	0.097%
52	9.619	763	764	767	rVB3	24001	22892	1.55%	0.074%
53	9.688	767	770	774	rBV4	13700	43154	2.92%	0.140%
54	9.905	788	789	790	rBV	25848	27804	1.88%	0.090%
55	9.939	790	792	795	rVB	1202394	1135750	76.74%	3.682%
56	10.031	797	800	802	rBV3	6852	19979	1.35%	0.065%
57	10.076	802	804	806	rBV2	25226	34802	2.35%	0.113%
58	10.156	810	811	813	rVB	24232	26733	1.81%	0.087%
59	10.316	820	825	826	rBV3	25666	49866	3.37%	0.162%
60	10.339	826	827	829	rVV2	13112	20646	1.40%	0.067%
61	10.396	829	832	835	rVV3	21495	50499	3.41%	0.164%
62	10.453	835	837	840	rVV	135530	175308	11.85%	0.568%
63	10.693	856	858	860	rBV3	19348	29171	1.97%	0.095%
64	10.762	860	864	866	rBV2	388362	511284	34.55%	1.658%
65	11.025	884	887	889	rBV3	29338	65390	4.42%	0.212%
66	11.128	895	896	898	rBV	24187	32740	2.21%	0.106%
67	11.173	898	900	901	rBV2	24040	32823	2.22%	0.106%
68	11.288	906	910	912	rBV3	47356	115048	7.77%	0.373%
69	11.356	912	916	919	rBV	69148	159472	10.78%	0.517%
70	11.402	919	920	922	rBV2	39580	44241	2.99%	0.143%
71	11.482	925	927	930	rBV3	40455	87328	5.90%	0.283%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040215\
 Data File : BF078203.D
 Acq On : 2 Apr 2015 16:53
 Operator : TP/IZ
 Sample : G1653-06RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FD2RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	11.631	937	940	943	rBV	180235	248367	16.78%	0.805%
73	11.734	947	949	953	rBV	590995	689488	46.59%	2.235%
74	11.836	956	958	959	rBV	41039	59306	4.01%	0.192%
75	11.871	959	961	963	rBV2	56003	52315	3.53%	0.170%
76	11.916	963	965	966	rBV2	63386	96730	6.54%	0.314%
77	11.962	966	969	975	rVV	558349	760303	51.37%	2.465%
78	12.054	975	977	979	rBV3	58288	116848	7.90%	0.379%
79	12.191	986	989	990	rBV2	92036	143833	9.72%	0.466%
80	12.225	990	992	995	rVB2	72149	100718	6.81%	0.327%
81	12.465	1011	1013	1014	rBV	104254	134323	9.08%	0.435%
82	12.499	1014	1016	1018	rVV2	87705	143239	9.68%	0.464%
83	12.545	1018	1020	1022	rVB	495968	623827	42.15%	2.023%
84	12.591	1022	1024	1027	rBV	407754	515508	34.83%	1.671%
85	12.682	1030	1032	1034	rBV	119881	179538	12.13%	0.582%
86	12.979	1056	1058	1062	rVB	295779	439618	29.71%	1.425%
87	14.431	1183	1185	1186	rBV	14666	21776	1.47%	0.071%
88	14.591	1196	1199	1201	rBV	1091433	1318472	89.09%	4.275%
89	14.945	1228	1230	1231	rBV	19000	20524	1.39%	0.067%
90	15.460	1273	1275	1277	rVB	60022	71685	4.84%	0.232%
91	15.768	1300	1302	1308	rBV2	153560	308533	20.85%	1.000%
92	15.871	1308	1311	1313	rVB	316932	454284	30.70%	1.473%
93	17.608	1460	1463	1467	rVB	294552	460115	31.09%	1.492%
94	17.746	1473	1475	1480	rVB4	56882	99797	6.74%	0.324%
95	18.260	1518	1520	1529	rVB2	115242	279496	18.89%	0.906%
96	18.648	1551	1554	1558	rVB	128075	222211	15.01%	0.720%
97	19.094	1589	1593	1596	rBV	294927	569134	38.46%	1.845%
98	19.231	1602	1605	1614	rVB7	48253	164802	11.14%	0.534%
99	19.380	1615	1618	1621	rVB3	46622	85078	5.75%	0.276%
100	19.814	1653	1656	1659	rVB4	27260	59440	4.02%	0.193%


Sum of corrected areas: 30844242

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040215\
Data File : BF078203.D
Acq On : 2 Apr 2015 16:53
Operator : TP/IZ
Sample : G1653-06RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
FD2RE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

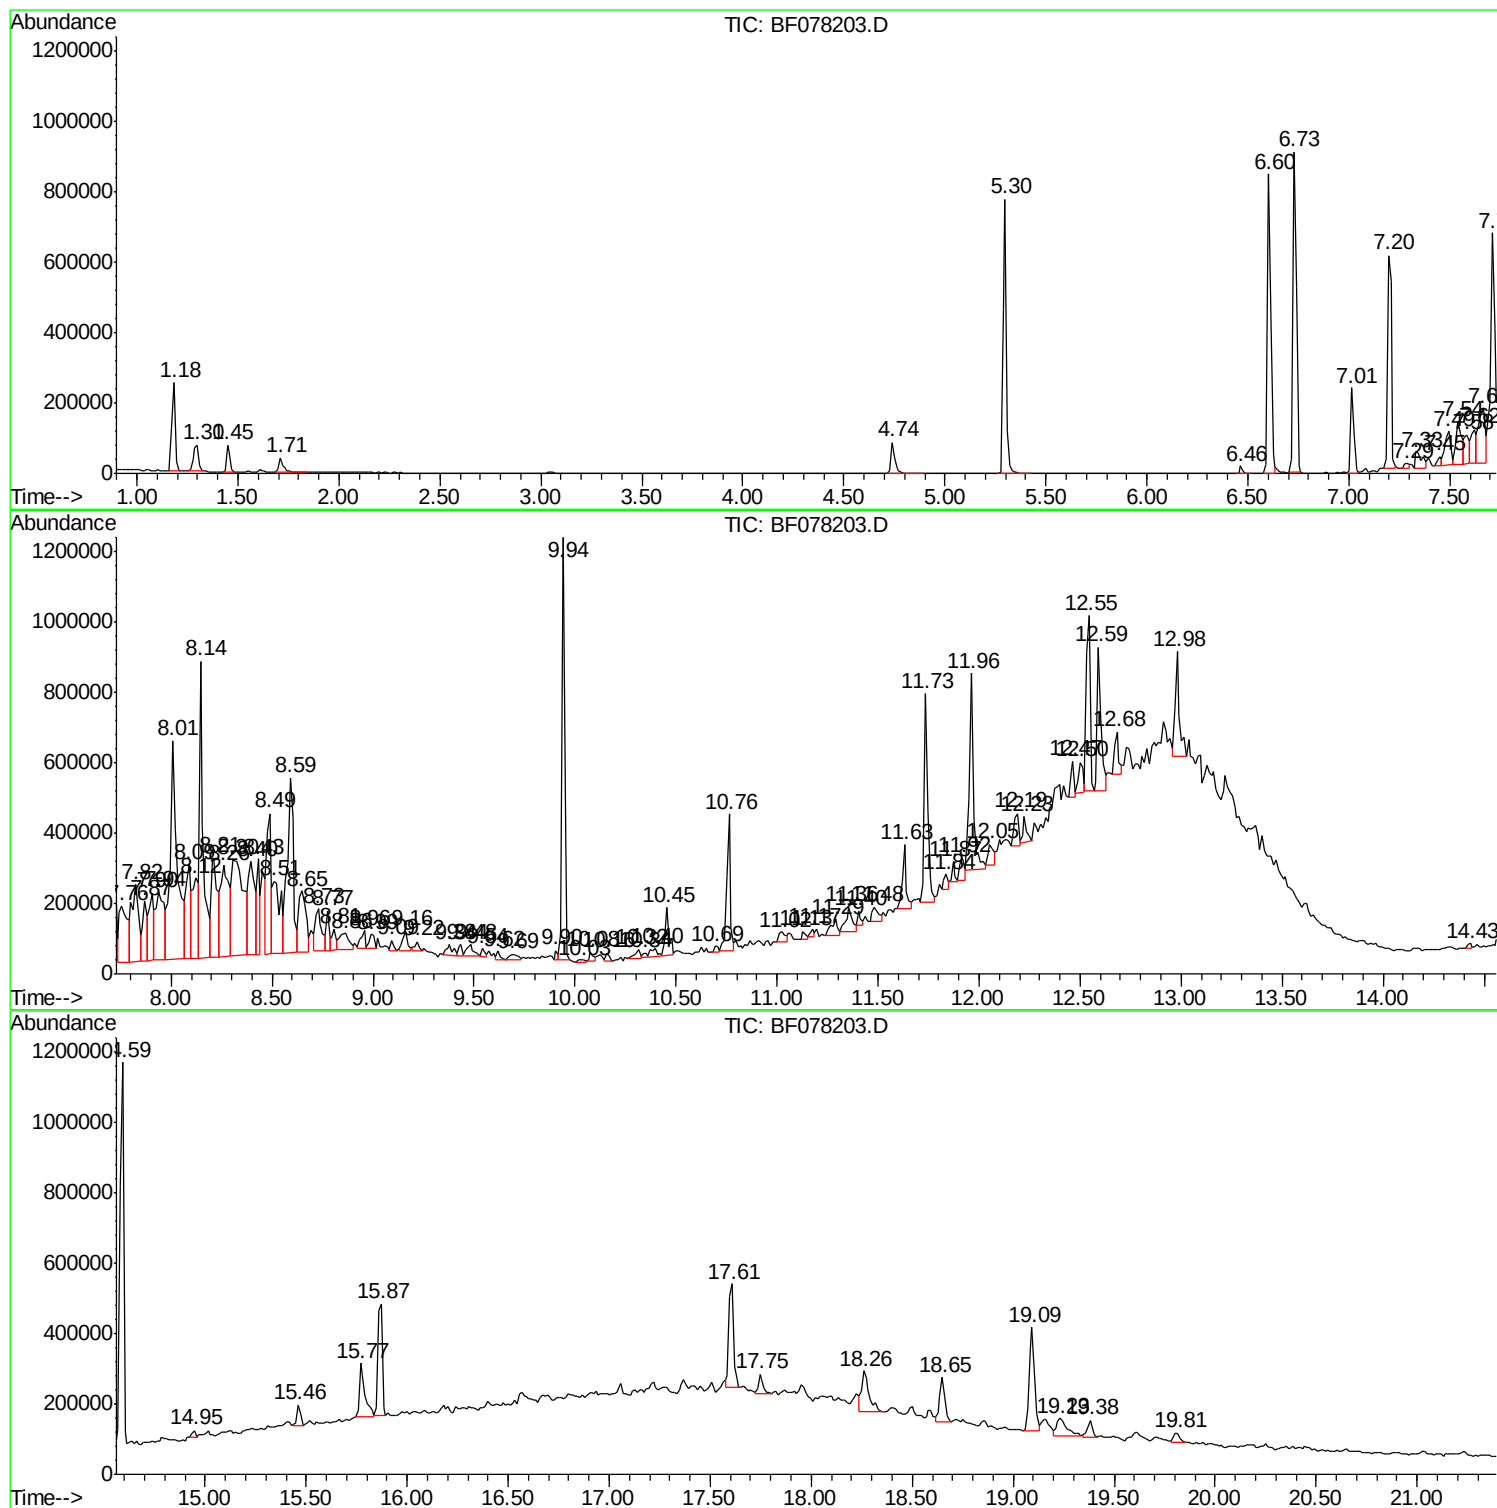

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF040215\
Data_File : BF078203.D
Acq_On : 2_Apr.2015_ 16:533
Operator : TP/IZZ
Sample : G1653-06REE
Misc :
ALS_Vial : 8 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
FD2RE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
