


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040215\
 Data File : BF078196.D
 Acq On : 2 Apr 2015 13:33
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 02 13:21:29 2015

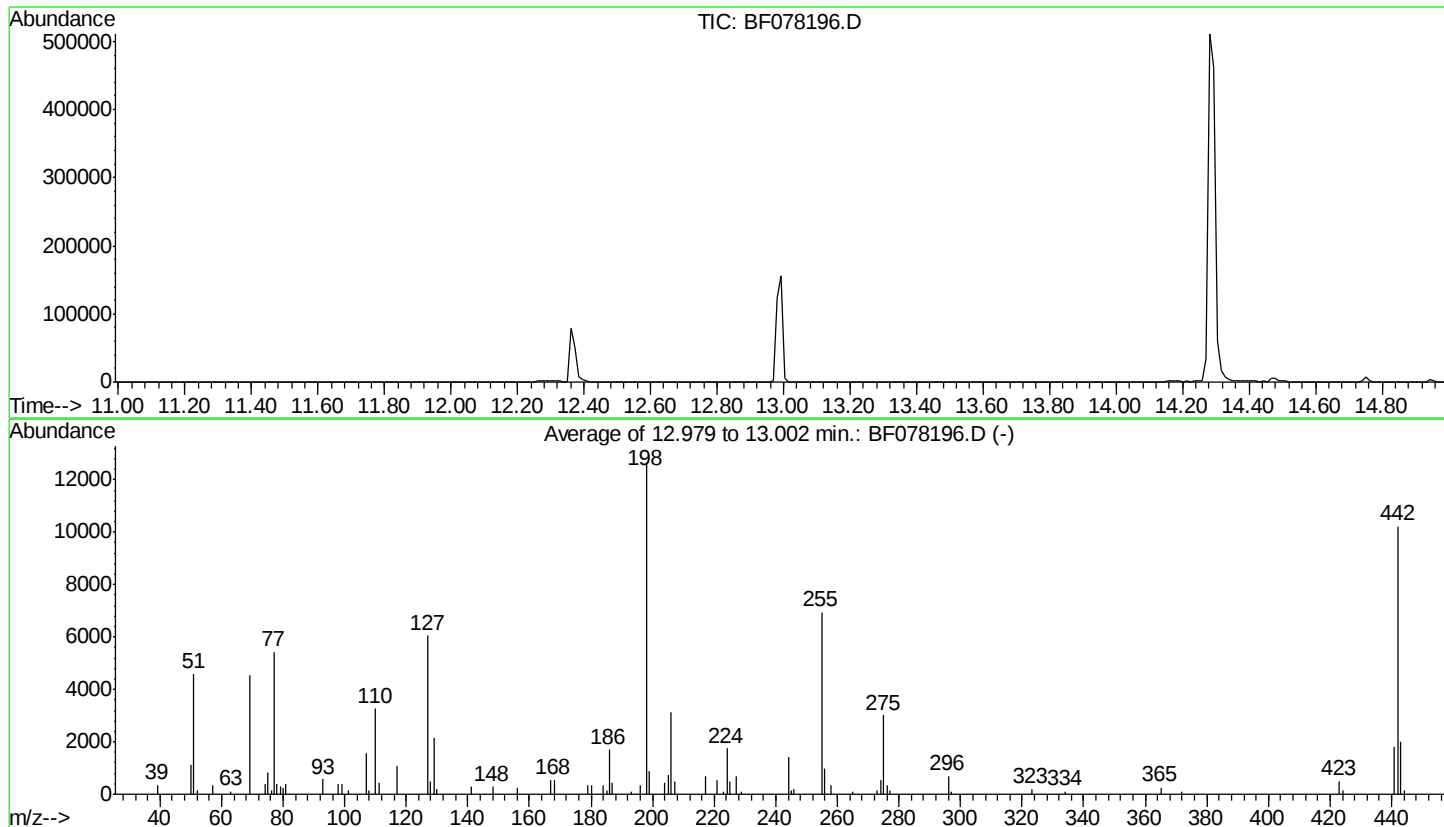

AutoFind: Scans 1058, 1059, 1060; Background Corrected with Scan 1054

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	4598	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.7	4520	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.8	6047	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12651	PASS
199	198	5	9	6.9	877	PASS
275	198	10	60	23.9	3022	PASS
365	198	1	100	2.1	270	PASS
441	442	0.01	24	17.6	1796	PASS
442	198	50	100	80.7	10208	PASS
443	442	15	24	19.7	2015	PASS