


Data Path : Z:\HPCHEM1\BNA F\DATA\BF040215\
Data File : BF078218.D
Acq On : 3 Apr 2015 1:12
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 02 13:21:29 2015

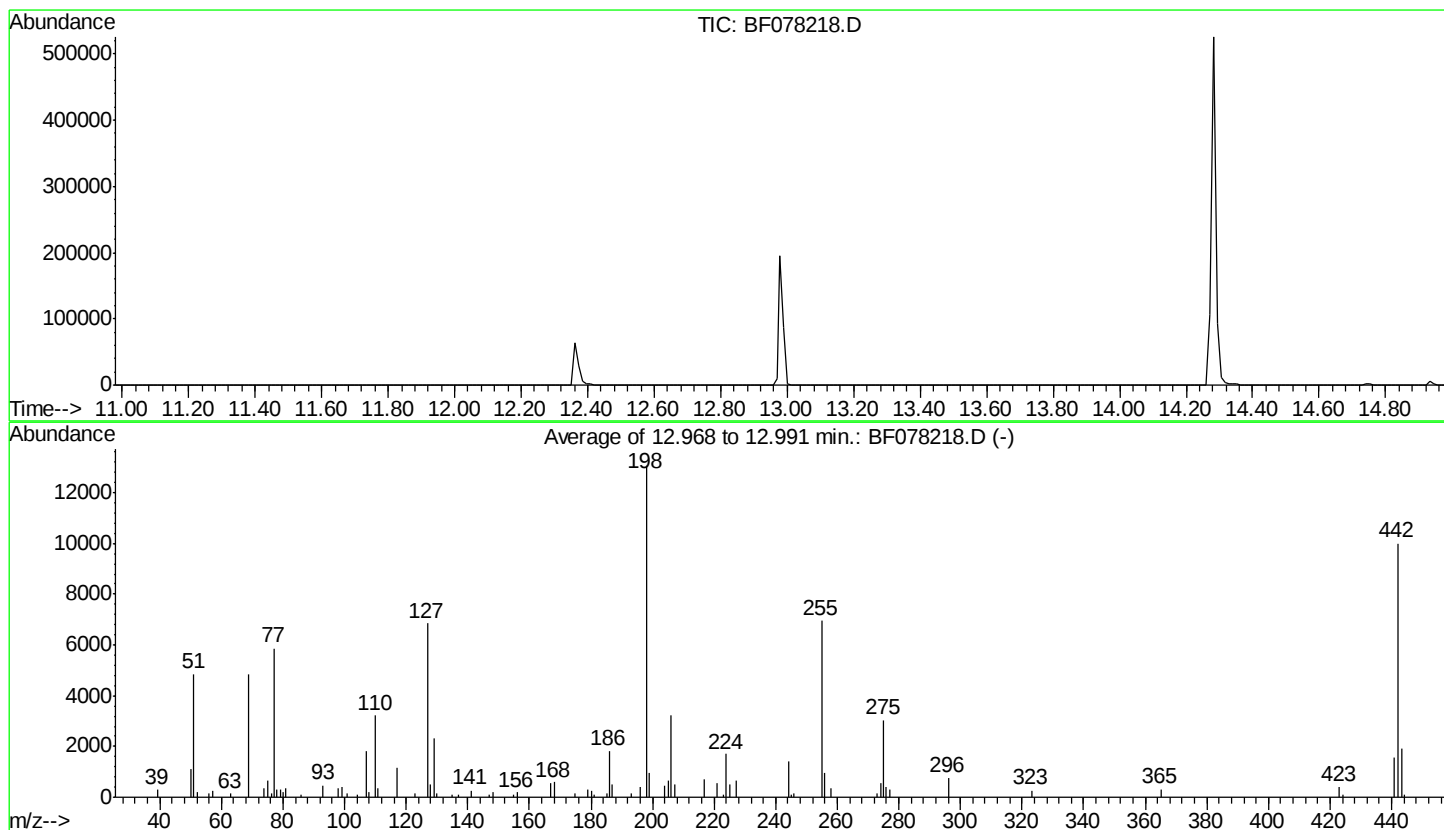

AutoFind: Scans 1057, 1058, 1059; Background Corrected with Scan 1054

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	4846	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.9	4822	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.4	6847	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13062	PASS
199	198	5	9	7.2	935	PASS
275	198	10	60	23.2	3027	PASS
365	198	1	100	2.4	320	PASS
441	442	0.01	24	15.8	1575	PASS
442	198	50	100	76.5	9991	PASS
443	442	15	24	19.1	1906	PASS