
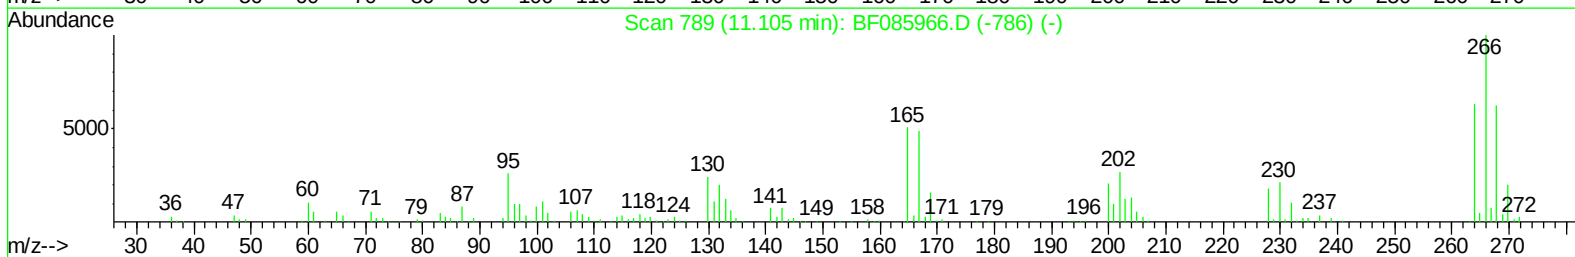
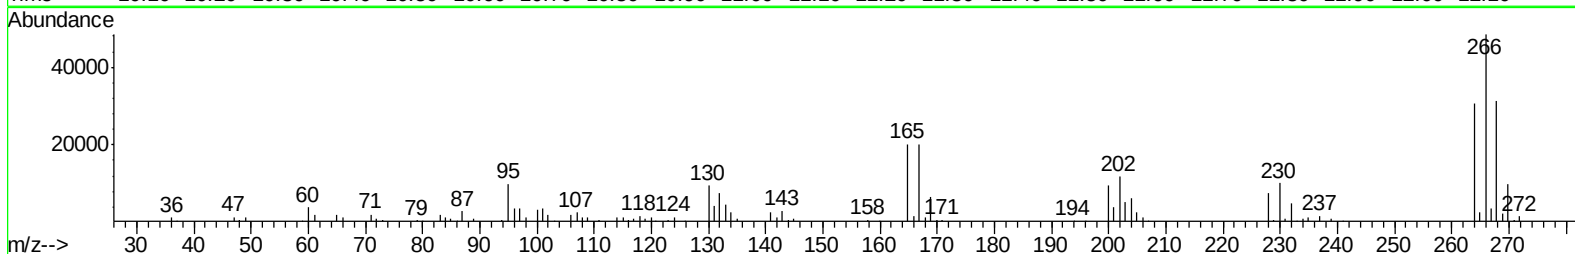


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040216\
Data File : BF085962.D
Acq On : 1 Apr 2016 15:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 05:38:03 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

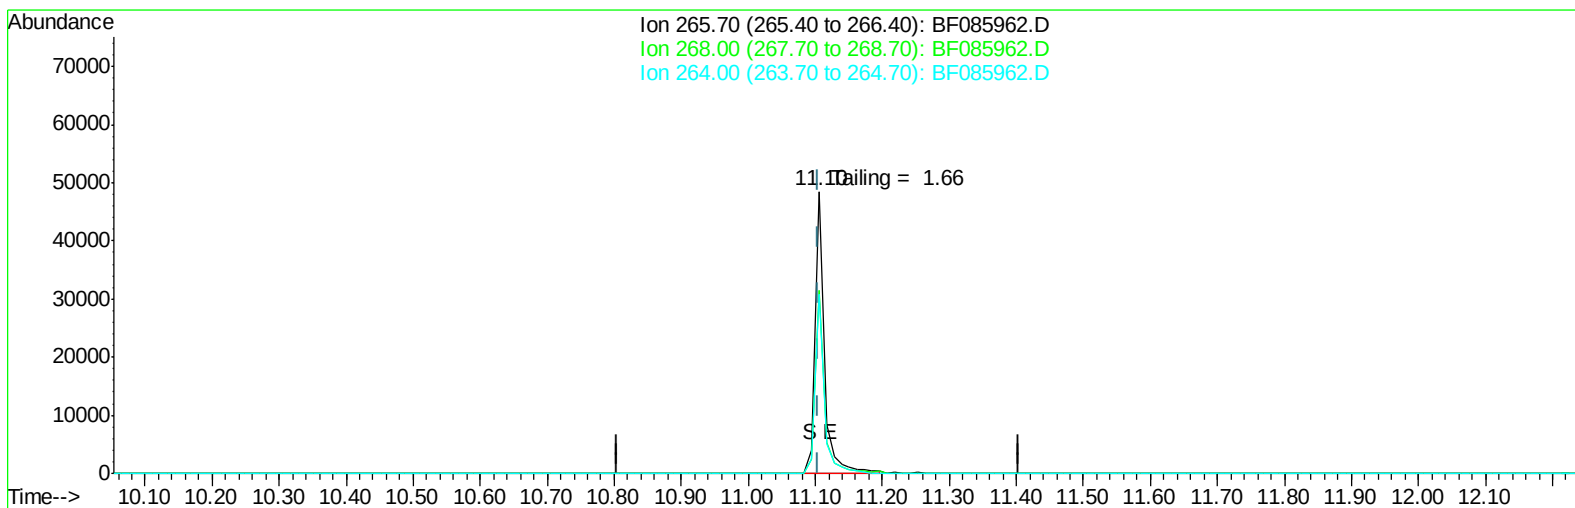

TIC: BF085962.D

(69) Pentachlorophenol (C)

11.105min (+0.000) 0.00ng

response 47055

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.95
264.00	63.30	63.48
0.00	0.00	0.00

