
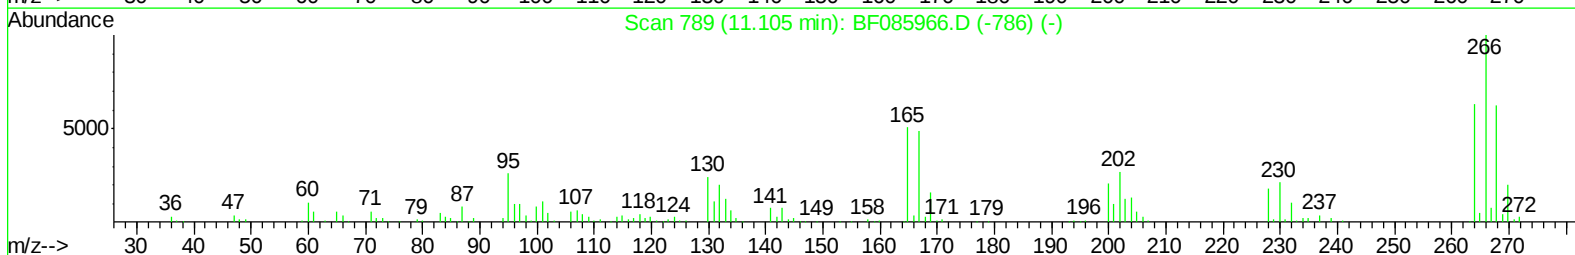
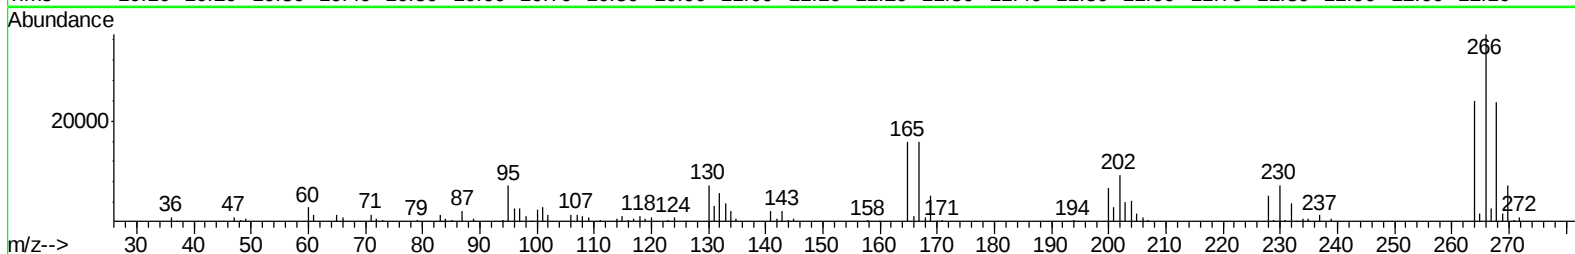


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040216\
Data File : BF085971.D
Acq On : 1 Apr 2016 19:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 05:39:11 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

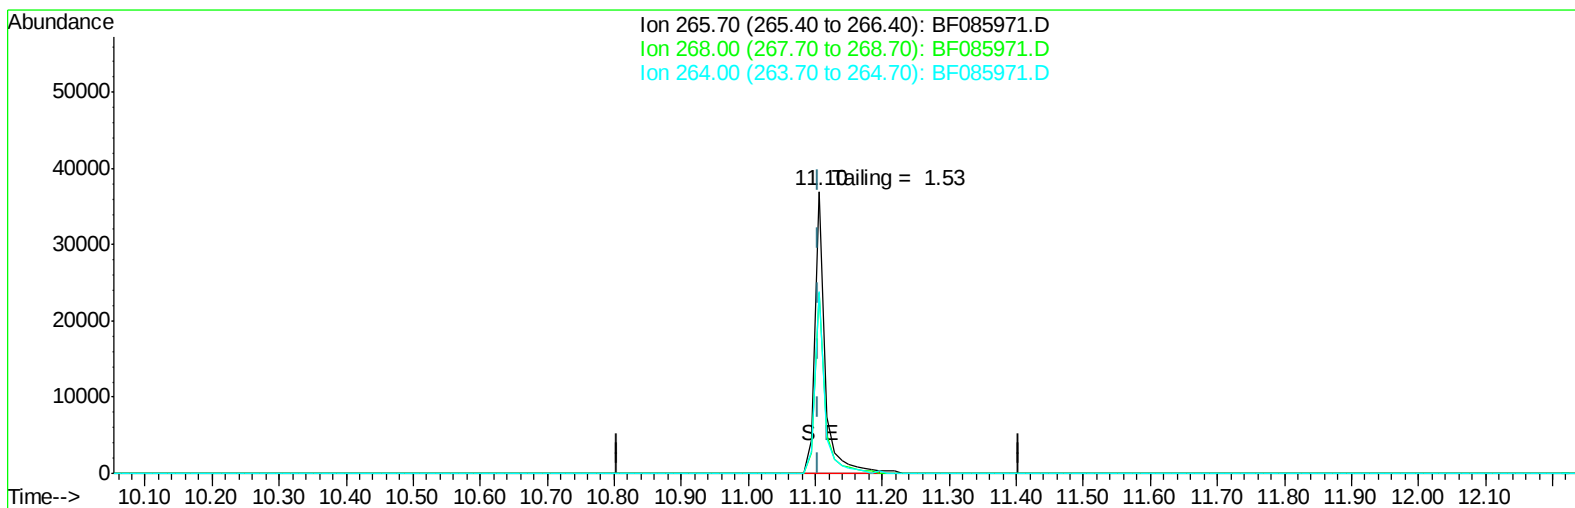

TIC: BF085971.D

(69) Pentachlorophenol (C)




11.105min (+0.000) 0.00ng

response 39412

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.23
264.00	63.30	64.49
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040216\
Data File : BF085971.D
Acq On : 1 Apr 2016 19:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 05:39:11 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

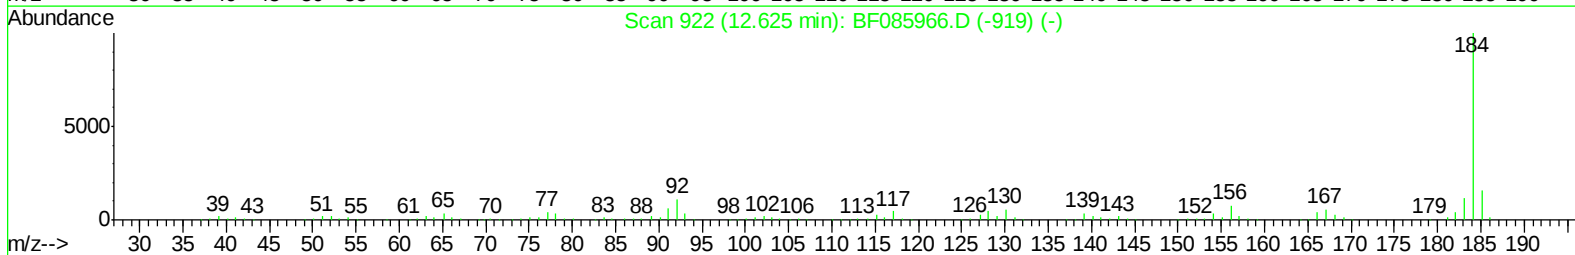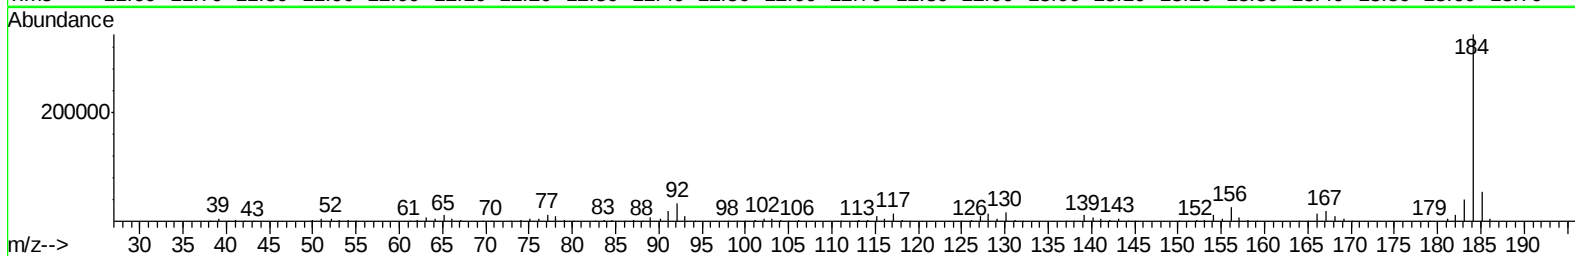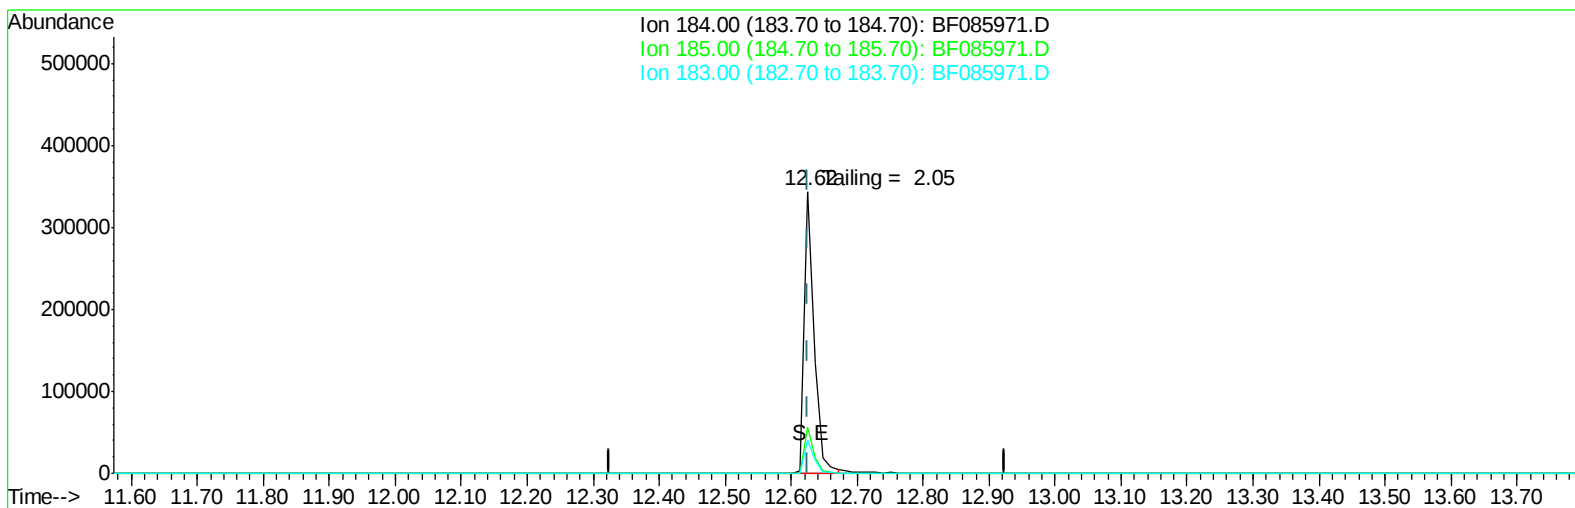

TIC: BF085971.D

(76) Benzidine

12.625min (+0.000) 0.00ng

response 361099

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	16.16
183.00	11.80	11.71
0.00	0.00	0.00