
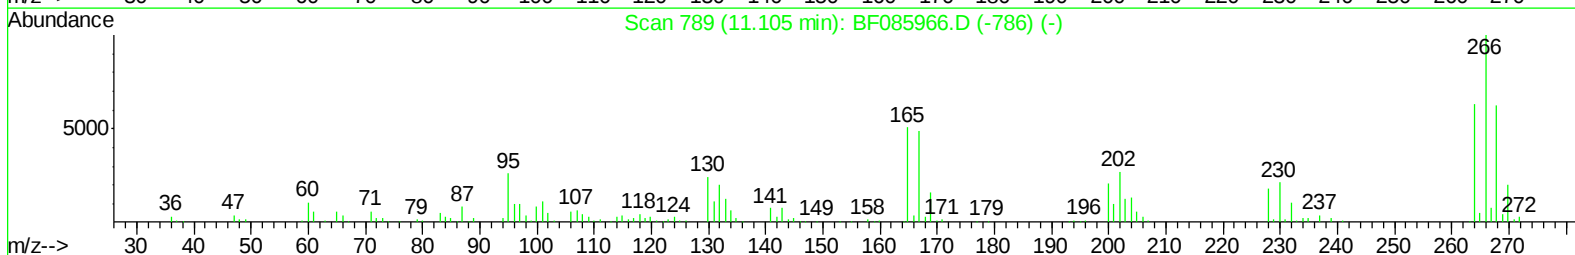
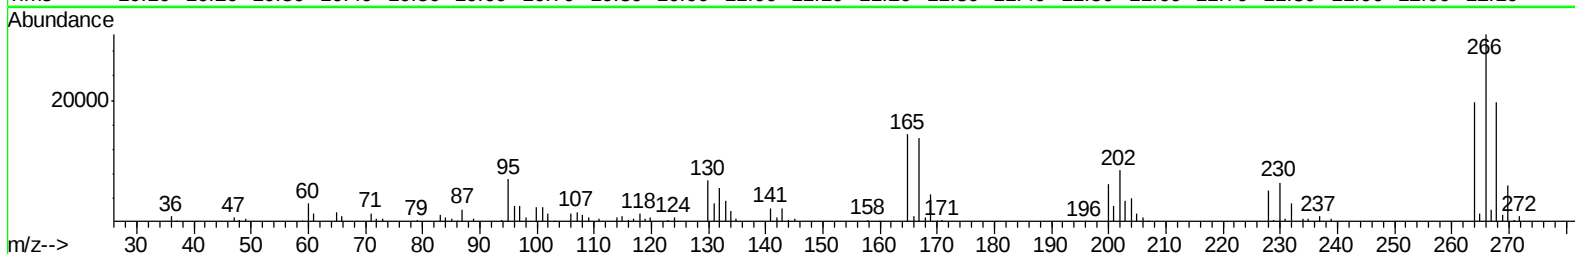


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040216\
Data File : BF086023.D
Acq On : 2 Apr 2016 20:40
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 05:33:08 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

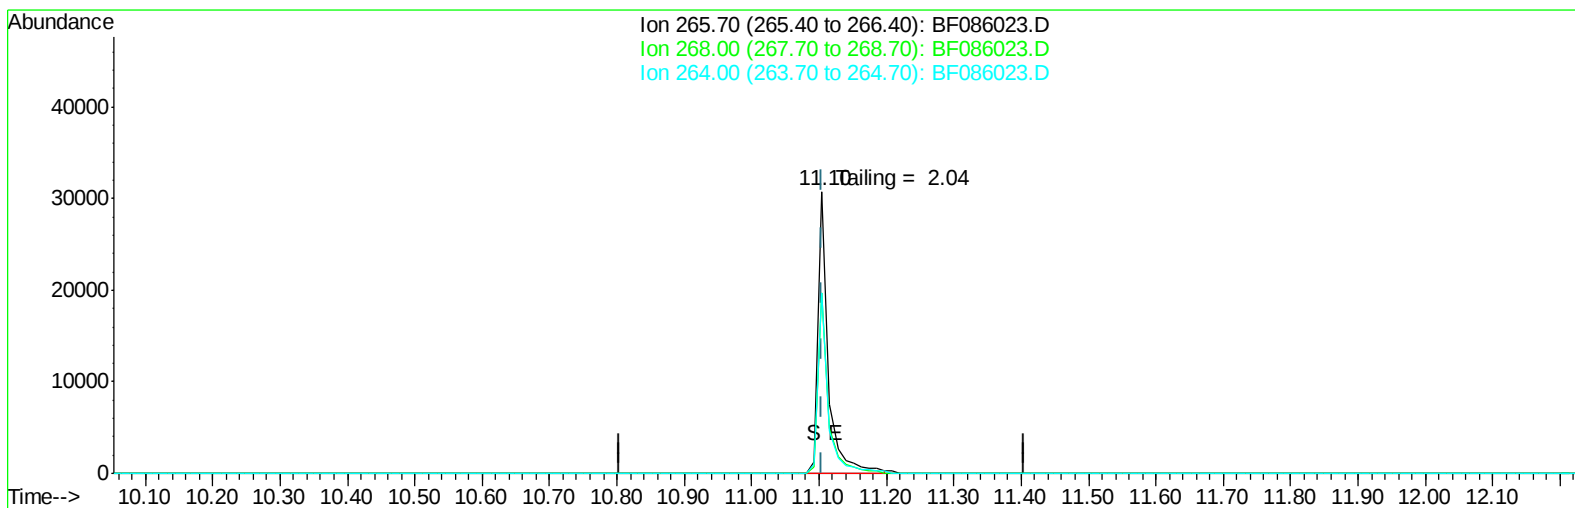

TIC: BF086023.D

(69) Pentachlorophenol (C)




11.105min (+0.000) 0.00ng

response 32385

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.22
264.00	63.30	63.93
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040216\
Data File : BF086023.D
Acq On : 2 Apr 2016 20:40
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 05:33:08 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

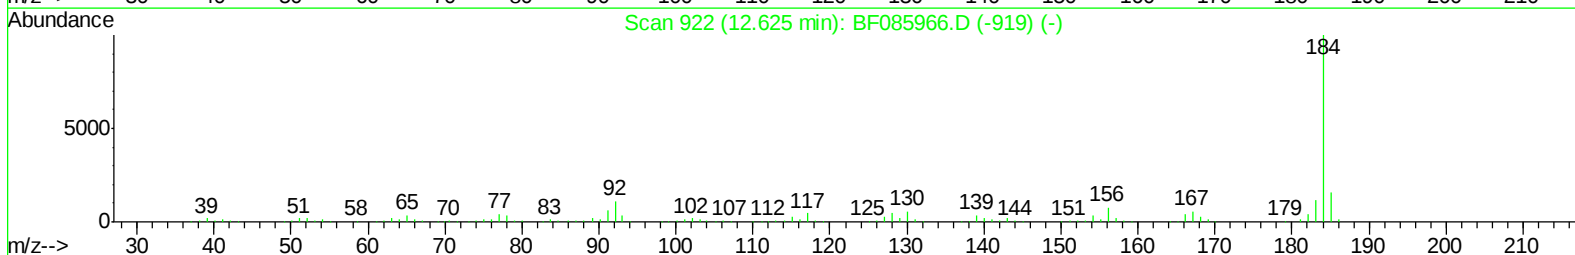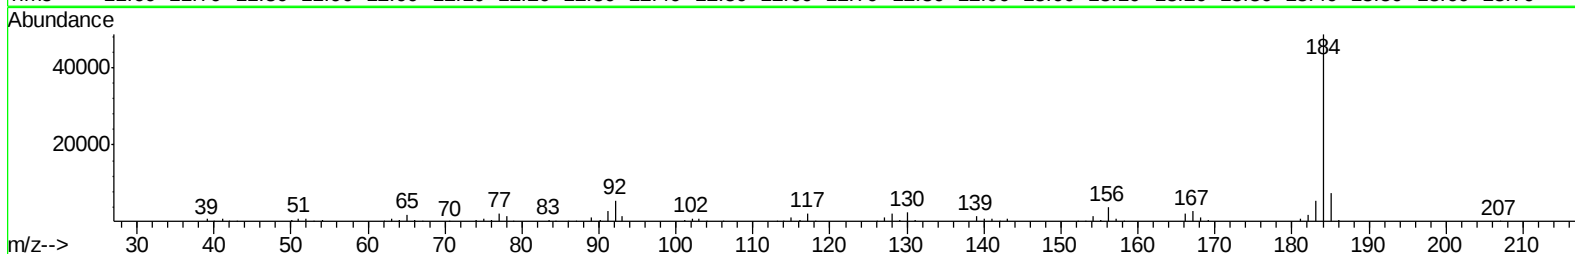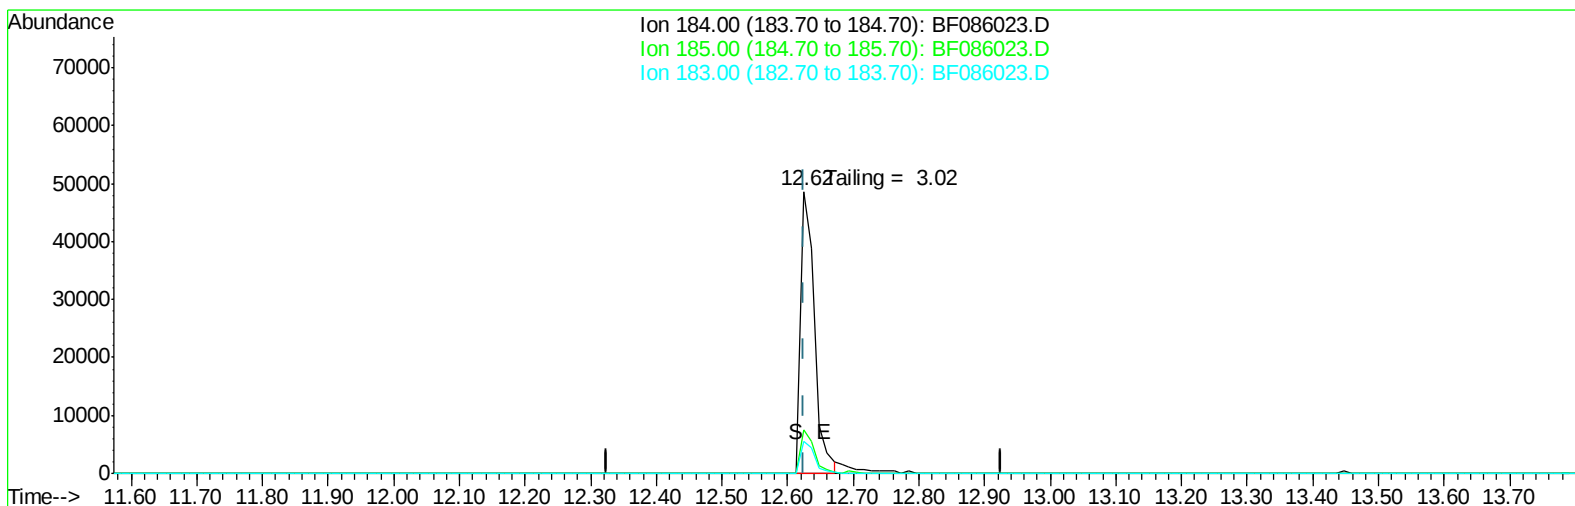

TIC: BF086023.D

(76) Benzidine

12.625min (+0.000) 0.00ng m

response 69502

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	15.29
183.00	11.80	11.45
0.00	0.00	0.00