

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040216\
 Data File : BF086025.D
 Acq On : 2 Apr 2016 21:36
 Operator : UM/SJ
 Sample : PB89347BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB89347BL

Quant Time: Apr 04 03:59:45 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 01 23:17:06 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.77	152	111756	20.00	ng	0.00
21) Naphthalene-d8	8.05	136	429516	20.00	ng	-0.01
38) Acenaphthene-d10	9.81	164	188322	20.00	ng	0.00
63) Phenanthrene-d10	11.29	188	361799	20.00	ng	-0.01
75) Chrysene-d12	13.93	240	235830	20.00	ng	0.00
86) Perylene-d12	15.33	264	208571	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.38	112	842483	128.86	ng	0.01
7) Phenol-d6	6.42	99	943918	113.66	ng	0.00
23) Nitrobenzene-d5	7.34	82	671532	92.20	ng	0.00
41) 2,4,6-Tribromophenol	10.60	330	251903	142.51	ng	0.00
44) 2-Fluorobiphenyl	9.14	172	1128571	99.64	ng	0.00
78) Terphenyl-d14	12.88	244	926624	92.36	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040216\
Data File : BF086025.D
Acq On : 2 Apr 2016 21:36
Operator : UM/SJ
Sample : PB89347BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB89347BL

Quant Time: Apr 04 03:59:45 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

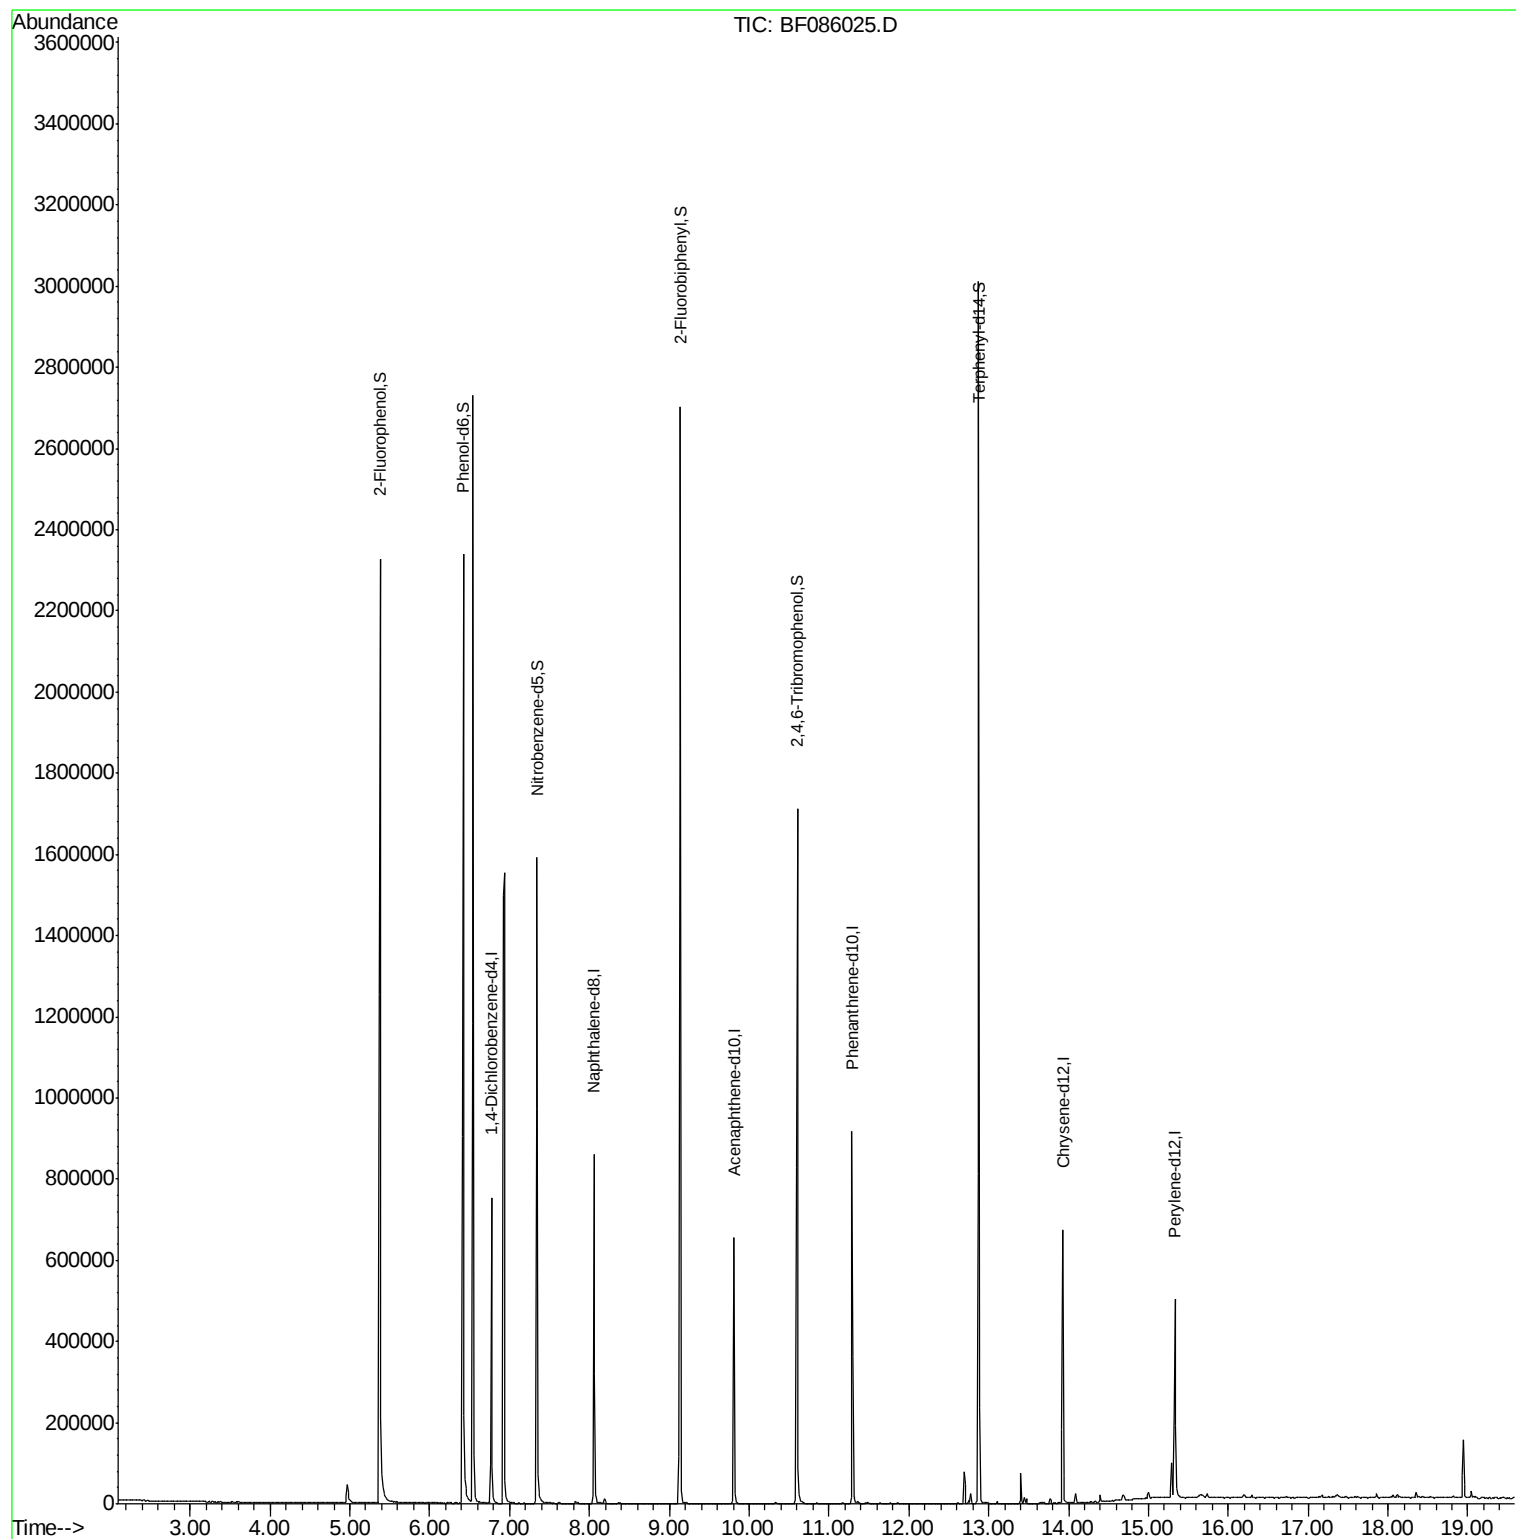

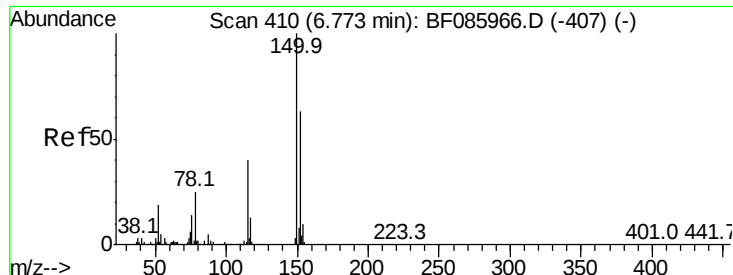

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.77 min Scan# 410

Delta R.T. 0.00 min

Lab File: BF086025.D

Acq: 2 Apr 2016 21:36

Instrument :

BNA_F

ClientSampleId :

PB89347BL




Tot Ion:152 Resp: 111756

Ion Ratio Lower Upper

152 100

150 158.6 124.2 186.2

115 61.6 47.0 70.6

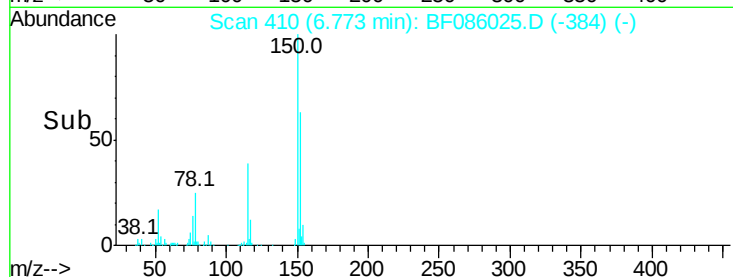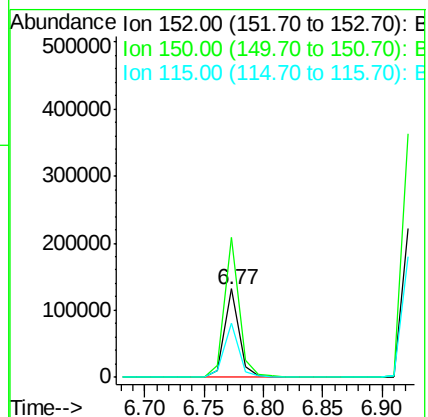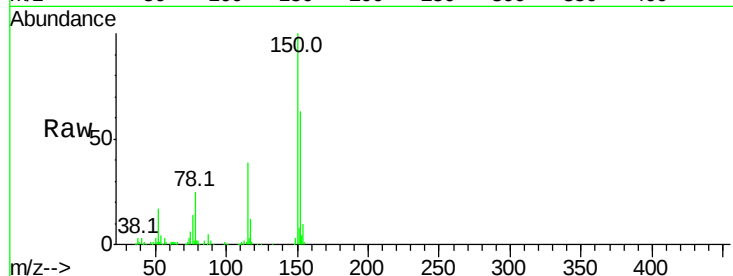

#5

2-Fluorophenol

Concen: 128.86 ng

RT: 5.38 min Scan# 288

Delta R.T. 0.01 min

Lab File: BF086025.D

Acq: 2 Apr 2016 21:36




Tgt Ion:112 Resp: 842483

Ion Ratio Lower Upper

112 100

64 49.9 39.9 59.9

63 25.3 20.2 30.2

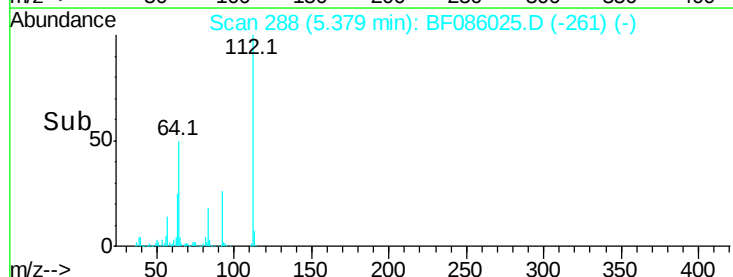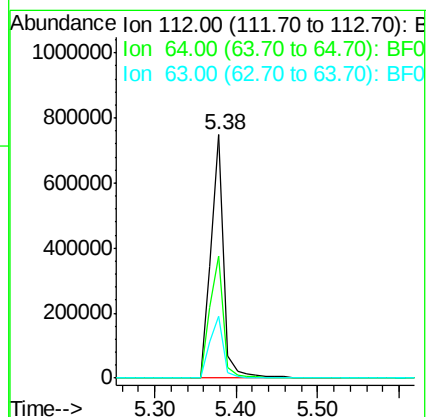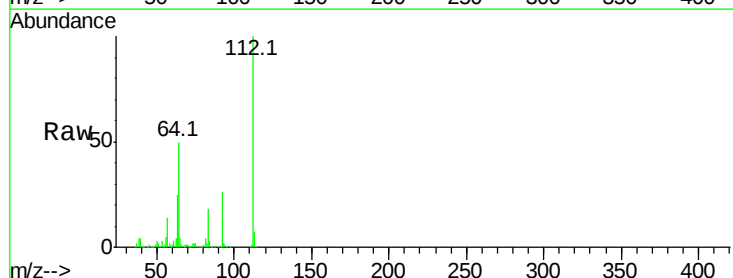



#7

Phenol-d6

Concen: 113.66 ng

RT: 6.42 min Scan# 379

Delta R.T. 0.00 min

Lab File: BF086025.D

Acq: 2 Apr 2016 21:36

Instrument :

BNA_F

ClientSampleId :

PB89347BL


Tot Ion: 99 Resp: 943918

Ion Ratio Lower Upper




99 100

42 15.1 11.1 16.7

71 33.1 24.9 37.3

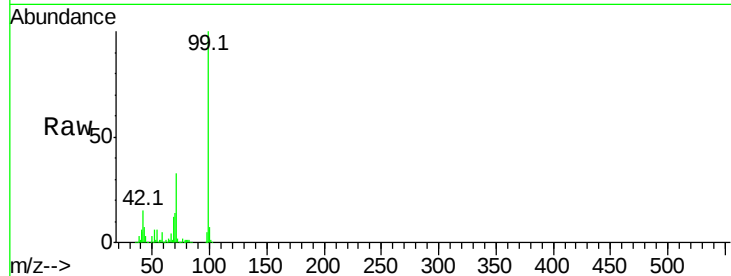

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

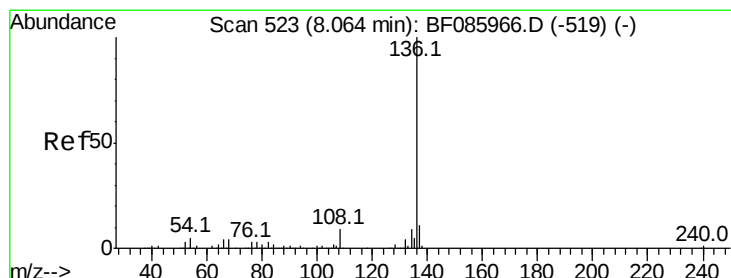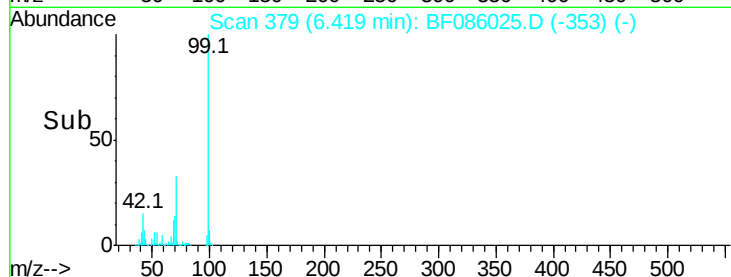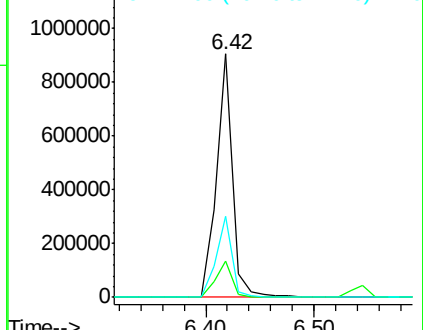

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.05 min Scan# 522

Delta R.T. -0.01 min

Lab File: BF086025.D

Acq: 2 Apr 2016 21:36

Tgt Ion: 136 Resp: 429516


Ion Ratio Lower Upper

136 100



137 11.4 9.1 13.7

54 8.2 7.4 11.0

68 6.7 5.8 8.8

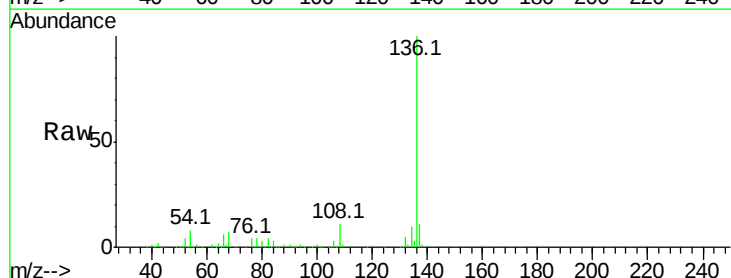

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

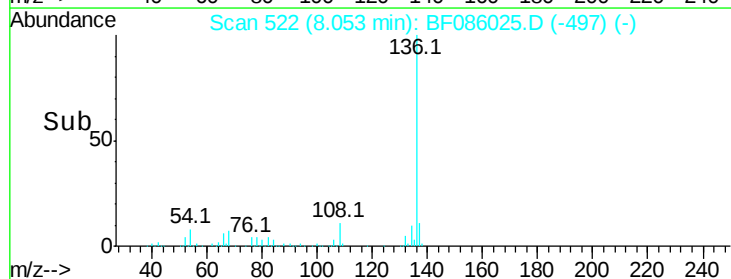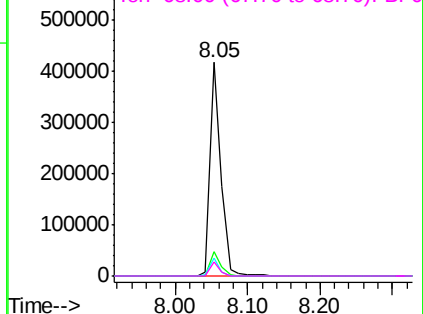







#23
 Nitrobenzene-d5
 Concen: 92.20 ng
 RT: 7.34 min Scan# 460
 Delta R.T. 0.00 min
 Lab File: BF086025.D
 Acq: 2 Apr 2016 21:36

Instrument :
 BNA_F
 ClientSampleID :
 PB89347BL

Tot Ion: 82 Resp: 671532
 Ion Ratio Lower Upper
 82 100
 128 51.1 41.8 62.8
 54 42.2 33.4 50.0

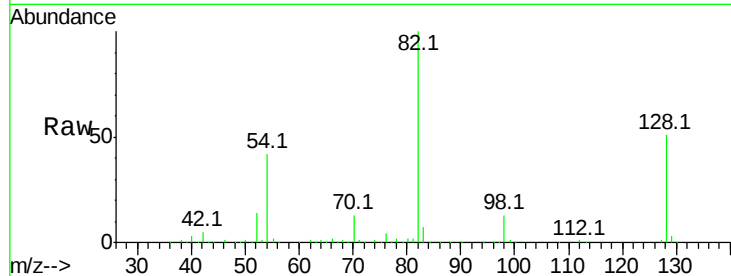


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

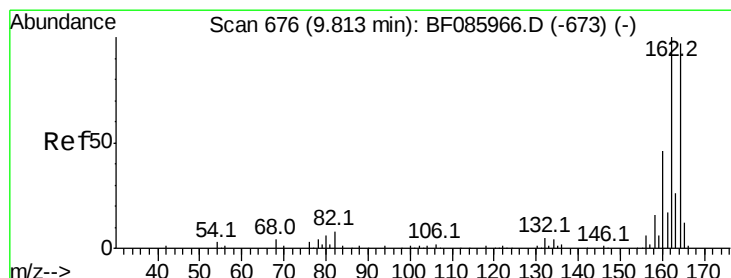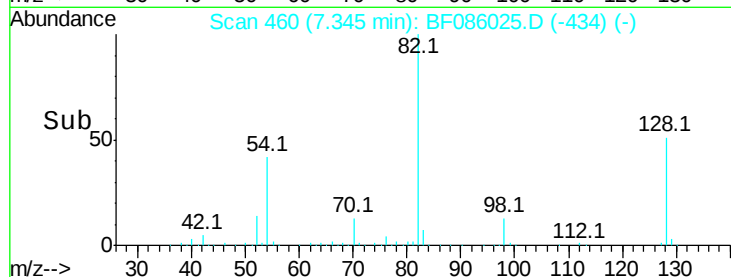
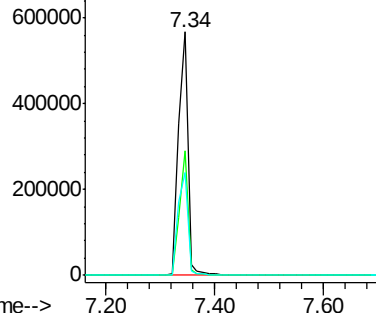



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.81 min Scan# 676
 Delta R.T. 0.00 min
 Lab File: BF086025.D
 Acq: 2 Apr 2016 21:36

Tgt Ion:164 Resp: 188322
 Ion Ratio Lower Upper
 164 100
 162 106.5 82.1 123.1
 160 50.0 37.4 56.2

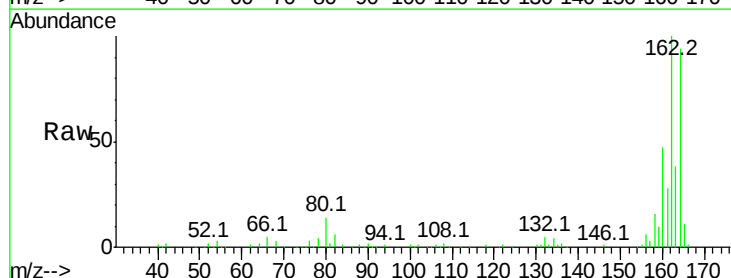

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

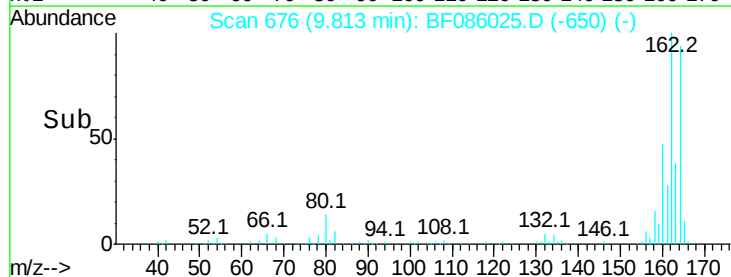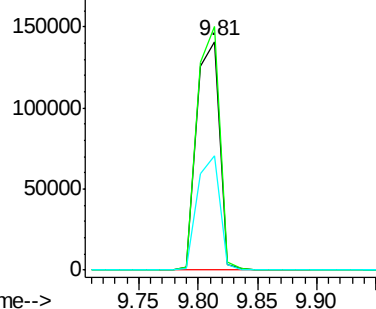


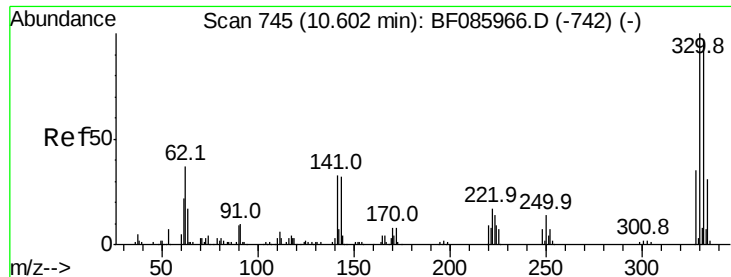



#41
 2,4,6-Tribromophenol
 Concen: 142.51 ng
 RT: 10.60 min Scan# 745
 Delta R.T. 0.00 min
 Lab File: BF086025.D
 Acq: 2 Apr 2016 21:36

Instrument :
 BNA_F
 ClientSampleId :
 PB89347BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.9	78.2	117.2
141	33.7	31.5	47.3

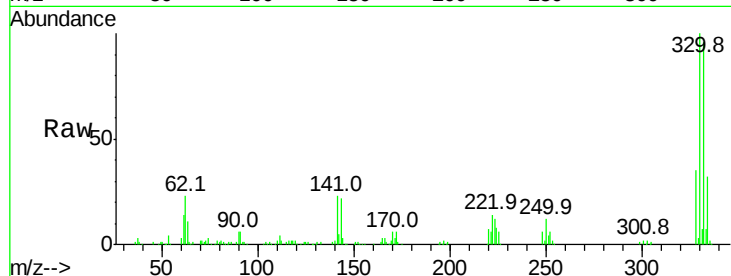


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

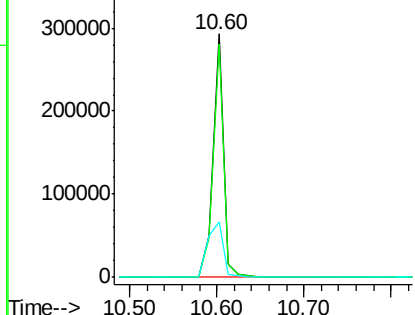
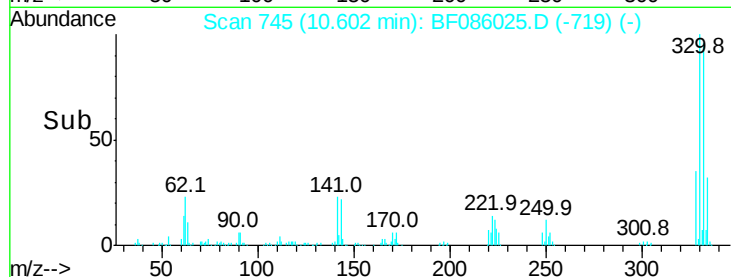



#44
 2-Fluorobiphenyl
 Concen: 99.64 ng
 RT: 9.14 min Scan# 617
 Delta R.T. 0.00 min
 Lab File: BF086025.D
 Acq: 2 Apr 2016 21:36

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	29.4	44.2
170	24.3	19.8	29.6

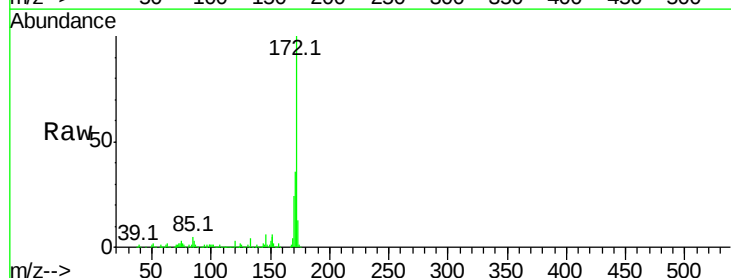

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

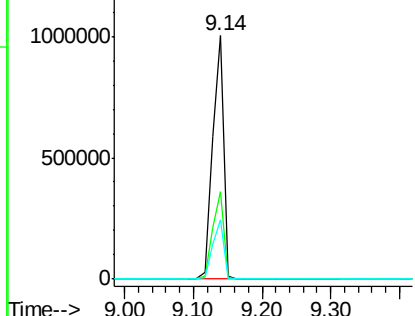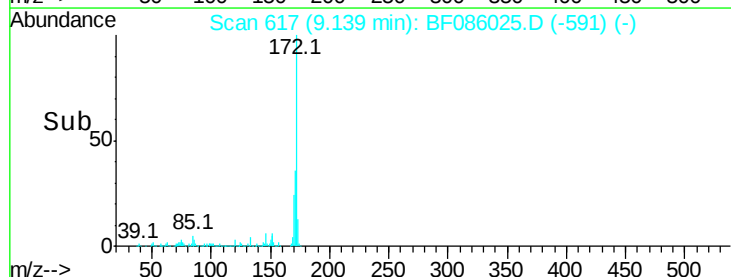


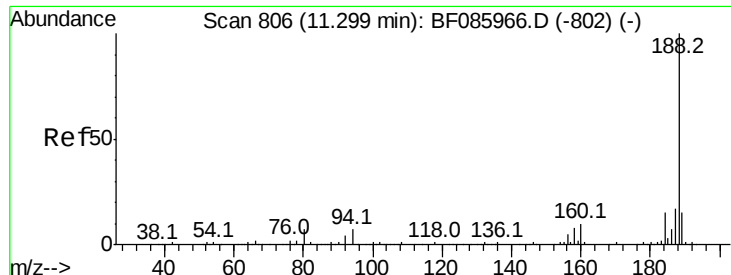




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.29 min Scan# 805
 Delta R.T. -0.01 min
 Lab File: BF086025.D
 Acq: 2 Apr 2016 21:36

Instrument :
 BNA_F
 ClientSampleId :
 PB89347BL

Tot Ion:188 Resp: 361799
 Ion Ratio Lower Upper
 188 100
 94 12.0 5.4 8.0#
 80 13.3 5.5 8.3#

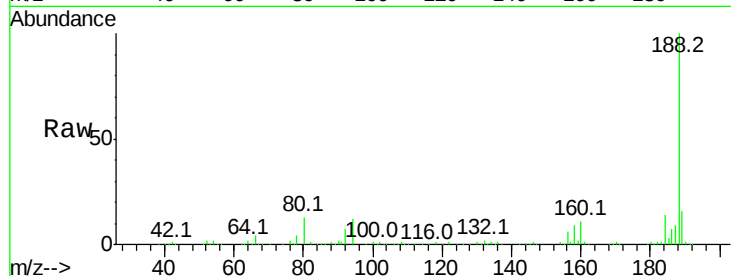


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

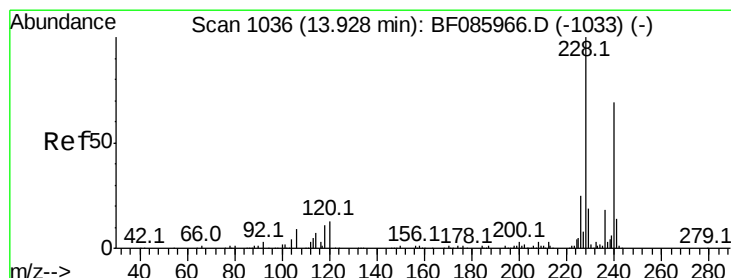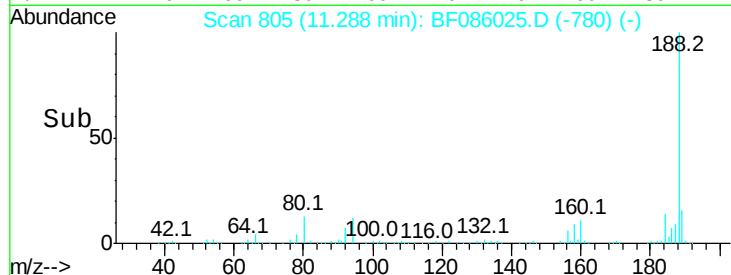
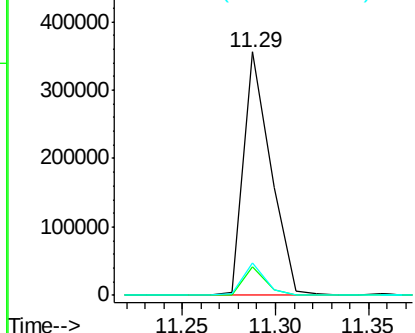



#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 13.93 min Scan# 1036
 Delta R.T. 0.00 min
 Lab File: BF086025.D
 Acq: 2 Apr 2016 21:36

Tgt Ion:240 Resp: 235830
 Ion Ratio Lower Upper
 240 100
 120 10.5 13.8 20.8#
 236 26.7 20.6 30.8

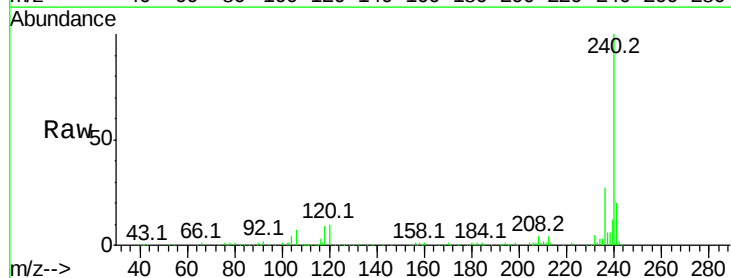

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E



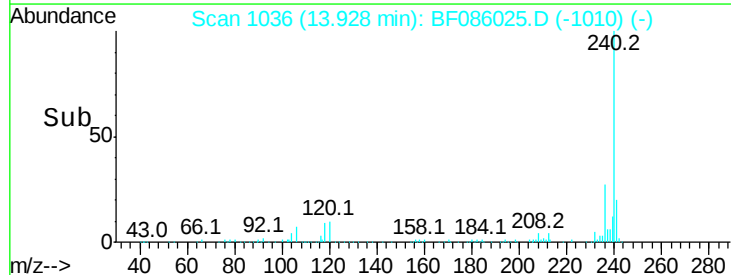
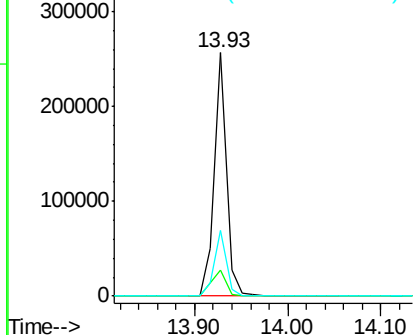


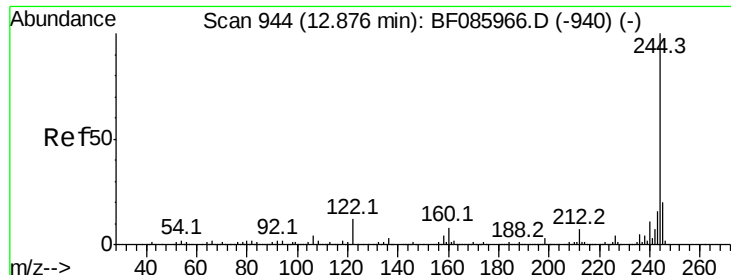

#78
 Terphenyl-d14
 Concen: 92.36 ng
 RT: 12.88 min Scan# 944
 Delta R.T. 0.00 min
 Lab File: BF086025.D
 Acq: 2 Apr 2016 21:36

Instrument :
 BNA_F
 ClientSampleID :
 PB89347BL

Tot Ion:244 Resp: 926624
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.1 9.1
 122 11.7 10.2 15.4

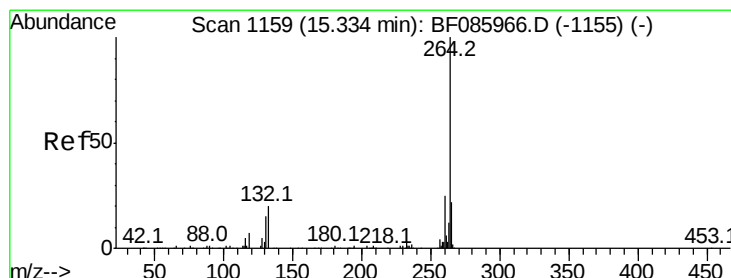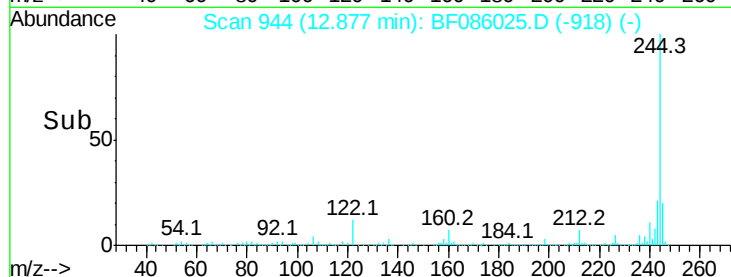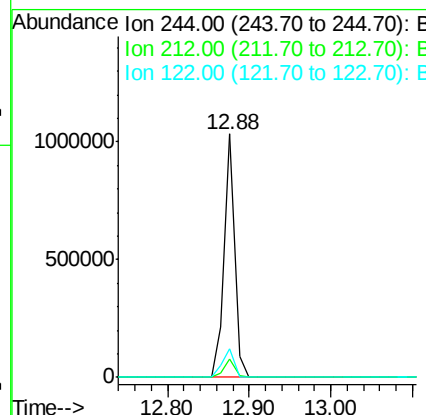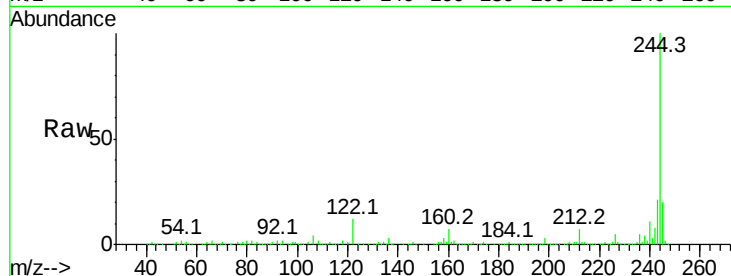

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.33 min Scan# 1159
 Delta R.T. 0.00 min
 Lab File: BF086025.D
 Acq: 2 Apr 2016 21:36

Tgt Ion:264 Resp: 208571
 Ion Ratio Lower Upper
 264 100
 260 24.9 19.4 29.2
 265 21.5 17.2 25.8

