

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040216\
 Data File : BF085977.D
 Acq On : 1 Apr 2016 22:43
 Operator : UM/SJ
 Sample : PB89314BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB89314BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.967	250	252	265	rBV	30901	54126	1.77%	0.249%
2	5.367	285	287	290	rBV	1578981	2016284	66.07%	9.261%
3	6.407	376	378	381	rBV	1586149	2050045	67.18%	9.416%
4	6.544	387	390	392	rBV	1794772	2271474	74.43%	10.433%
5	6.773	408	410	421	rBB	655143	589113	19.30%	2.706%
6	6.922	421	423	426	rBV	1479965	1770220	58.01%	8.131%
7	7.333	457	459	462	rBV	967895	1390491	45.56%	6.387%
8	8.053	520	522	525	rBV	788575	800215	26.22%	3.676%
9	9.128	614	616	619	rBV	2045711	2654640	86.99%	12.193%
10	9.802	673	675	678	rBV	688534	863933	28.31%	3.968%
11	10.602	742	745	747	rBV2	1271620	1644428	53.88%	7.553%
12	11.288	803	805	808	rBV	1047213	959628	31.45%	4.408%
13	12.876	941	944	946	rBV	3158193	3051759	100.00%	14.017%
14	13.928	1033	1036	1038	rBV	731679	885505	29.02%	4.067%
15	15.334	1156	1159	1167	rBV	510902	769480	25.21%	3.534%


Sum of corrected areas: 21771341

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040216\
Data File : BF085977.D
Acq On : 1 Apr 2016 22:43
Operator : UM/SJ
Sample : PB89314BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB89314BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

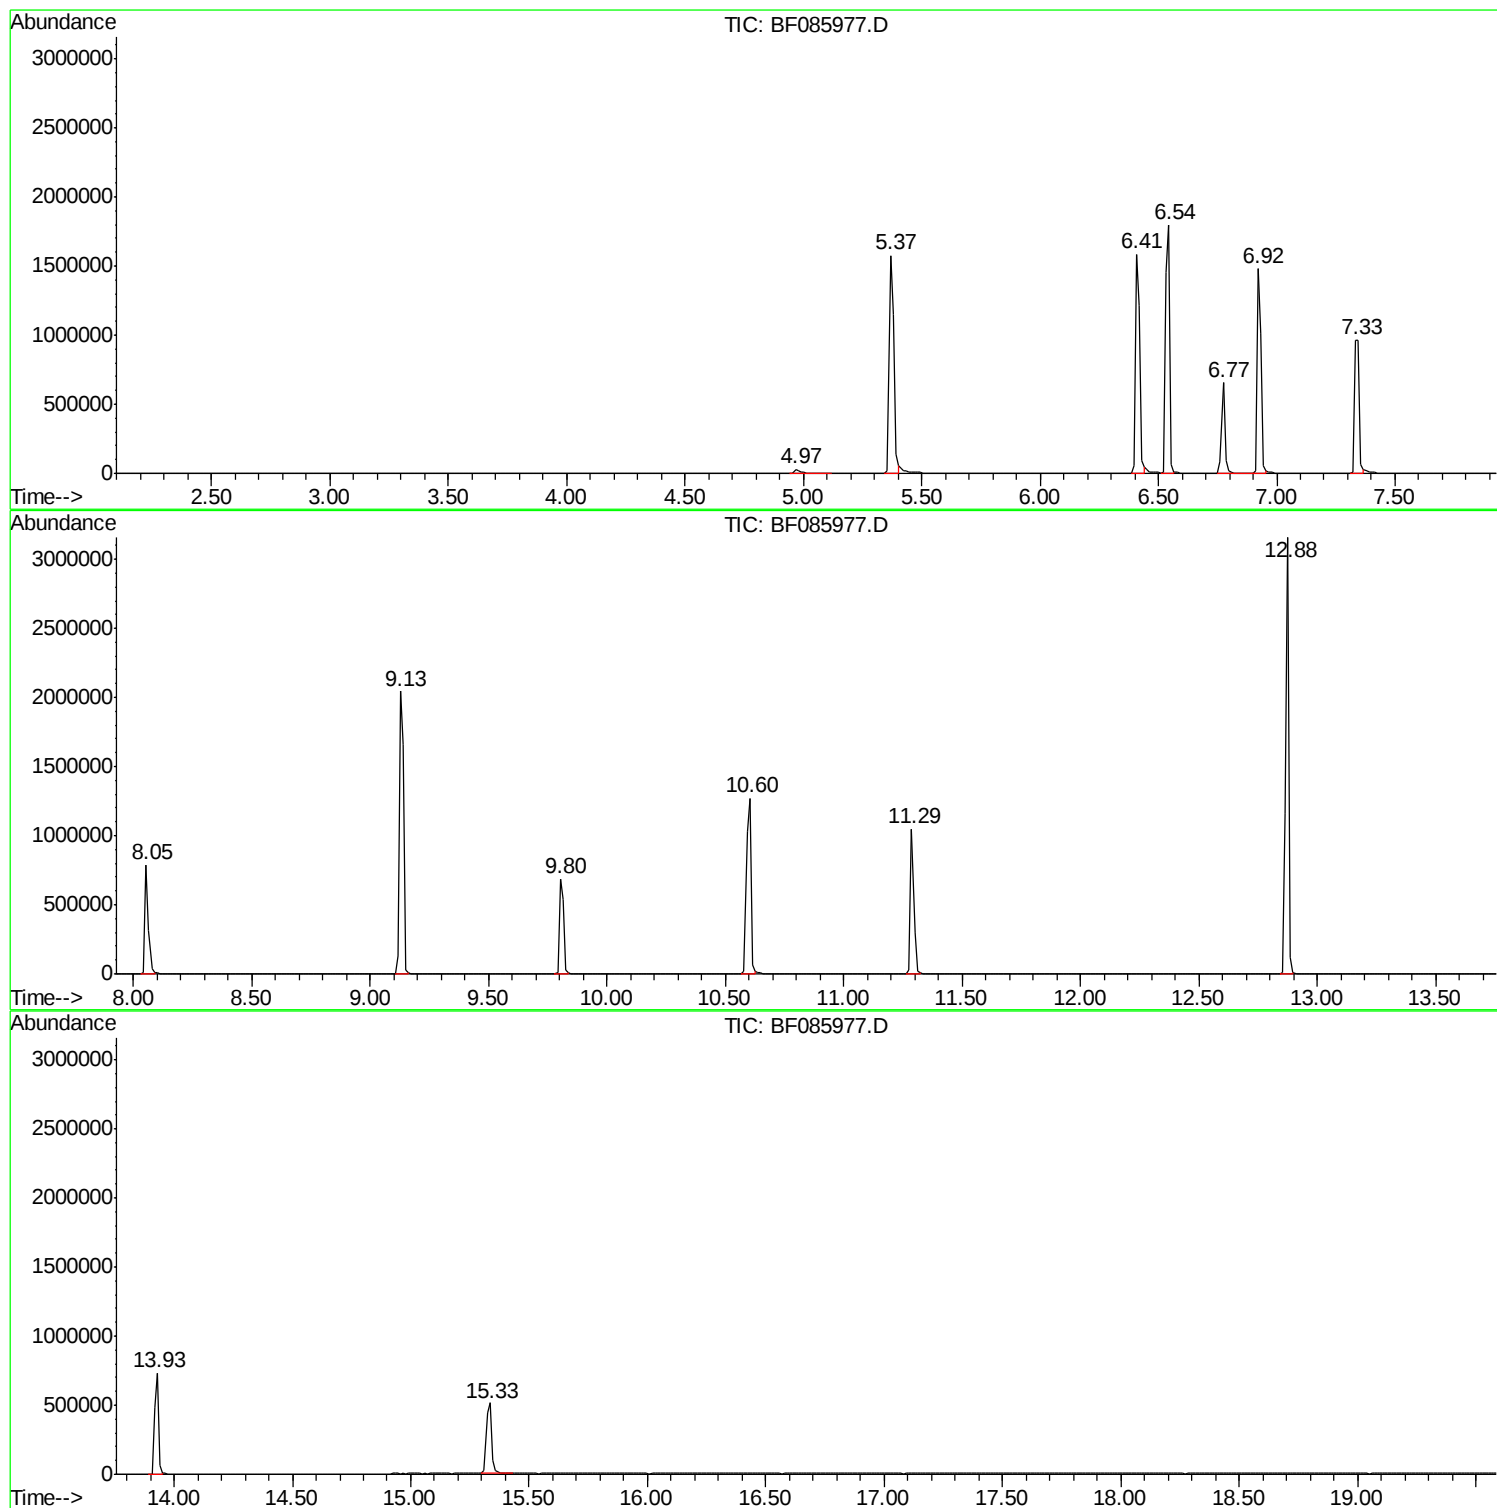

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040216\
Data File : BF085977.D
Acq On : 1 Apr 2016 22:43
Operator : UM/SJ
Sample : PB89314BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB89314BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.54 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.54	77.12 ng	2271470	1,4-Dichlorobenzene-d4	6.77

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		Xenon	132	Xe	007440-63-3	9

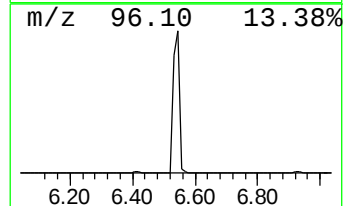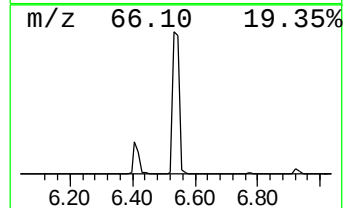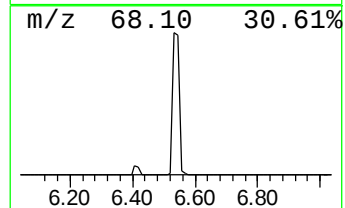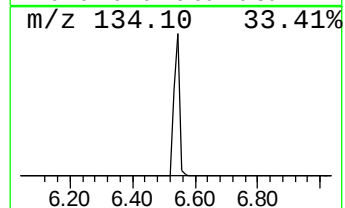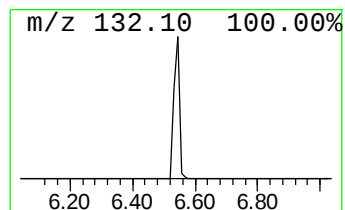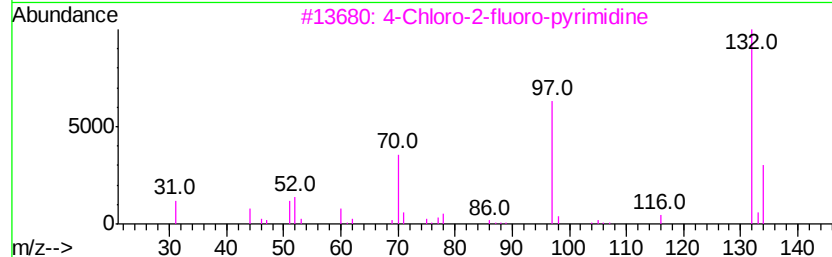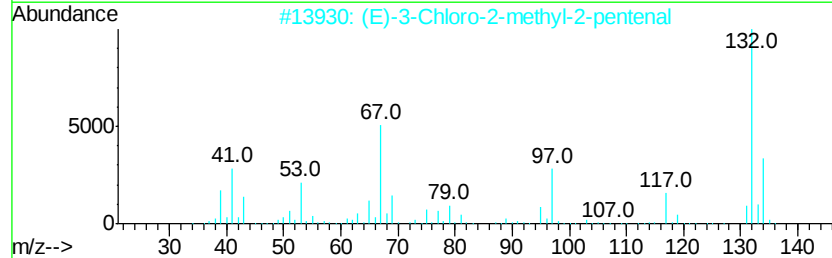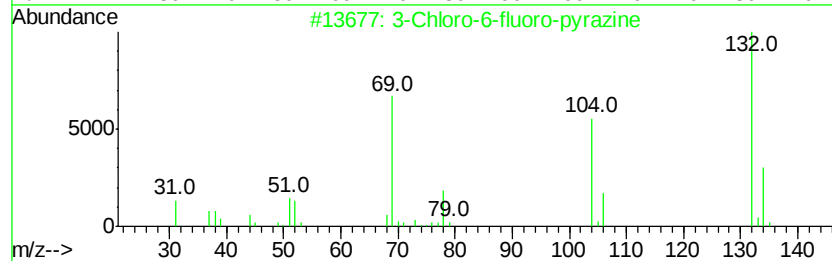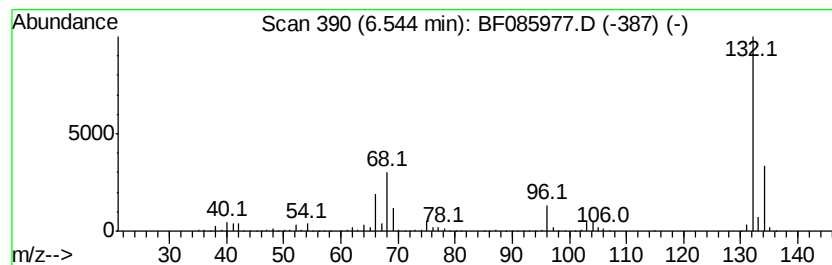

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040216\
Data File : BF085977.D
Acq On : 1 Apr 2016 22:43
Operator : UM/SJ
Sample : PB89314BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB89314BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.54	6.54	77.1	ng	2271470	1	6.77	589113	20.0