
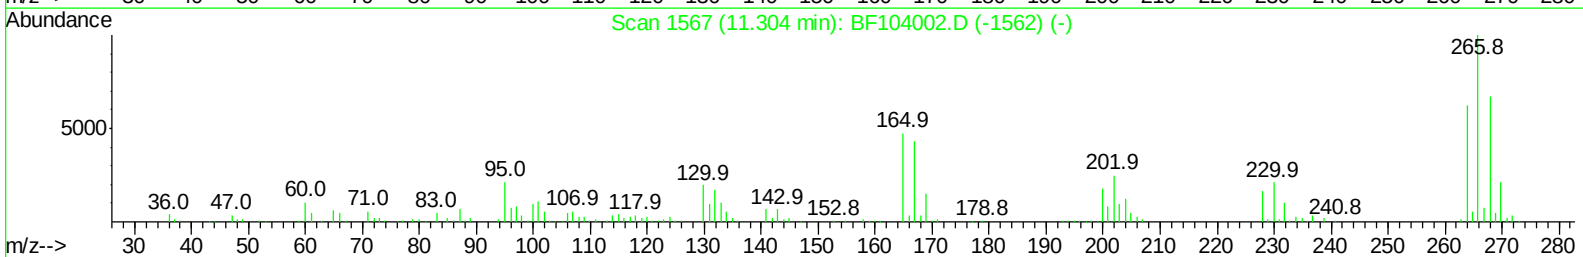
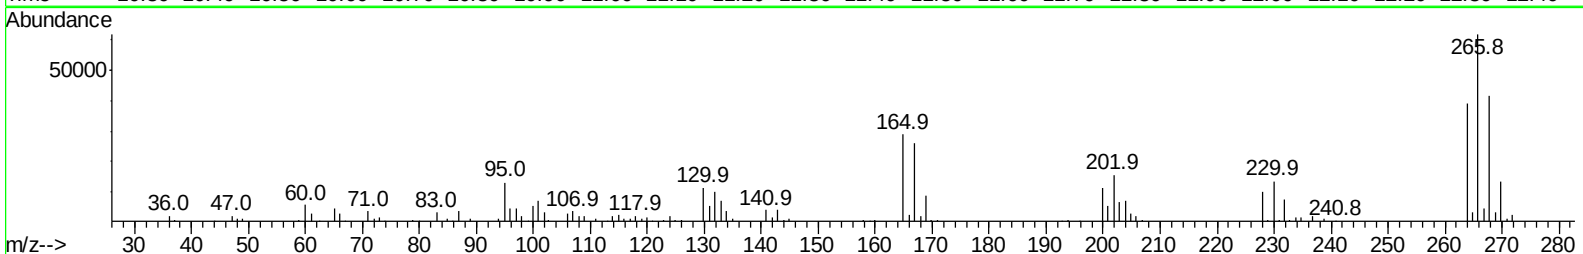


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF040218\  
Data File : BF104124.D  
Acq On : 2 Apr 2018 10:21  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 03:34:04 2018  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Apr 02 13:40:00 2018  
Response via : Initial Calibration

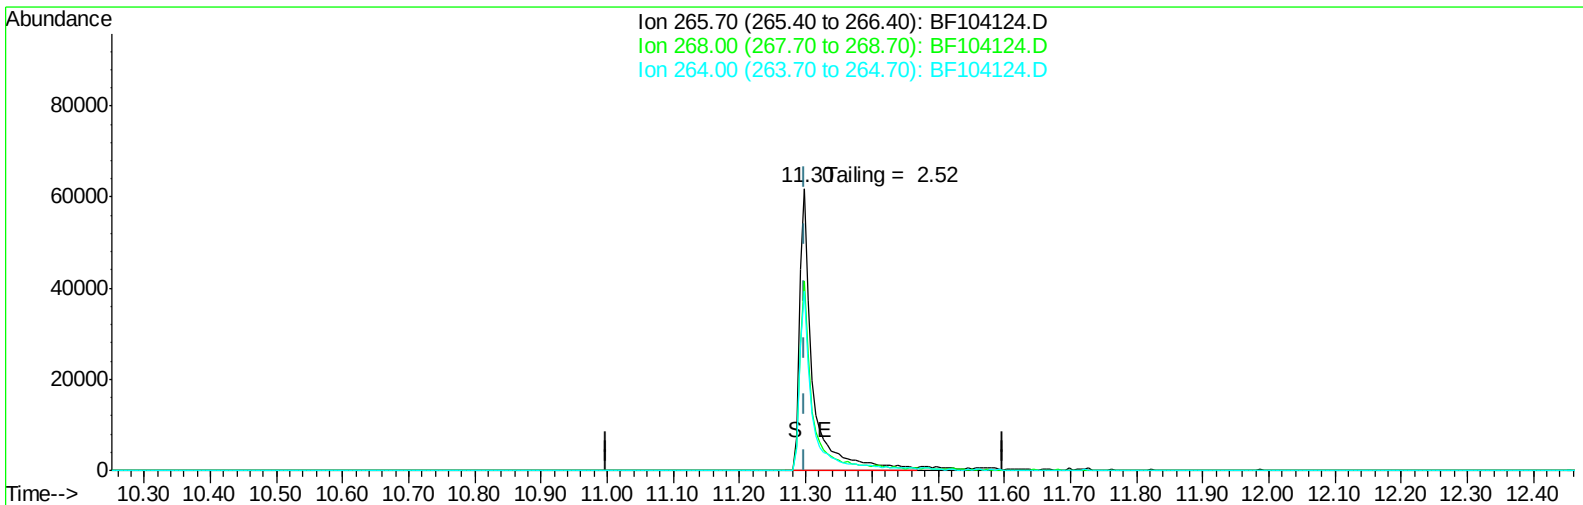

TIC: BF104124.D

(69) Pentachlorophenol (C)




11.298min (-0.000) 28558.62ng

response 85870

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 67.49 |
| 264.00 | 61.90 | 63.45 |
| 0.00   | 0.00  | 0.00  |

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF040218\  
 Data File : BF104124.D  
 Acq On : 2 Apr 2018 10:21  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 03:34:04 2018  
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Apr 02 13:40:00 2018  
 Response via : Initial Calibration

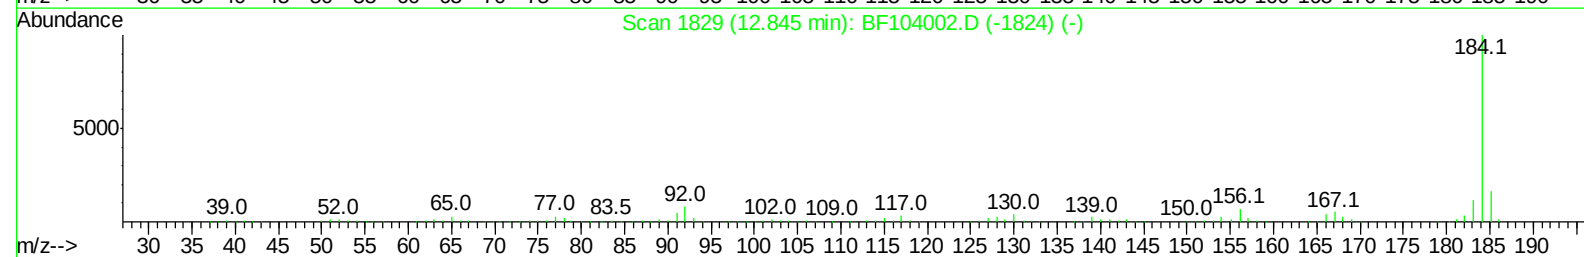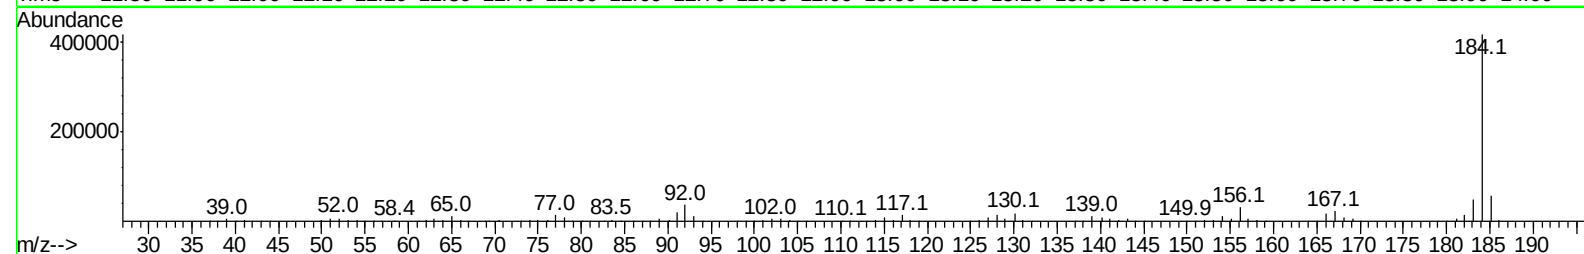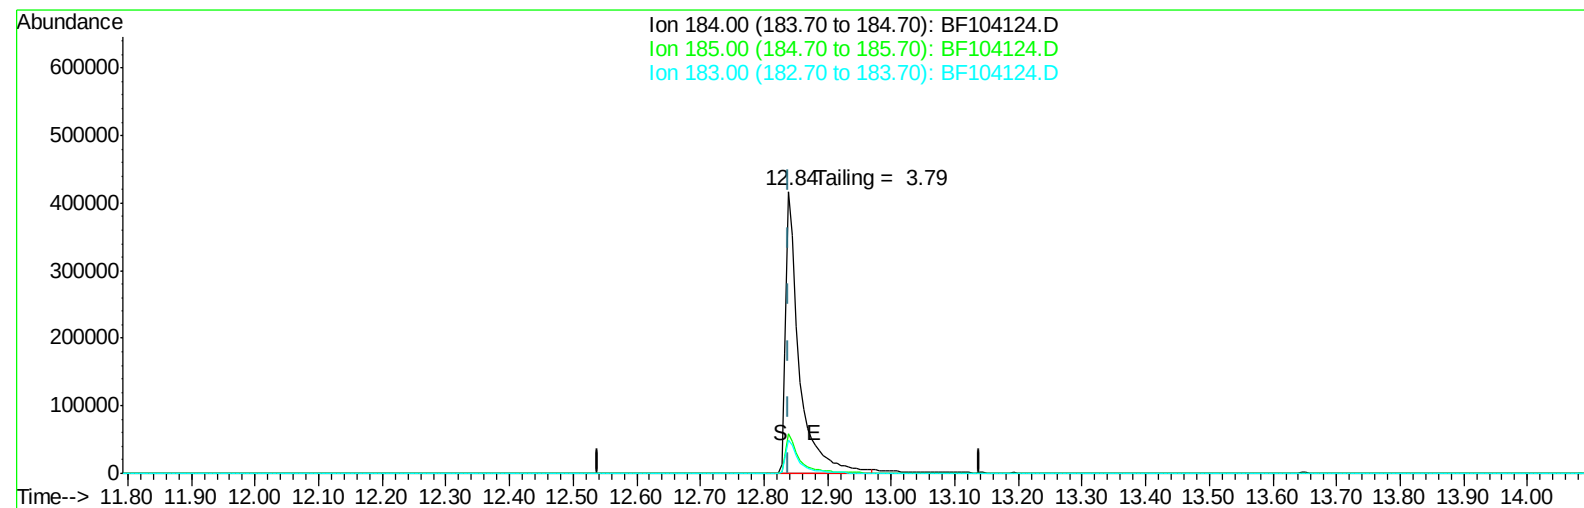

TIC: BF104124.D

(76) Benzidine

12.839min (-0.000) 0.00ng

response 641762

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 14.01 |
| 183.00 | 11.60 | 11.97 |
| 0.00   | 0.00  | 0.00  |