
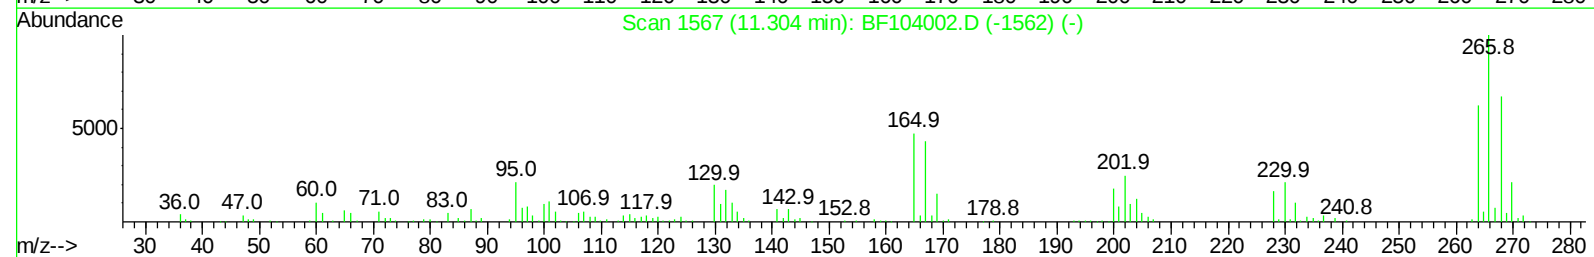
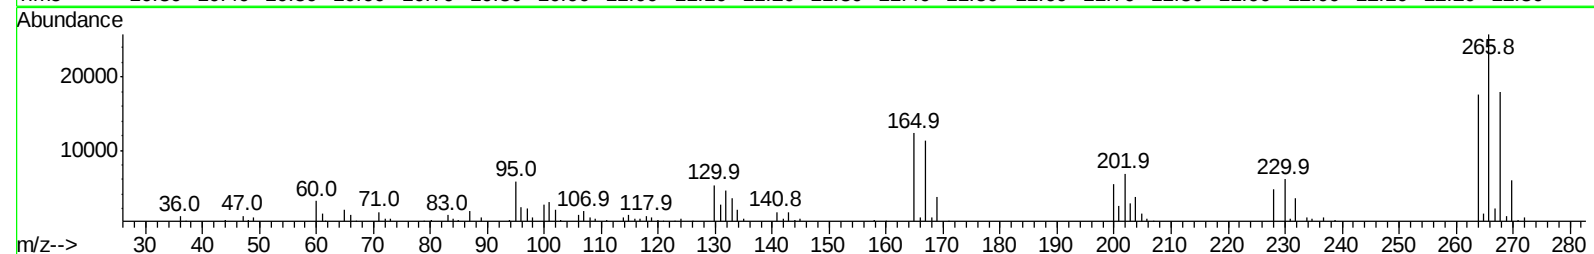


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF040218\
Data File : BF104151.D
Acq On : 2 Apr 2018 22:41
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 03:35:02 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 02 13:40:00 2018
Response via : Initial Calibration

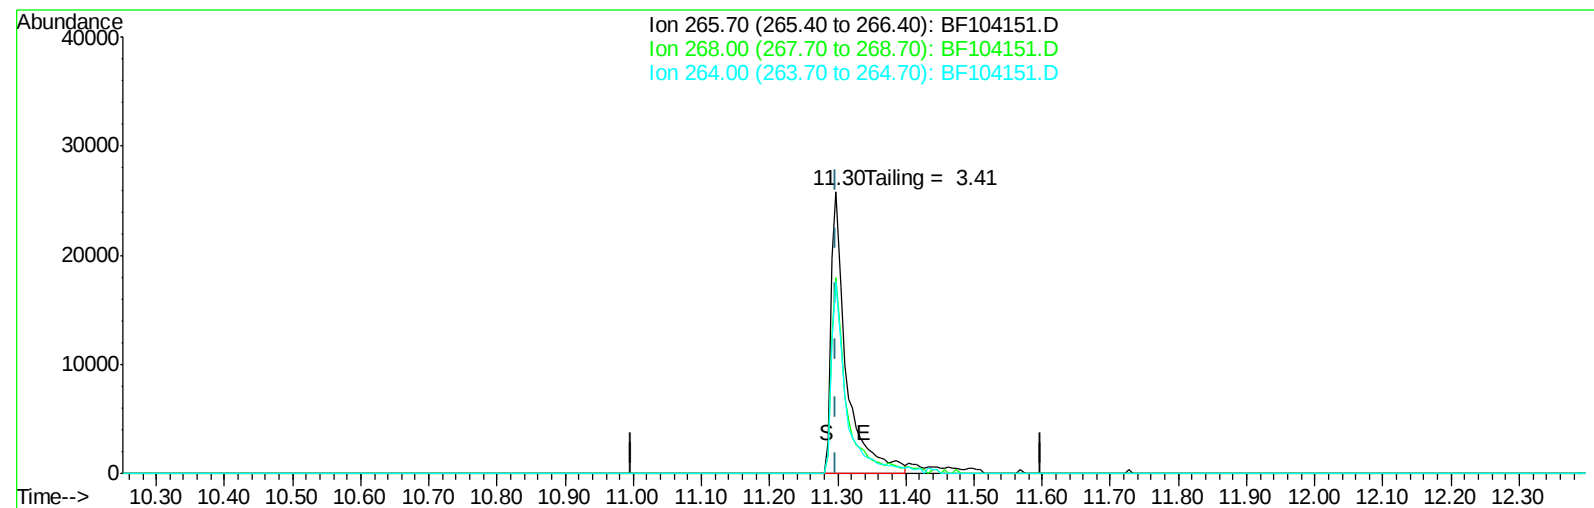

TIC: BF104151.D

(69) Pentachlorophenol (C)




11.298min (-0.000) 42524.40ng

response 39453

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	69.33
264.00	61.90	68.22
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF040218\
Data File : BF104151.D
Acq On : 2 Apr 2018 22:41
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 03:35:02 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 02 13:40:00 2018
Response via : Initial Calibration

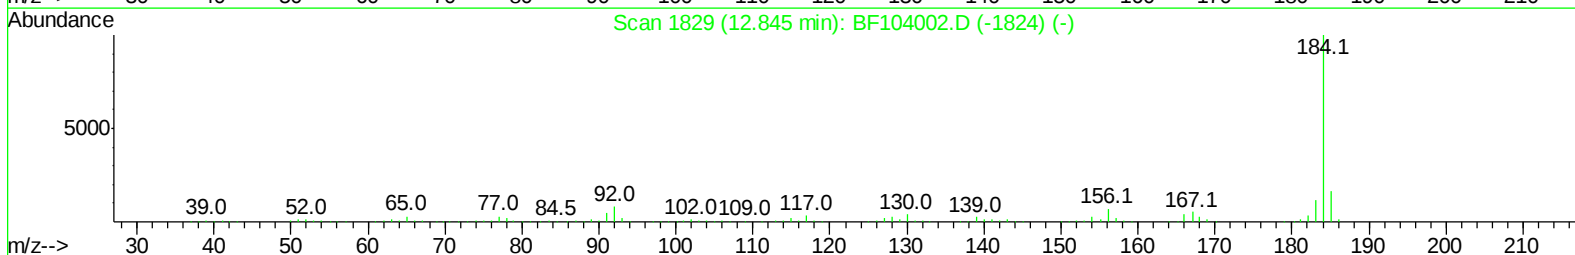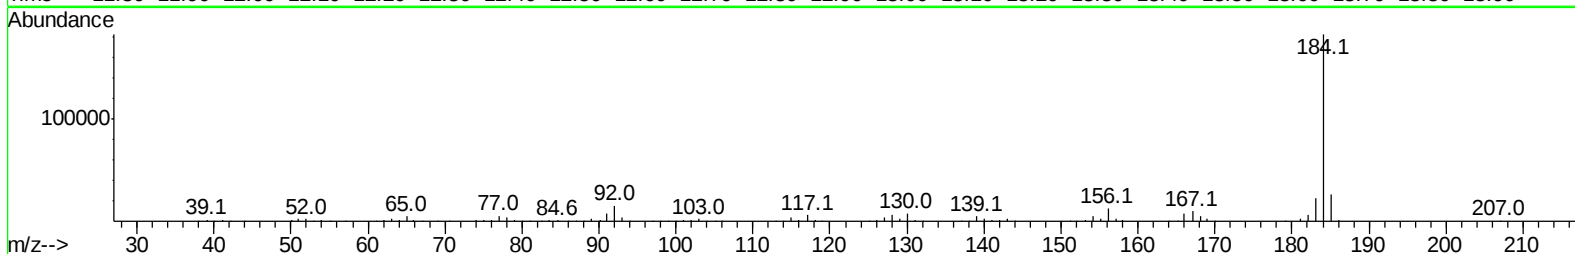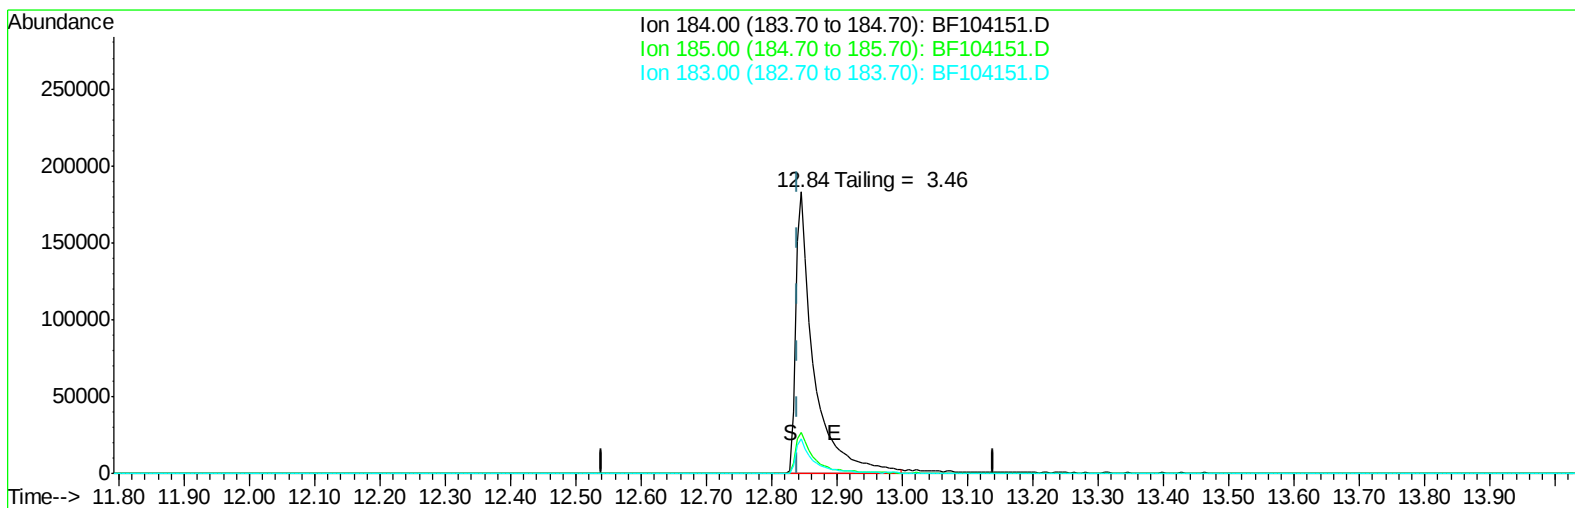

TIC: BF104151.D

(76) Benzidine

12.845min (+0.006) 0.00ng

response 354866

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.64
183.00	11.60	12.21
0.00	0.00	0.00