

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF040218\
 Data File : BF104132.D
 Acq On : 2 Apr 2018 13:56
 Operator : JU/SJ
 Sample : J2128-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EPE-124-2(5-10)

Quant Time: Apr 02 15:49:54 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 02 13:40:00 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.96	152	98469	20.00	ng	0.00
21) Naphthalene-d8	8.24	136	415594	20.00	ng	0.00
38) Acenaphthene-d10	9.99	164	203800	20.00	ng	0.00
63) Phenanthrene-d10	11.49	188	385234	20.00	ng	0.00
75) Chrysene-d12	14.14	240	253725	20.00	ng	0.00
86) Perylene-d12	15.69	264	231663	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	264920	42.90	ng	0.00
7) Phenol-d6	6.59	99	410743	54.07	ng	-0.01
23) Nitrobenzene-d5	7.52	82	240986	35.46	ng	0.00
41) 2,4,6-Tribromophenol	10.79	330	117793	51.91	ng	0.00
44) 2-Fluorobiphenyl	9.31	172	394952	30.56	ng	0.00
78) Terphenyl-d14	13.07	244	401456	36.53	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	9.70	163	35310	2.194	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF040218\
Data File : BF104132.D
Acq On : 2 Apr 2018 13:56
Operator : JU/SJ
Sample : J2128-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EPE-124-2(5-10)

Quant Time: Apr 02 15:49:54 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 02 13:40:00 2018
Response via : Initial Calibration

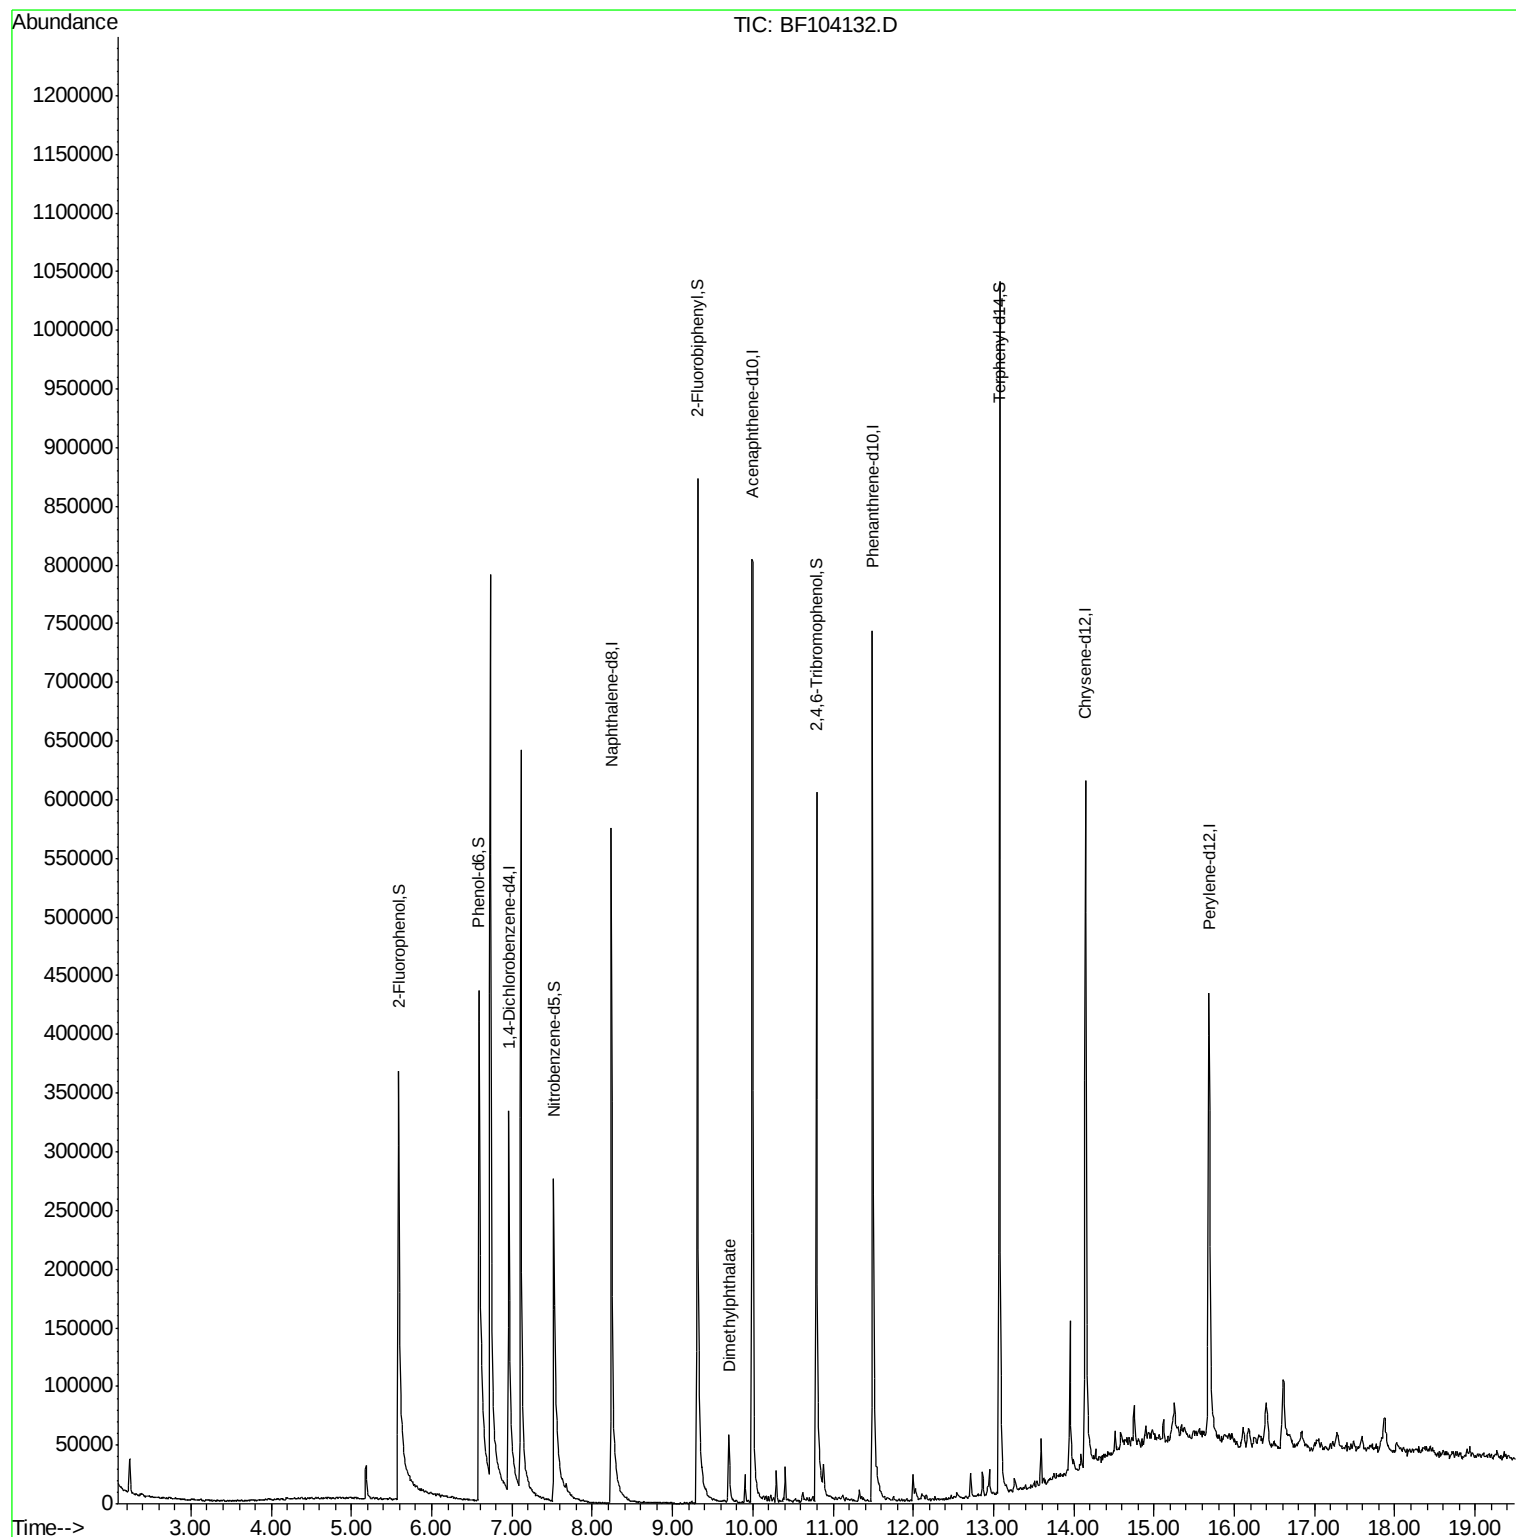







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.96 min Scan# 828
Delta R.T. -0.01 min
Lab File: BF104132.D
Acq: 2 Apr 2018 13:56

Instrument :
BNA_F
ClientSampleId :
EPE-124-2(5-10)




Tot Ion:152 Resp: 98469
Ion Ratio Lower Upper
152 100
150 153.7 124.6 186.8
115 62.3 50.1 75.1

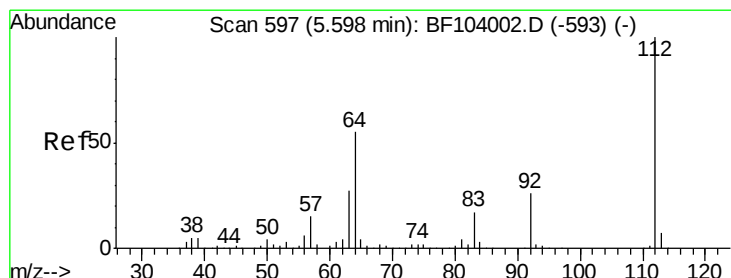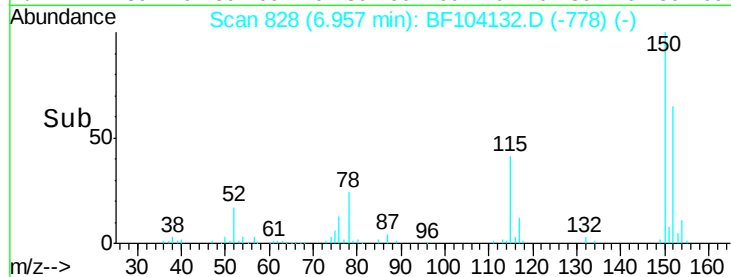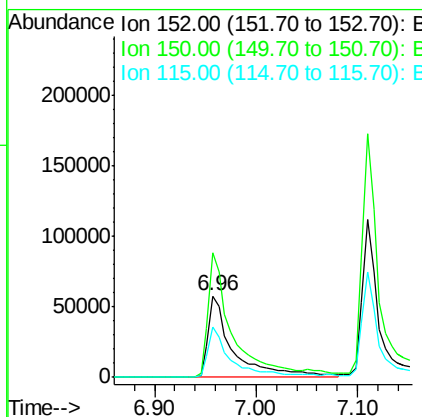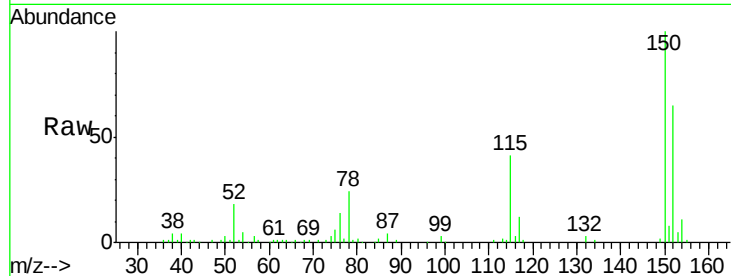


#5

2-Fluorophenol
Concen: 42.905 ng
RT: 5.59 min Scan# 595
Delta R.T. 0.00 min
Lab File: BF104132.D
Acq: 2 Apr 2018 13:56

Tgt Ion:112 Resp: 264920
Ion Ratio Lower Upper
112 100
64 51.9 47.9 71.9
63 26.2 23.7 35.5

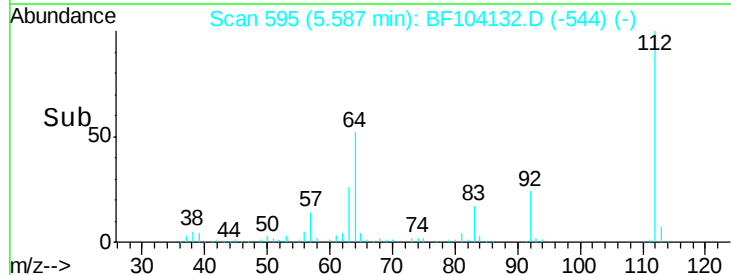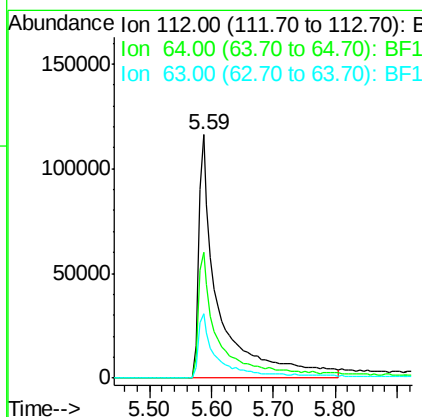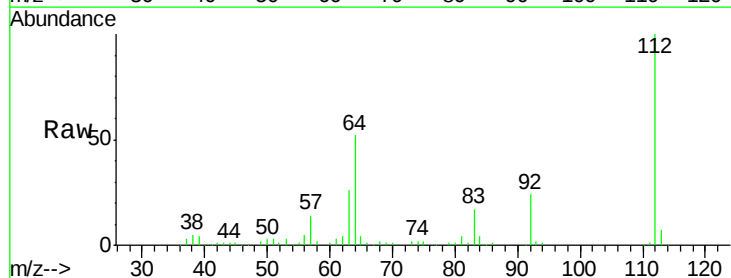

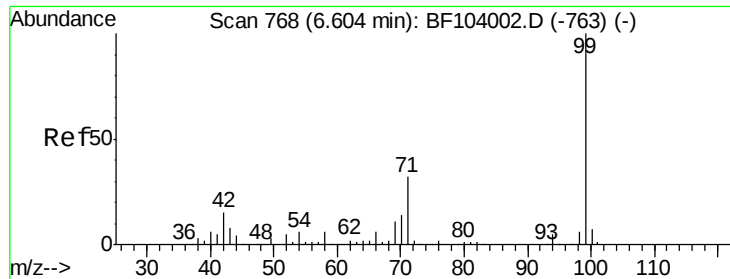

#7

Phenol-d6

Concen: 54.069 ng

RT: 6.59 min Scan# 765

Delta R.T. -0.01 min

Lab File: BF104132.D

Acq: 2 Apr 2018 13:56

Instrument :

BNA_F

ClientSampleId :

EPE-124-2(5-10)


Tot Ion: 99 Resp: 410743

Ion Ratio Lower Upper




99 100

42 15.1 14.5 21.7

71 31.0 25.4 38.0

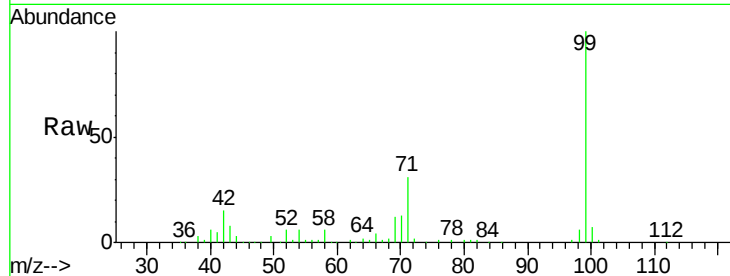

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

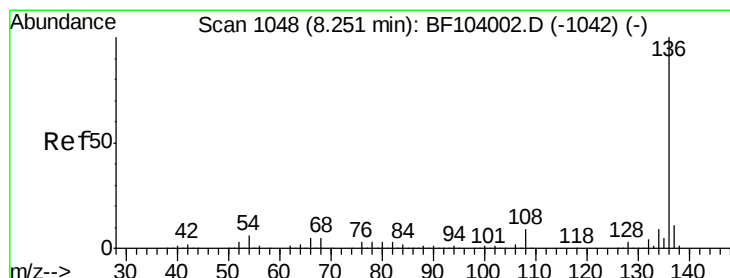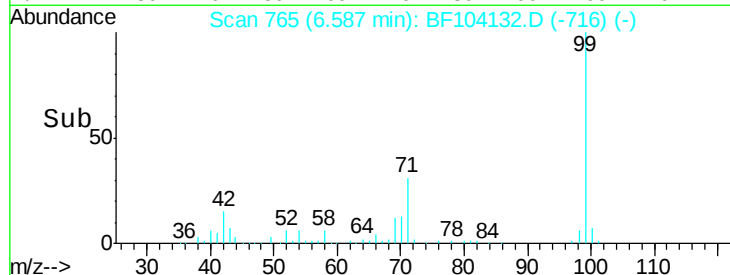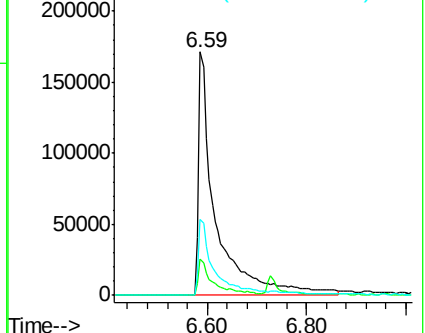

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.24 min Scan# 1046

Delta R.T. -0.01 min

Lab File: BF104132.D

Acq: 2 Apr 2018 13:56

Tgt Ion: 136 Resp: 415594


Ion Ratio Lower Upper

136 100



137 10.3 8.9 13.3


54 6.4 6.6 9.8#

68 5.8 5.0 7.4

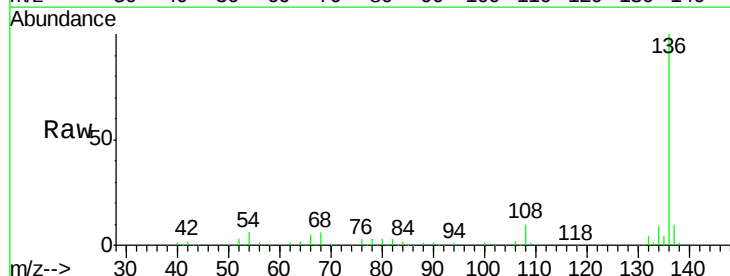

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



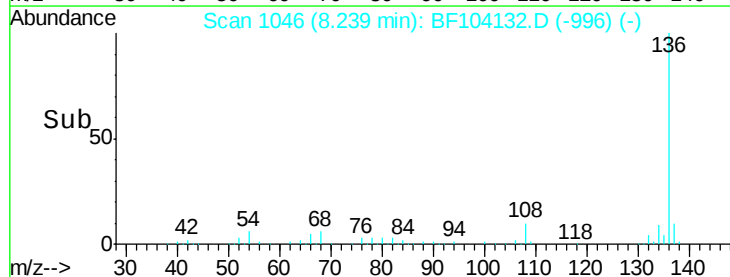
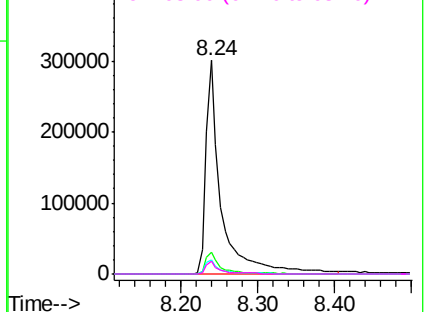


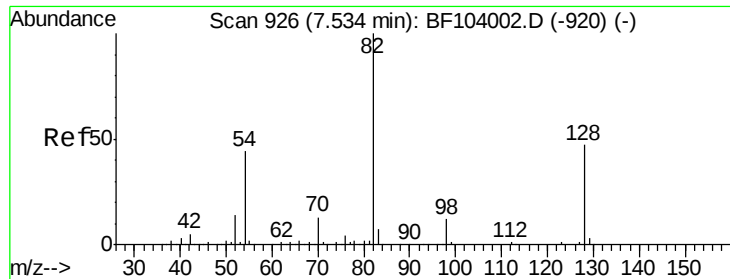

#23
 Nitrobenzene-d5
 Concen: 35.462 ng
 RT: 7.52 min Scan# 924
 Delta R.T. -0.01 min
 Lab File: BF104132.D
 Acq: 2 Apr 2018 13:56




Instrument :
 BNA_F
 ClientSampleId :
 EPE-124-2(5-10)


Tot Ion: 82 Resp: 240986
 Ion Ratio Lower Upper
 82 100
 128 46.6 36.1 54.1
 54 42.4 41.4 62.2

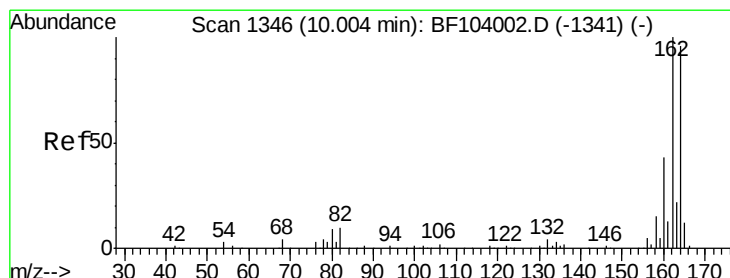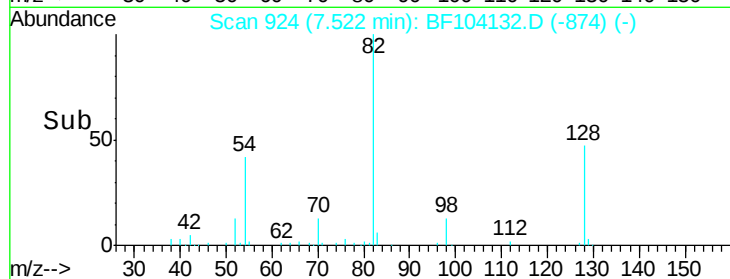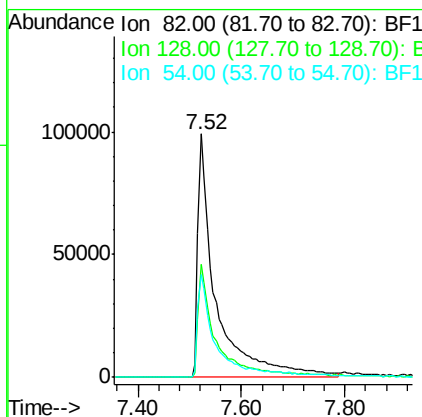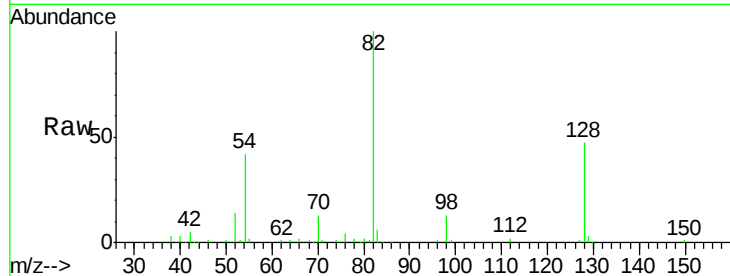

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.99 min Scan# 1344
 Delta R.T. -0.01 min
 Lab File: BF104132.D
 Acq: 2 Apr 2018 13:56

Tgt Ion: 164 Resp: 203800
 Ion Ratio Lower Upper
 164 100
 162 102.5 86.1 129.1
 160 44.1 38.3 57.5


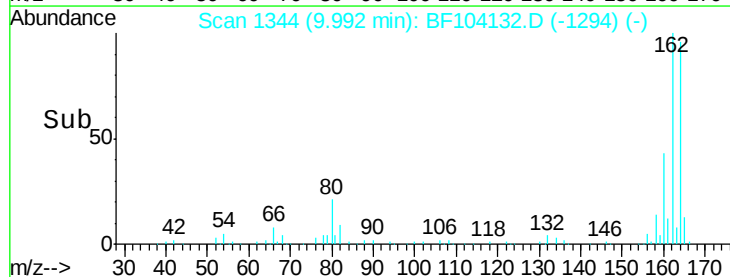
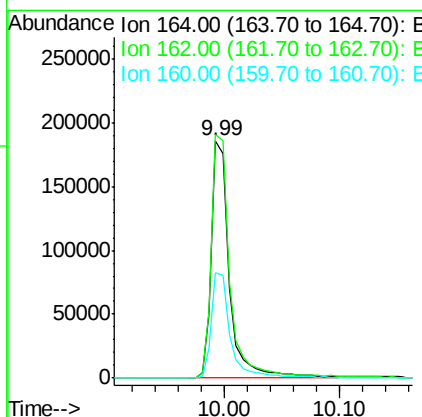
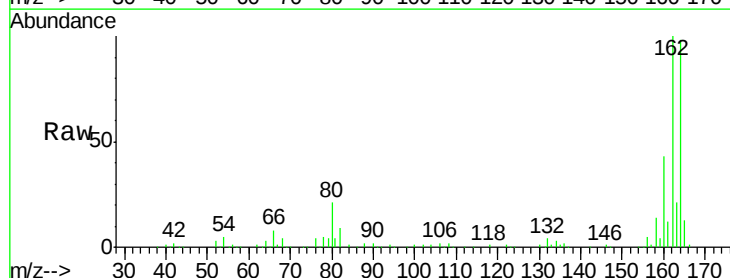


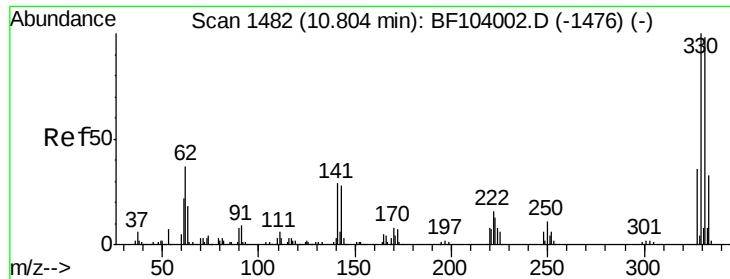

#41
 2,4,6-Tribromophenol
 Concen: 51.907 ng
 RT: 10.79 min Scan# 1480
 Delta R.T. -0.01 min
 Lab File: BF104132.D
 Acq: 2 Apr 2018 13:56




Instrument :
 BNA_F
 ClientSampleId :
 EPE-124-2(5-10)


Tot Ion	Ratio	Lower	Upper
330	100		
332	98.6	77.0	115.6
141	30.9	29.9	44.9

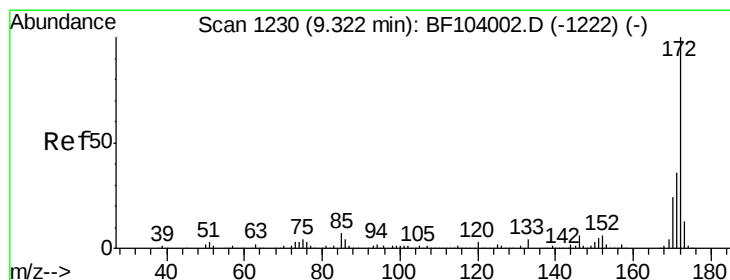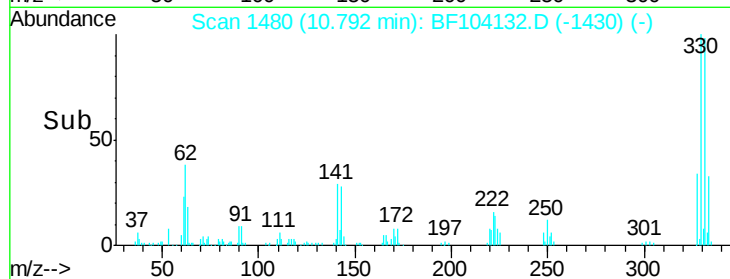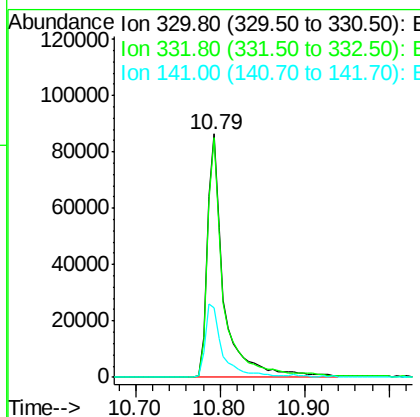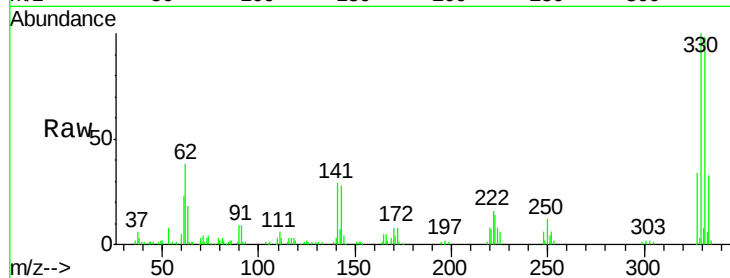

#44
 2-Fluorobiphenyl
 Concen: 30.560 ng
 RT: 9.31 min Scan# 1228
 Delta R.T. -0.01 min
 Lab File: BF104132.D
 Acq: 2 Apr 2018 13:56

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.8	29.7	44.5
170	22.9	19.6	29.4

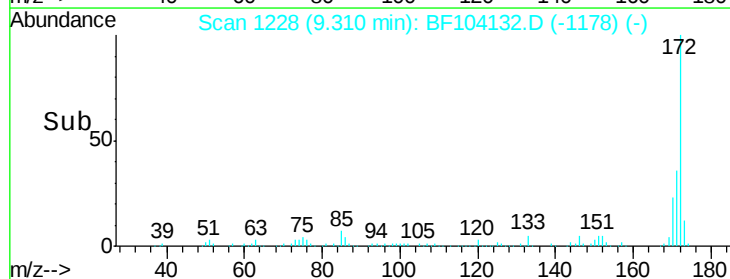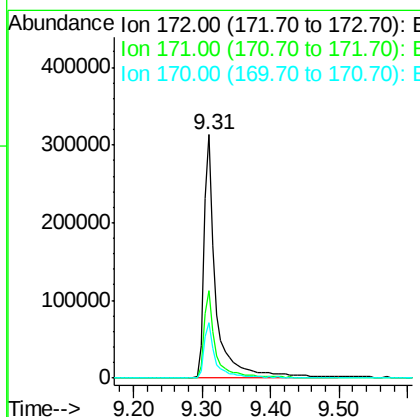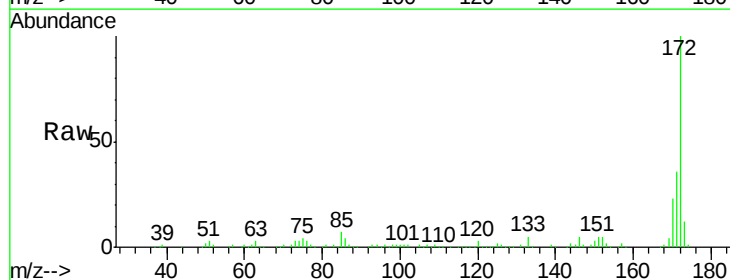

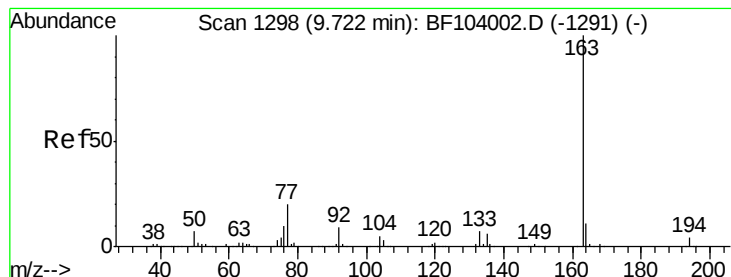

#49

Dimethylphthalate

Concen: 2.194 ng

RT: 9.70 min Scan# 1295

Delta R.T. -0.01 min

Lab File: BF104132.D

Acq: 2 Apr 2018 13:56

Instrument :

BNA_F

ClientSampleId :

EPE-124-2(5-10)


Tot Ion:163 Resp: 35310

Ion Ratio Lower Upper

163 100

194 4.0 2.7 4.1




164 10.4 8.2 12.2

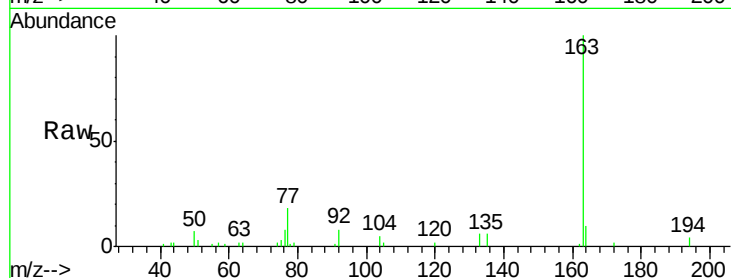

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

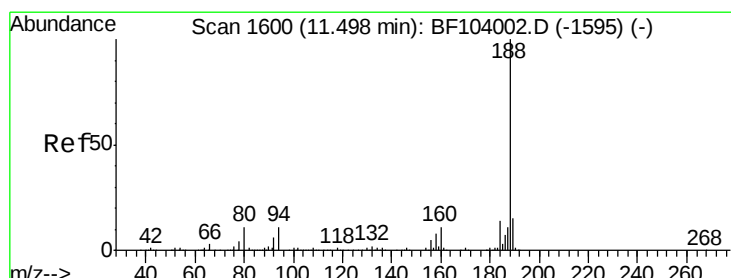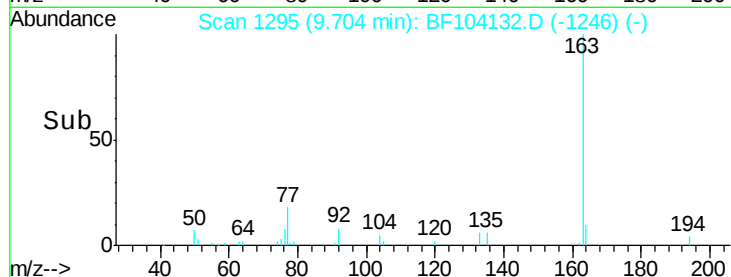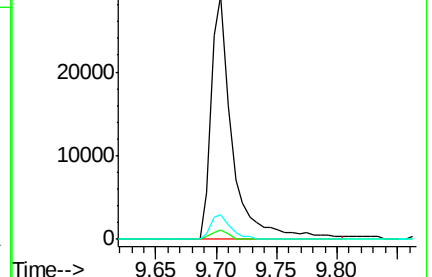

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.49 min Scan# 1599

Delta R.T. -0.01 min

Lab File: BF104132.D

Acq: 2 Apr 2018 13:56


Tgt Ion:188 Resp: 385234

Ion Ratio Lower Upper

188 100

94 10.4 8.5 12.7



80 11.2 9.2 13.8

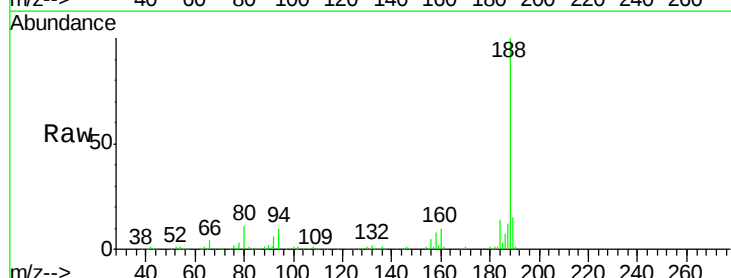


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

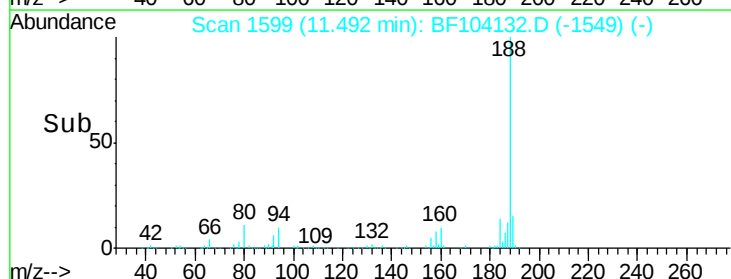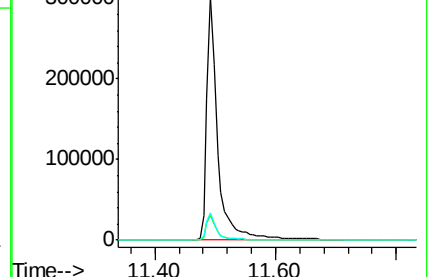

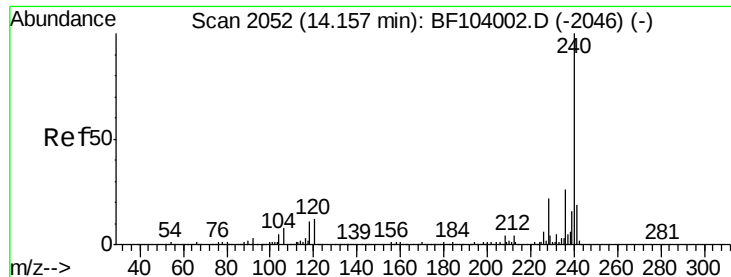

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.14 min Scan# 2050

Delta R.T. -0.01 min

Lab File: BF104132.D

Acq: 2 Apr 2018 13:56

Instrument :

BNA_F

ClientSampleId :

EPE-124-2(5-10)


Tot Ion:240 Resp: 253725

Ion Ratio Lower Upper

240 100

120 13.1 9.5 14.3




236 24.9 20.7 31.1

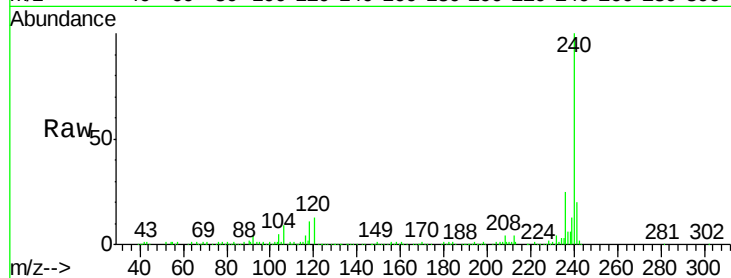

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

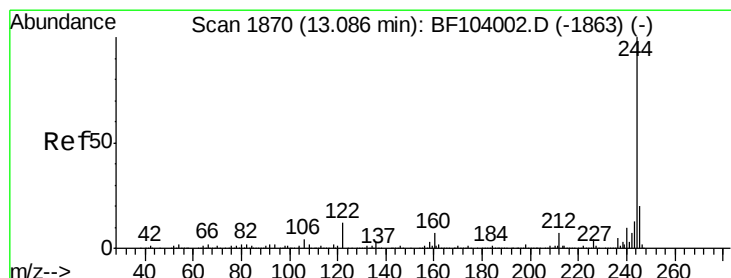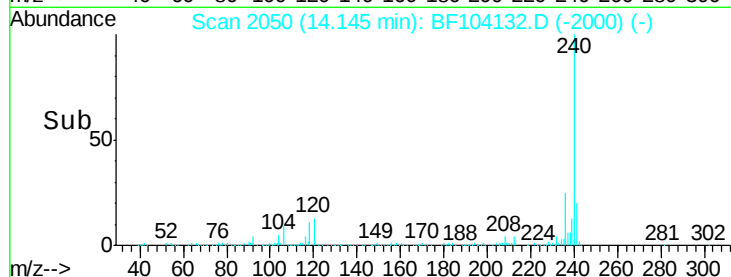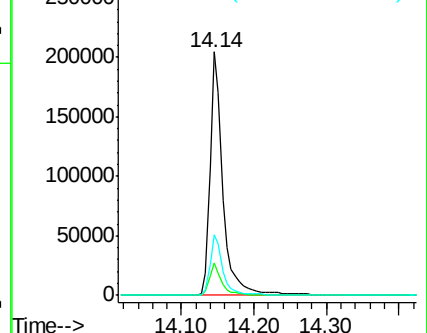

#78

Terphenyl-d14

Concen: 36.533 ng

RT: 13.07 min Scan# 1868

Delta R.T. -0.01 min

Lab File: BF104132.D

Acq: 2 Apr 2018 13:56


Tgt Ion:244 Resp: 401456

Ion Ratio Lower Upper

244 100

212 6.2 5.4 8.0



122 12.4 11.0 16.4



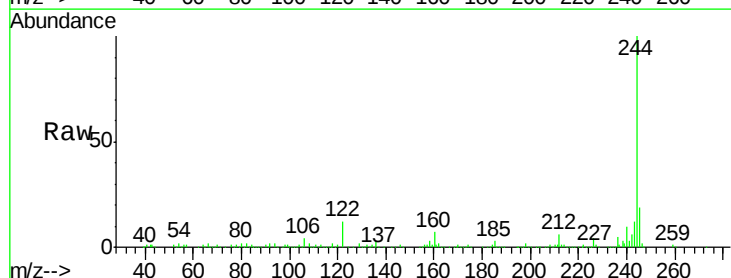


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

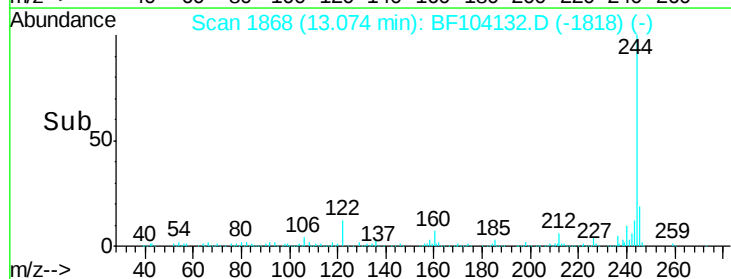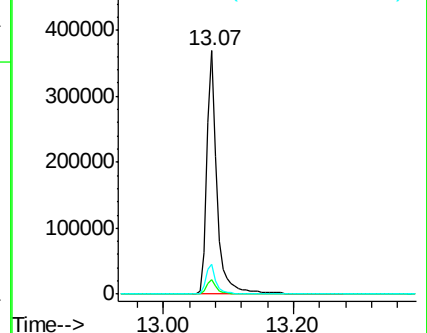

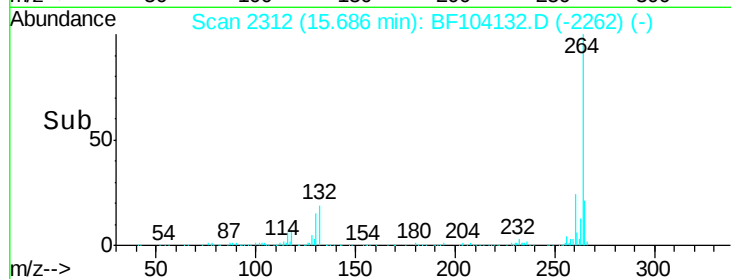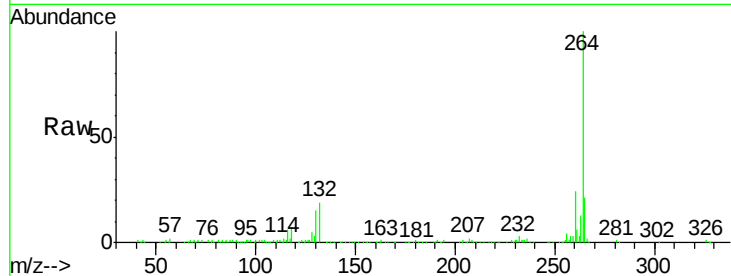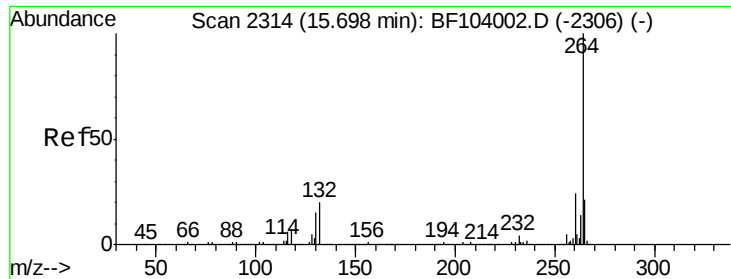

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.69 min Scan# 2312
Delta R.T. -0.01 min
Lab File: BF104132.D
Acq: 2 Apr 2018 13:56

Instrument :
BNA_F
ClientSampleId :
EPE-124-2(5-10)

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.7	19.2	28.8
265	21.0	17.5	26.3

