


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF040218\
 Data File : BF104124.D
 Acq On : 2 Apr 2018 10:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 02 13:40:00 2018

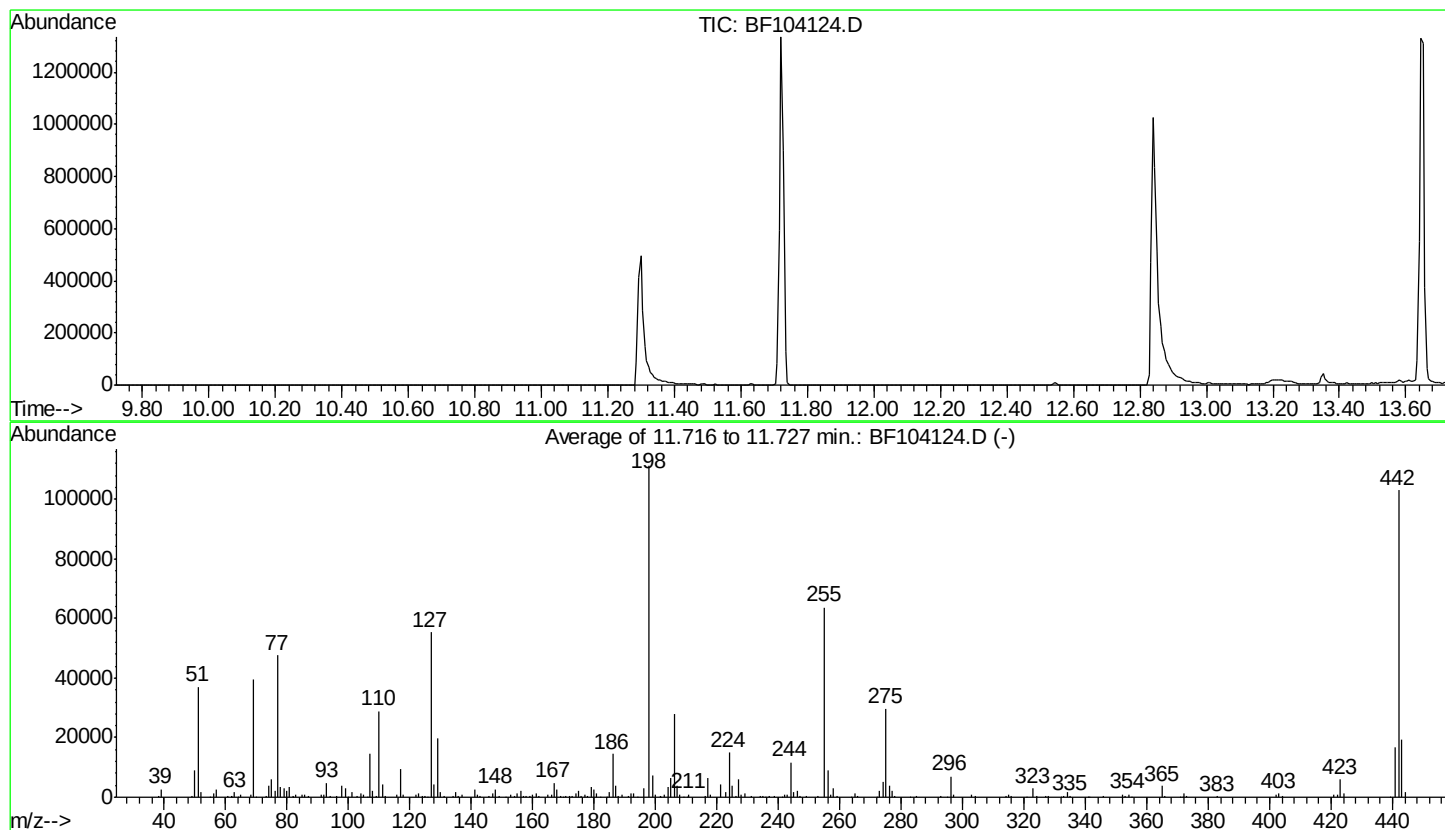

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	36968	PASS
68	69	0.00	2	2.0	791	PASS
69	198	0.00	100	35.4	39362	PASS
70	69	0.00	2	0.6	231	PASS
127	198	10	80	49.7	55282	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	111245	PASS
199	198	5	9	6.6	7288	PASS
275	198	10	60	26.7	29660	PASS
365	198	1	100	3.4	3831	PASS
441	443	0.01	100	85.6	16640	PASS
442	198	50	100	92.5	102954	PASS
443	442	15	24	18.9	19449	PASS