


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF040218\
Data File : BF104151.D
Acq On : 2 Apr 2018 22:41
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 02 13:40:00 2018

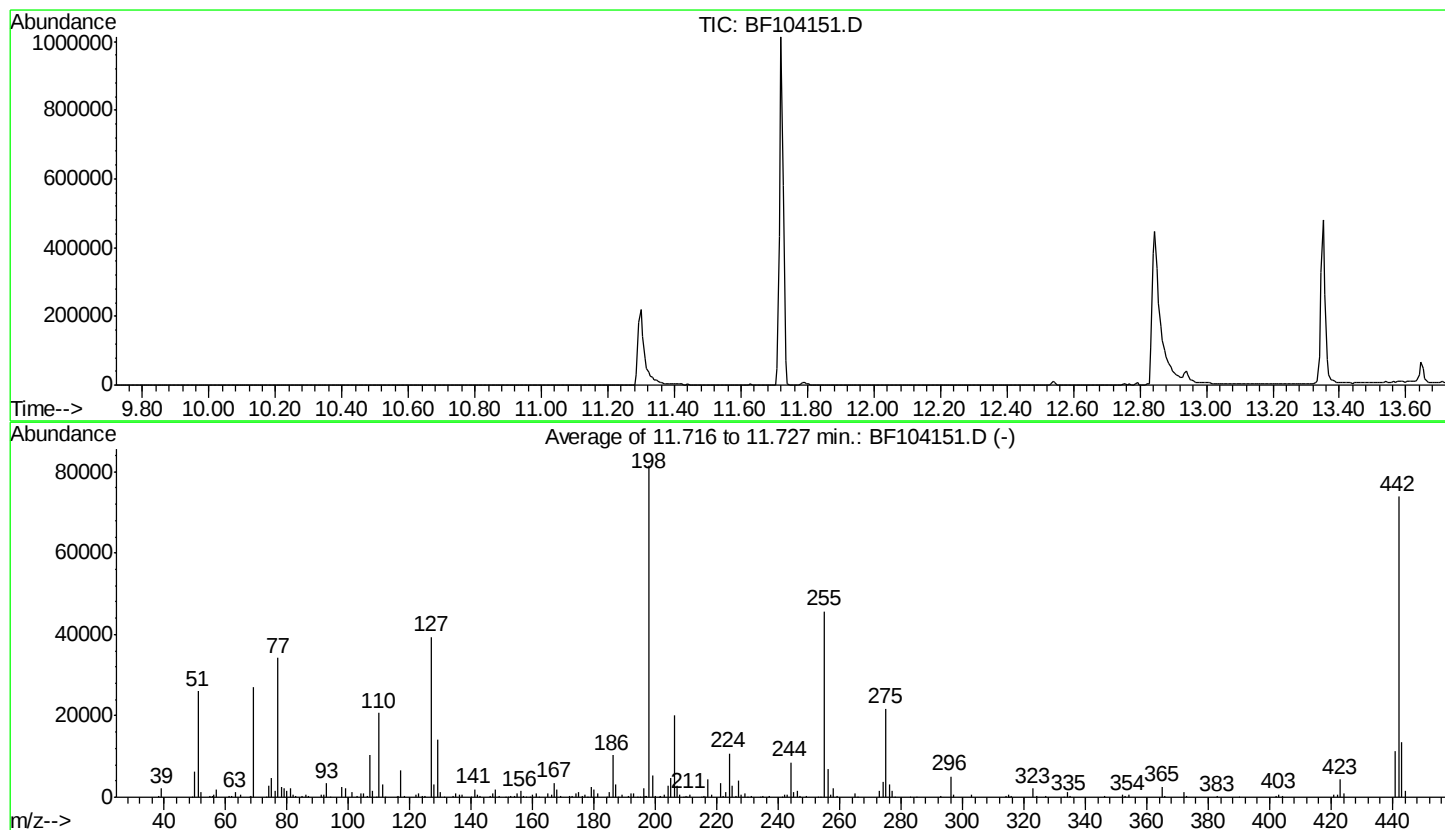

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	26051	PASS
68	69	0.00	2	1.1	309	PASS
69	198	0.00	100	33.2	27057	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.5	39490	PASS
197	198	0.00	2	0.5	447	PASS
198	198	100	100	100.0	81490	PASS
199	198	5	9	6.6	5366	PASS
275	198	10	60	26.8	21863	PASS
365	198	1	100	3.2	2617	PASS
441	443	0.01	100	83.2	11268	PASS
442	198	50	100	90.6	73800	PASS
443	442	15	24	18.4	13548	PASS