
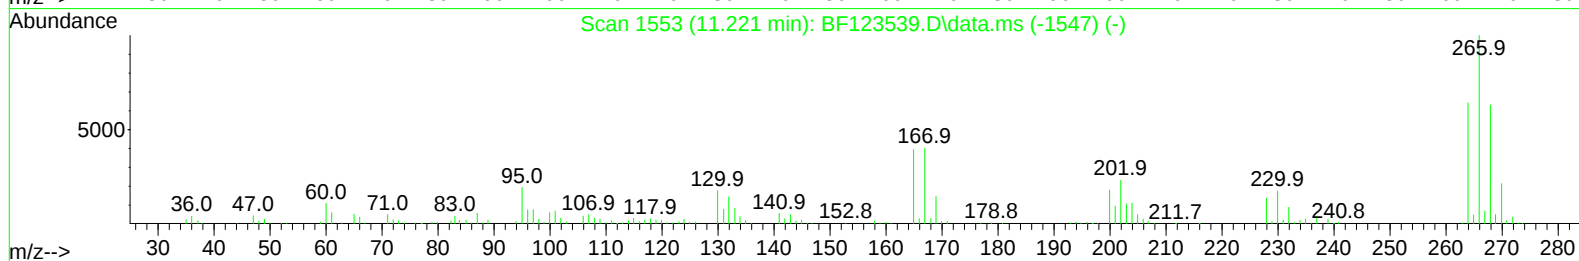
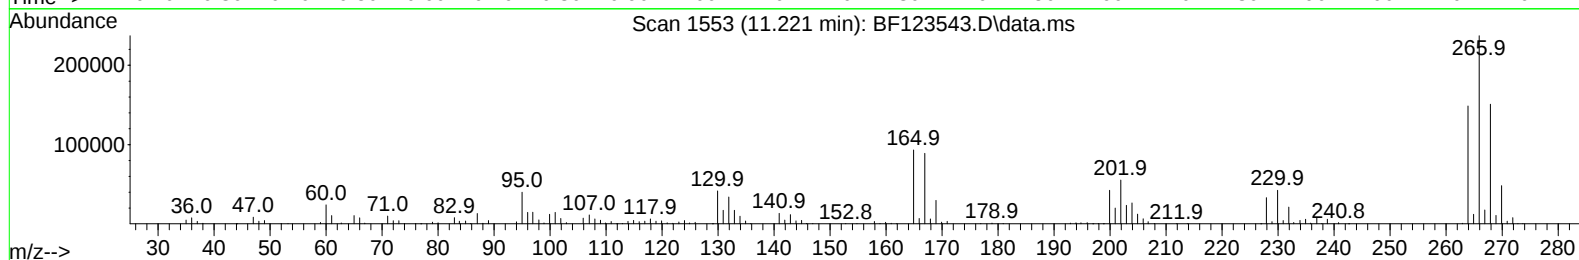


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040221\
Data File : BF123543.D
Acq On : 1 Apr 2021 16:09
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 17:07:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 15:12:46 2021
Response via : Initial Calibration

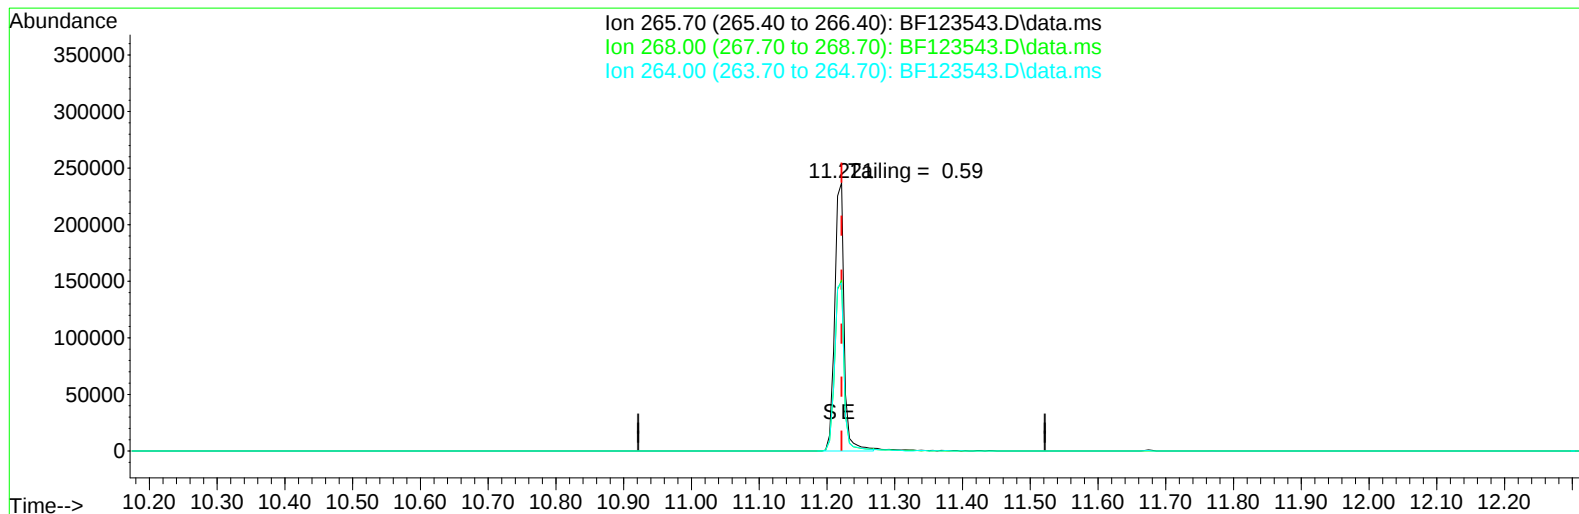

TIC: BF123543.D\data.ms




(70) Pentachlorophenol (C)

11.221min (-0.000) 28699.38 ng

response 233200

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.65
264.00	62.30	62.68
0.00	0.00	0.00

Quant Time: Apr 01 17:07:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 15:12:46 2021
Response via : Initial Calibration

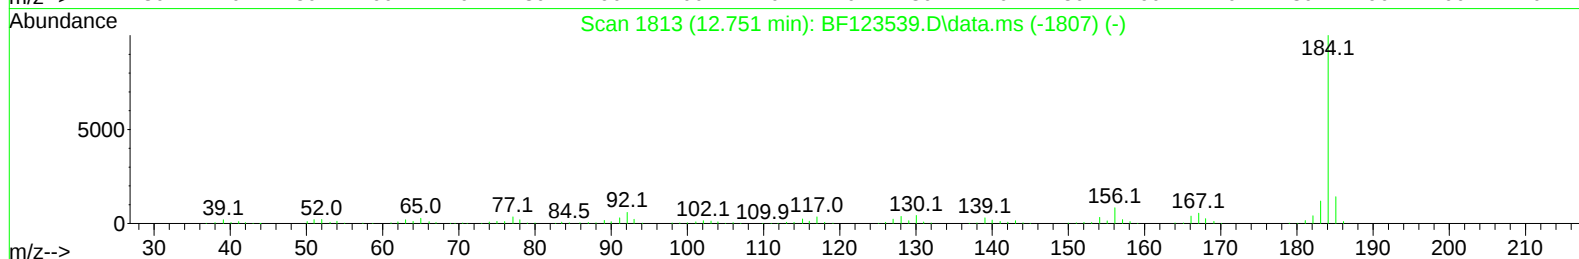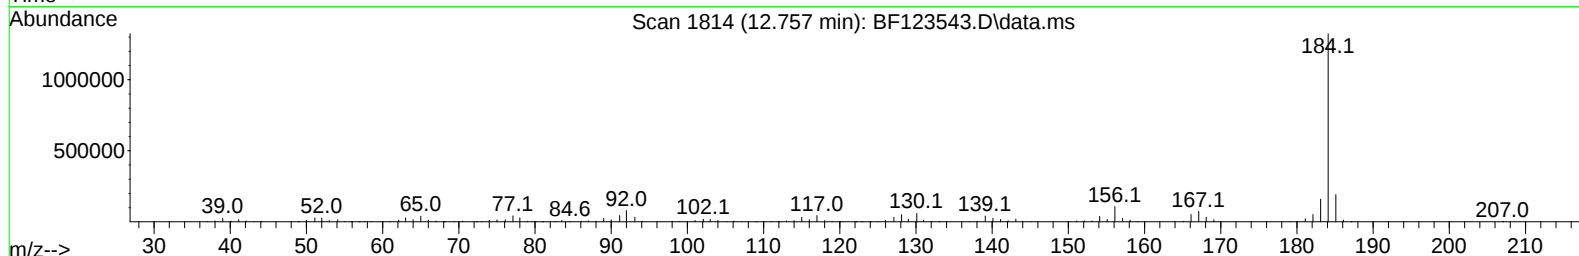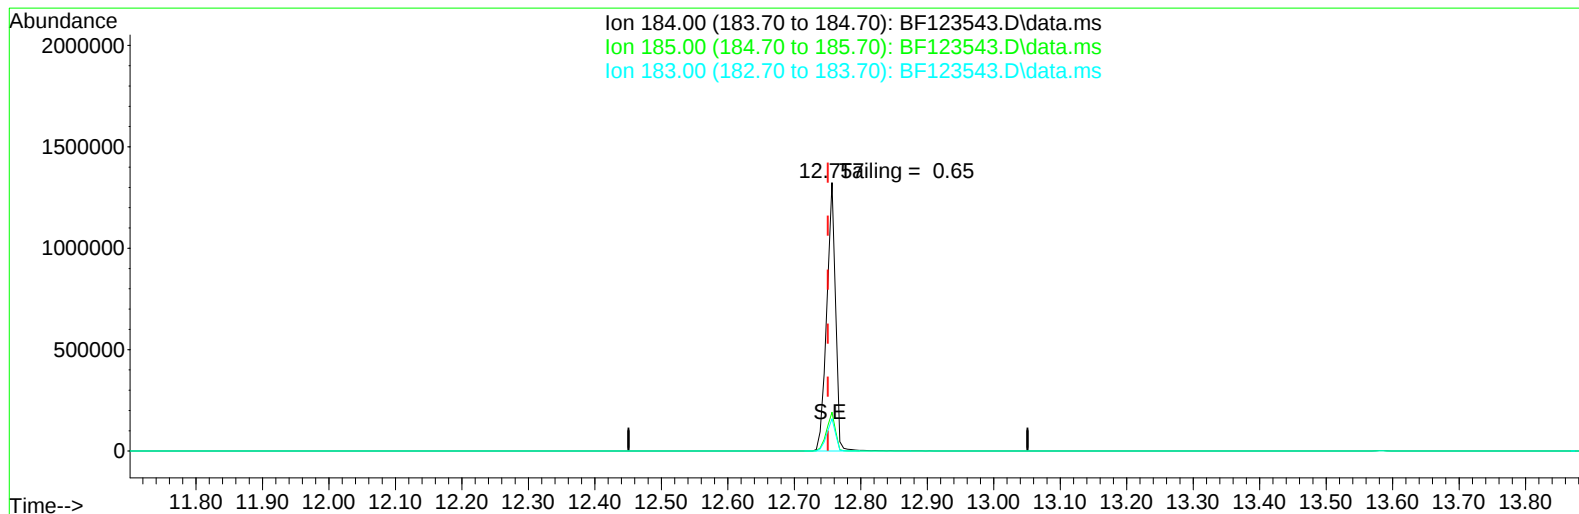

TIC: BF123543.D\data.ms

(77) Benzidine

12.757min (+ 0.006) 0.00 ng

response **1218528**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.47
183.00	12.10	12.04
0.00	0.00	0.00