
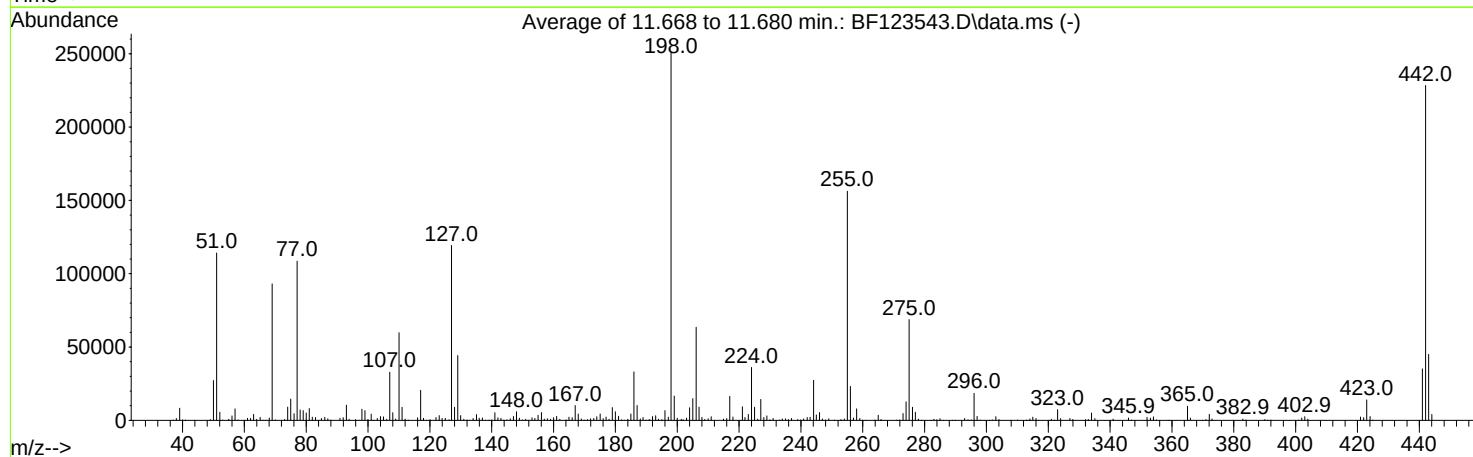


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040221\
 Data File : BF123543.D
 Acq On : 1 Apr 2021 16:09
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 02 01:16:47 2021

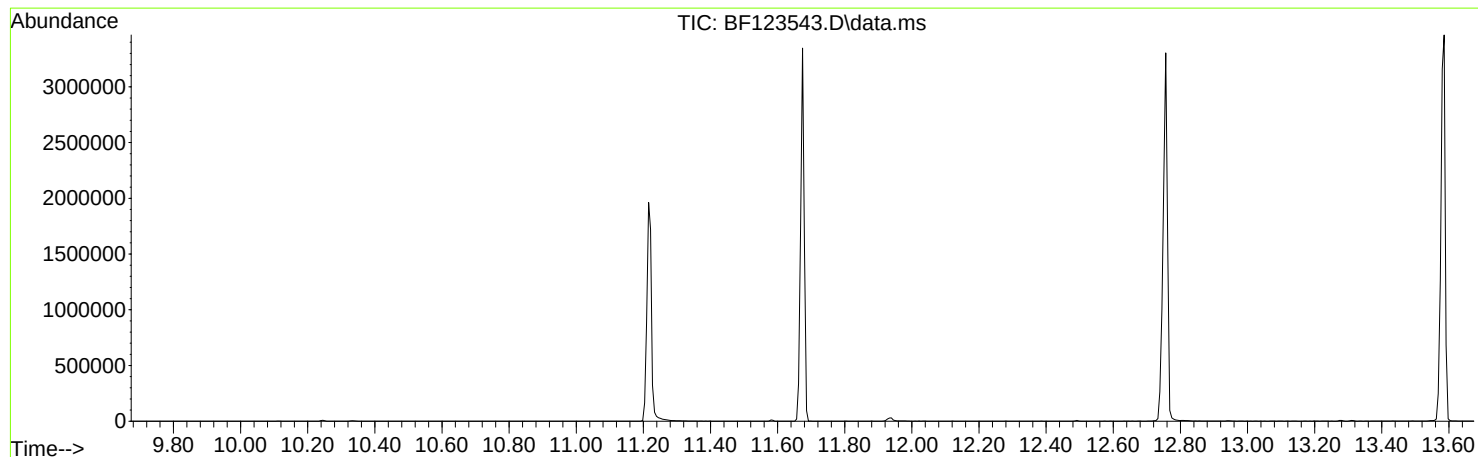

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	114115	PASS
68	69	0.00	2	1.8	1650	PASS
69	198	0.00	100	37.1	93091	PASS
70	69	0.00	2	0.4	331	PASS
127	198	10	80	47.5	119229	PASS
197	198	0.00	2	0.9	2165	PASS
198	198	100	100	100.0	250837	PASS
199	198	5	9	6.6	16602	PASS
275	198	10	60	27.4	68771	PASS
365	198	1	100	3.8	9591	PASS
441	198	0.01	100	14.0	35108	PASS
442	442	50	100	100.0	228309	PASS
443	442	15	24	19.7	44987	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/2/2021	BNA_F	<u>BF123543.D</u>
Compound Name	Response	Retention Time
DDT	605654	13.58
DDD	2247	13.17
DDE	877	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3124	608778	0.51

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040221\
Data File : BF123543.D
Acq On : 1 Apr 2021 16:09
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 01 17:07:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 15:12:46 2021
Response via : Initial Calibration

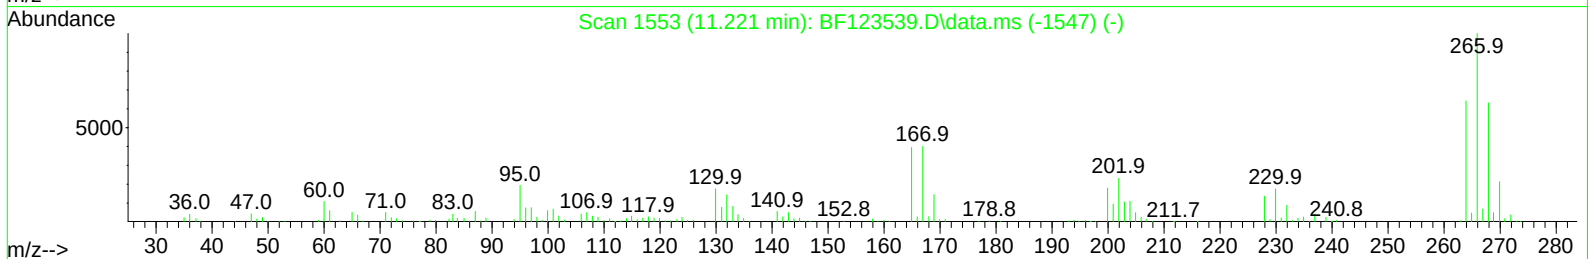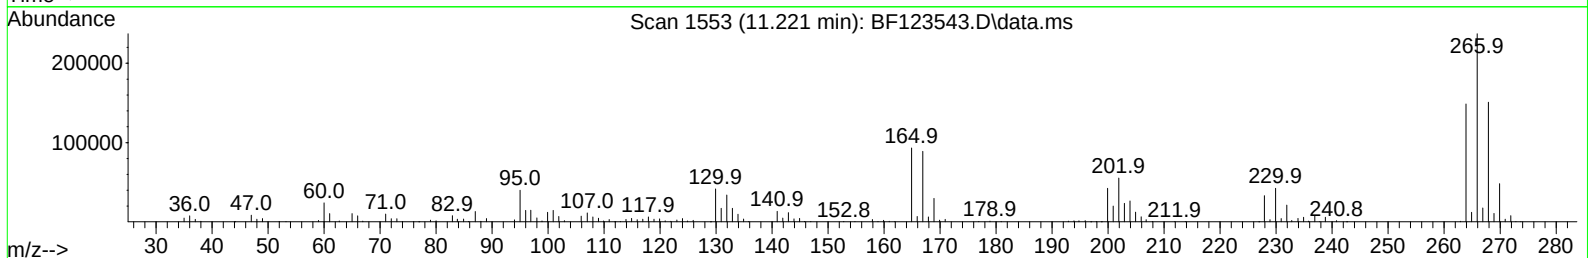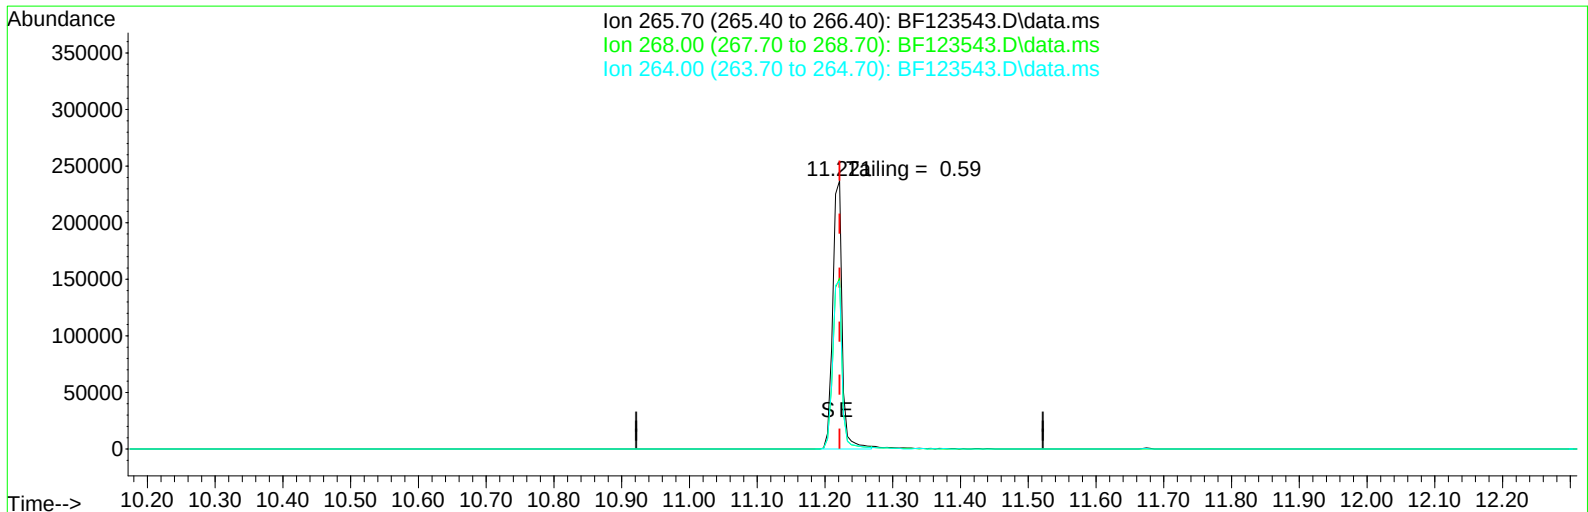

TIC: BF123543.D\data.ms

(70) Pentachlorophenol (C)

11.221min (-0.000) 28699.38 ng




response 233200

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.65
264.00	62.30	62.68
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040221\  
Data File : BF123543.D  
Acq On    : 1 Apr 2021 16:09  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 01 17:07:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 15:12:46 2021
Response via : Initial Calibration

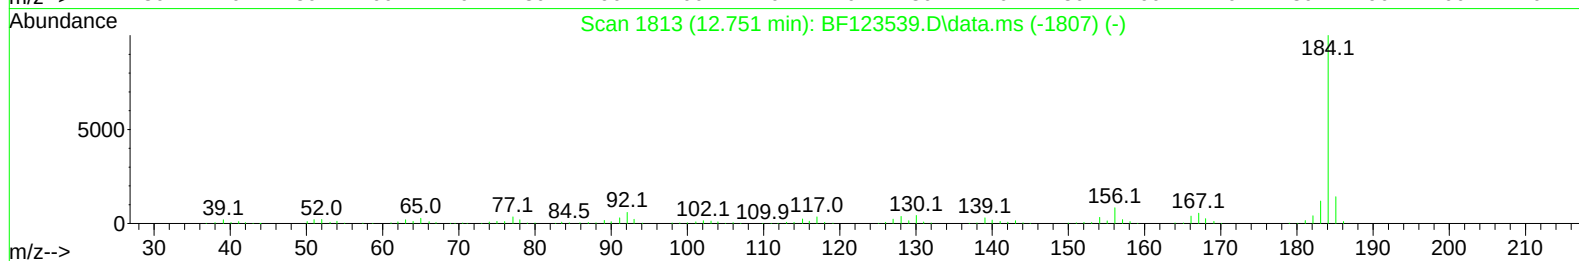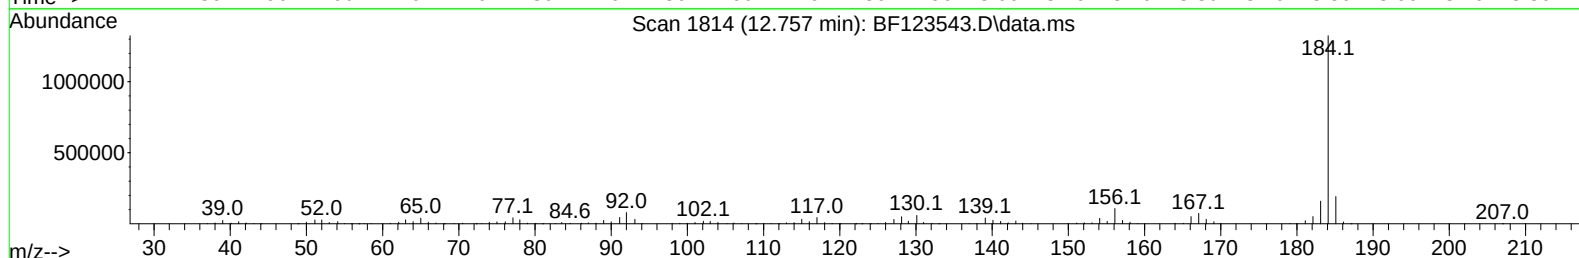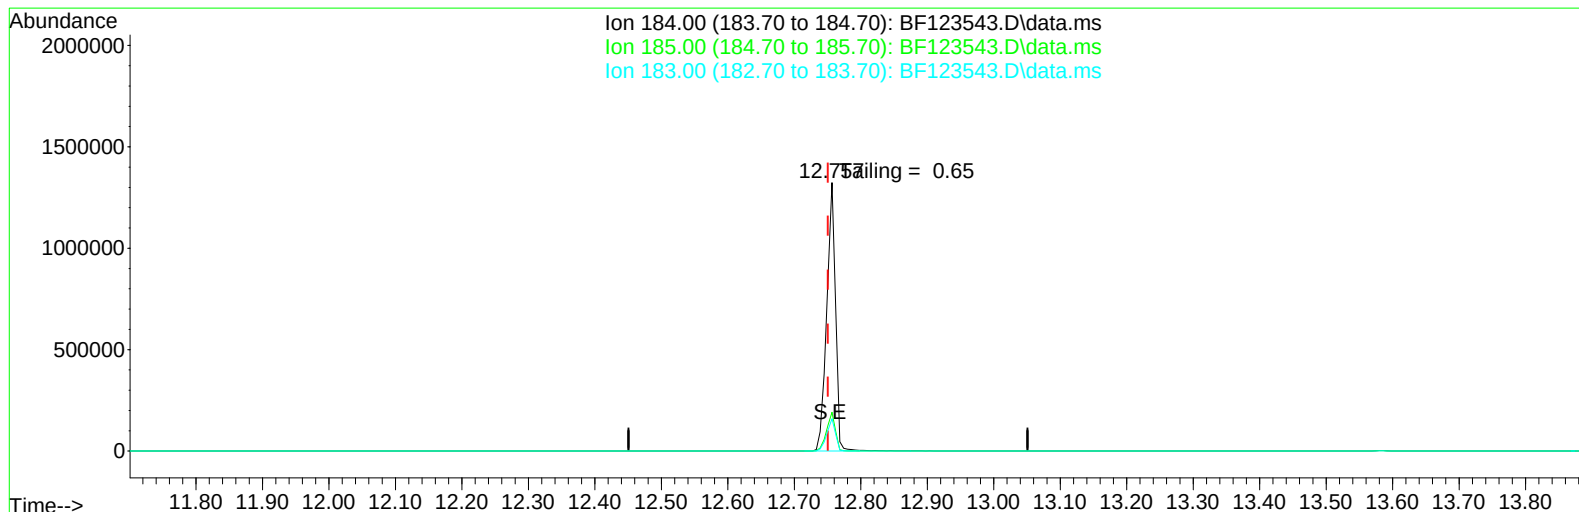

TIC: BF123543.D\data.ms

(77) Benzidine

12.757min (+ 0.006) 0.00 ng

```
response      1218528
```

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.47
183.00	12.10	12.04
0.00	0.00	0.00