
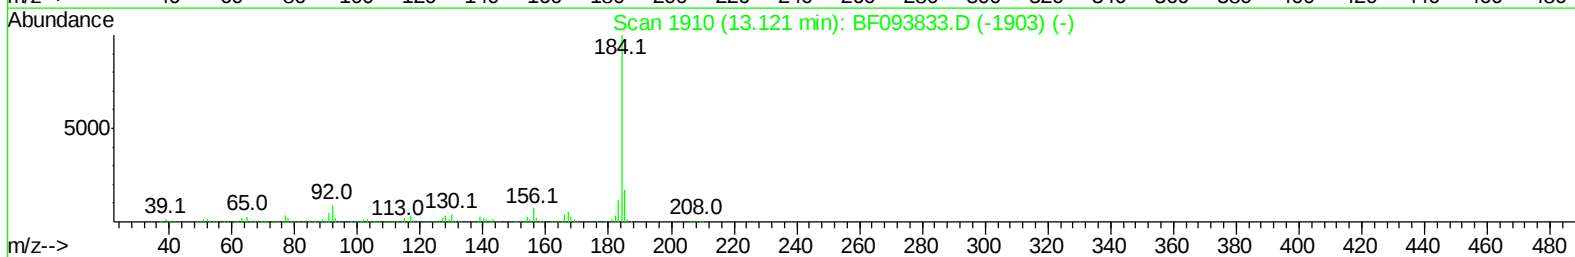
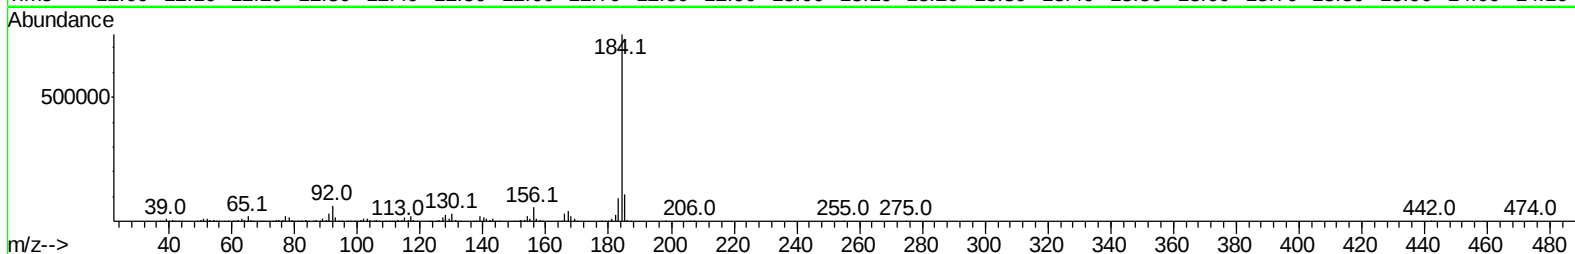


Data Path : U:\HPCHEM1\BNA F\Data\BF040317\
 Data File : BF094117.D
 Acq On : 3 Apr 2017 13:28
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 07:32:19 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 14:38:29 2017
 Response via : Initial Calibration

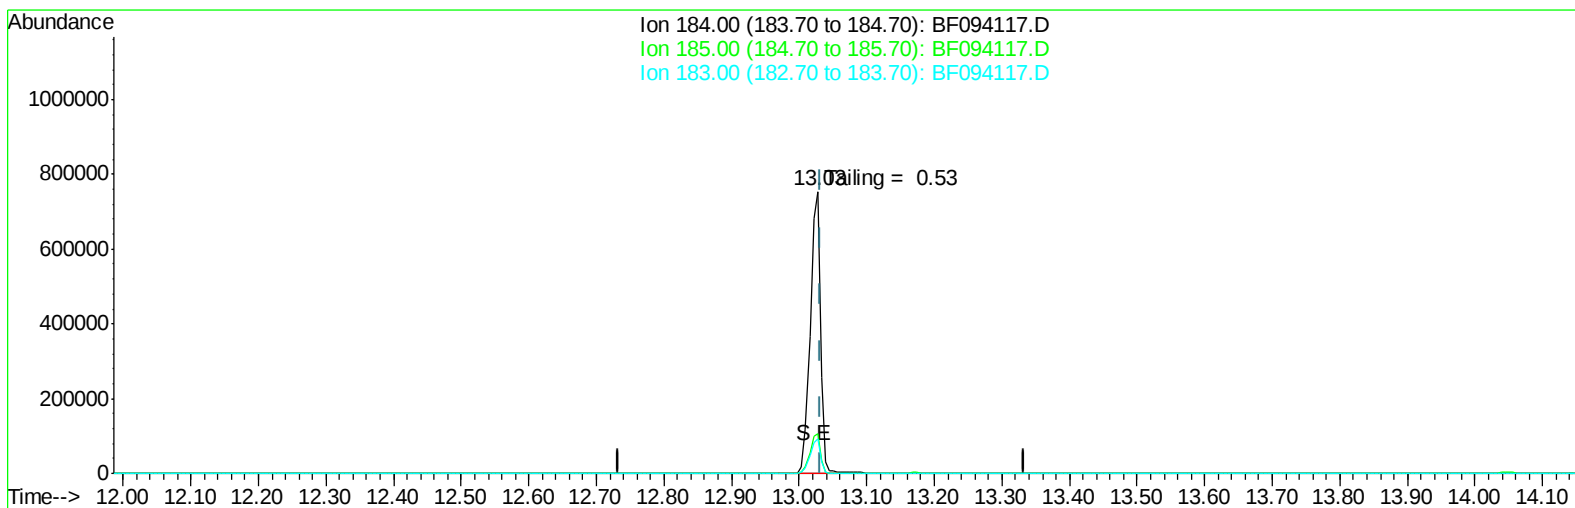

TIC: BF094117.D

(76) Benzidine




13.027min (-0.006) 0.00ng

response 798541

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.20#
183.00	12.20	12.10
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\Data\BF040317\
Data File : BF094117.D
Acq On : 3 Apr 2017 13:28
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 07:32:19 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 14:38:29 2017
Response via : Initial Calibration

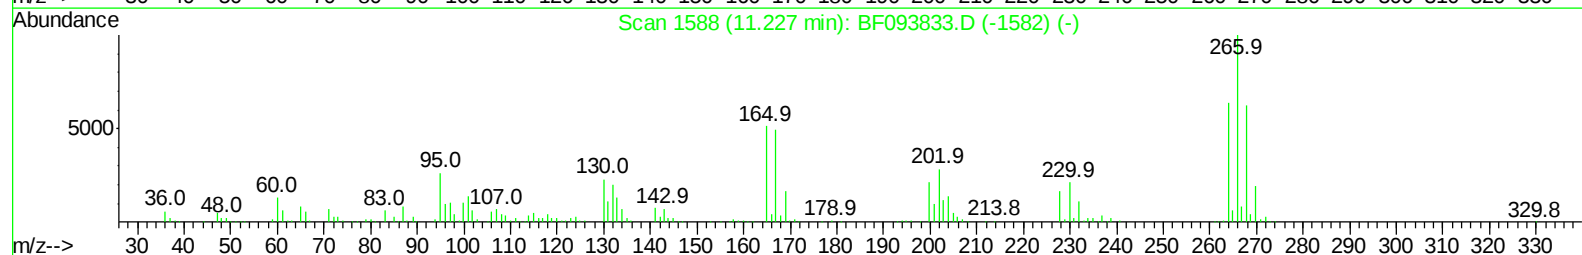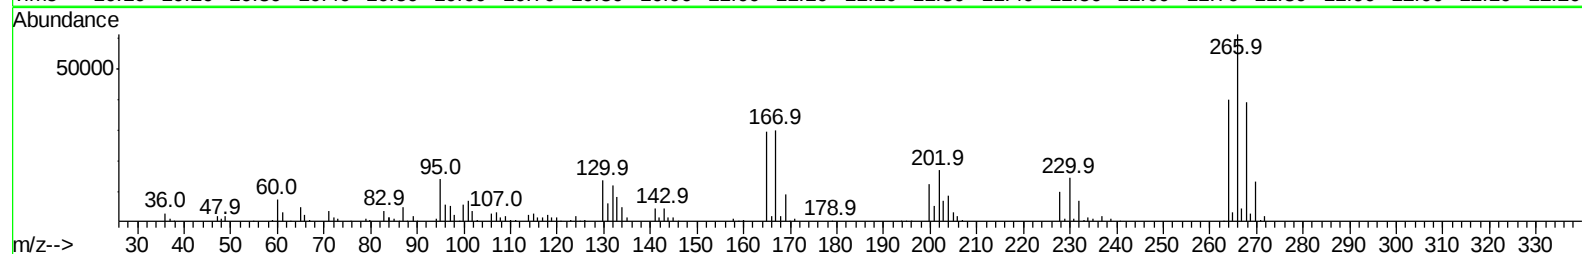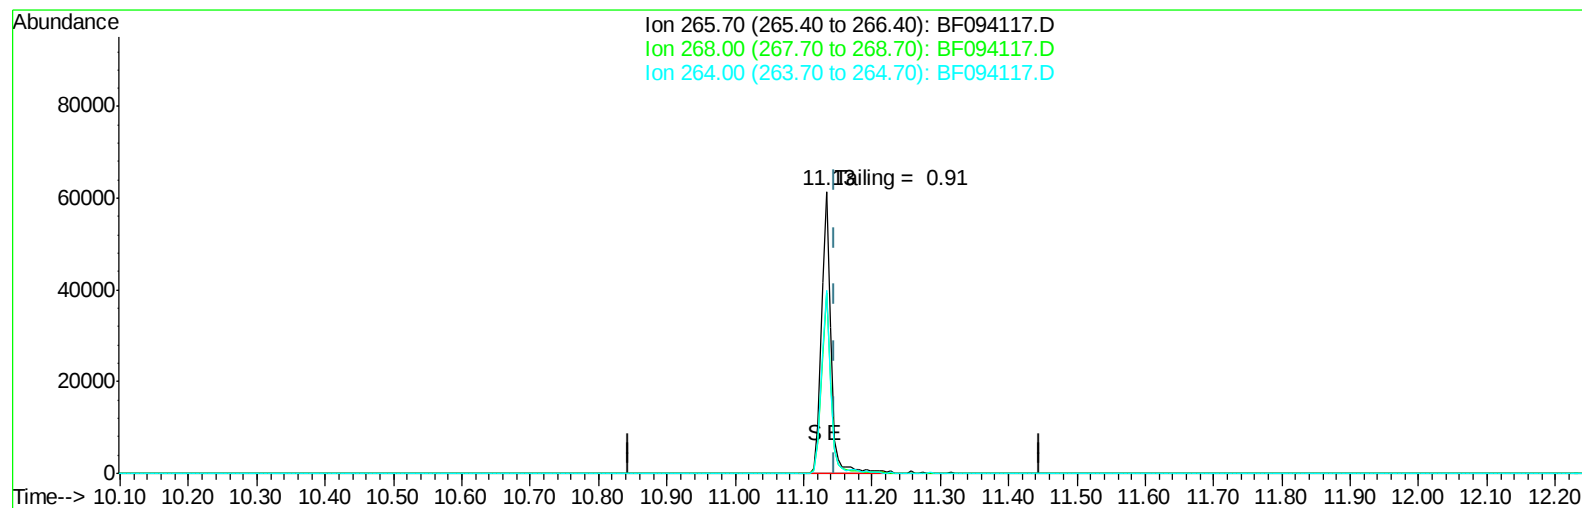

TIC: BF094117.D

(69) Pentachlorophenol (C)

11.133min (-0.012) 0.00ng

response 58875

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.94
264.00	64.60	65.16
0.00	0.00	0.00