

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040317\
 Data File : BF094163.D
 Acq On : 4 Apr 2017 12:12
 Operator : SJ/MA
 Sample : I2510-10 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-W-V-4-5-BASE

Quant Time: Apr 04 12:47:39 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 14:38:29 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	5.89	152	184446	20.00	ng	-0.02
21) Naphthalene-d8	7.39	136	691247	20.00	ng	-0.02
38) Acenaphthene-d10	9.53	164	268489	20.00	ng	-0.02
63) Phenanthrene-d10	11.36	188	423344	20.00	ng	-0.02
75) Chrysene-d12	14.62	240	360216	20.00	ng	-0.01
86) Perylene-d12	16.25	264	230517	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	4.42	112	23424	2.14	ng	-0.02
7) Phenol-d6	5.49	99	28965	2.14	ng	-0.02
23) Nitrobenzene-d5	6.53	82	12988	1.07	ng	-0.03
41) 2,4,6-Tribromophenol	10.50	330	3739	1.76	ng	-0.02
44) 2-Fluorobiphenyl	8.71	172	38632	2.19	ng	-0.02
78) Terphenyl-d14	13.33	244	27548	1.71	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040317\
Data File : BF094163.D
Acq On : 4 Apr 2017 12:12
Operator : SJ/MA
Sample : I2510-10 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-W-V-4-5-BASE

Quant Time: Apr 04 12:47:39 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 14:38:29 2017
Response via : Initial Calibration

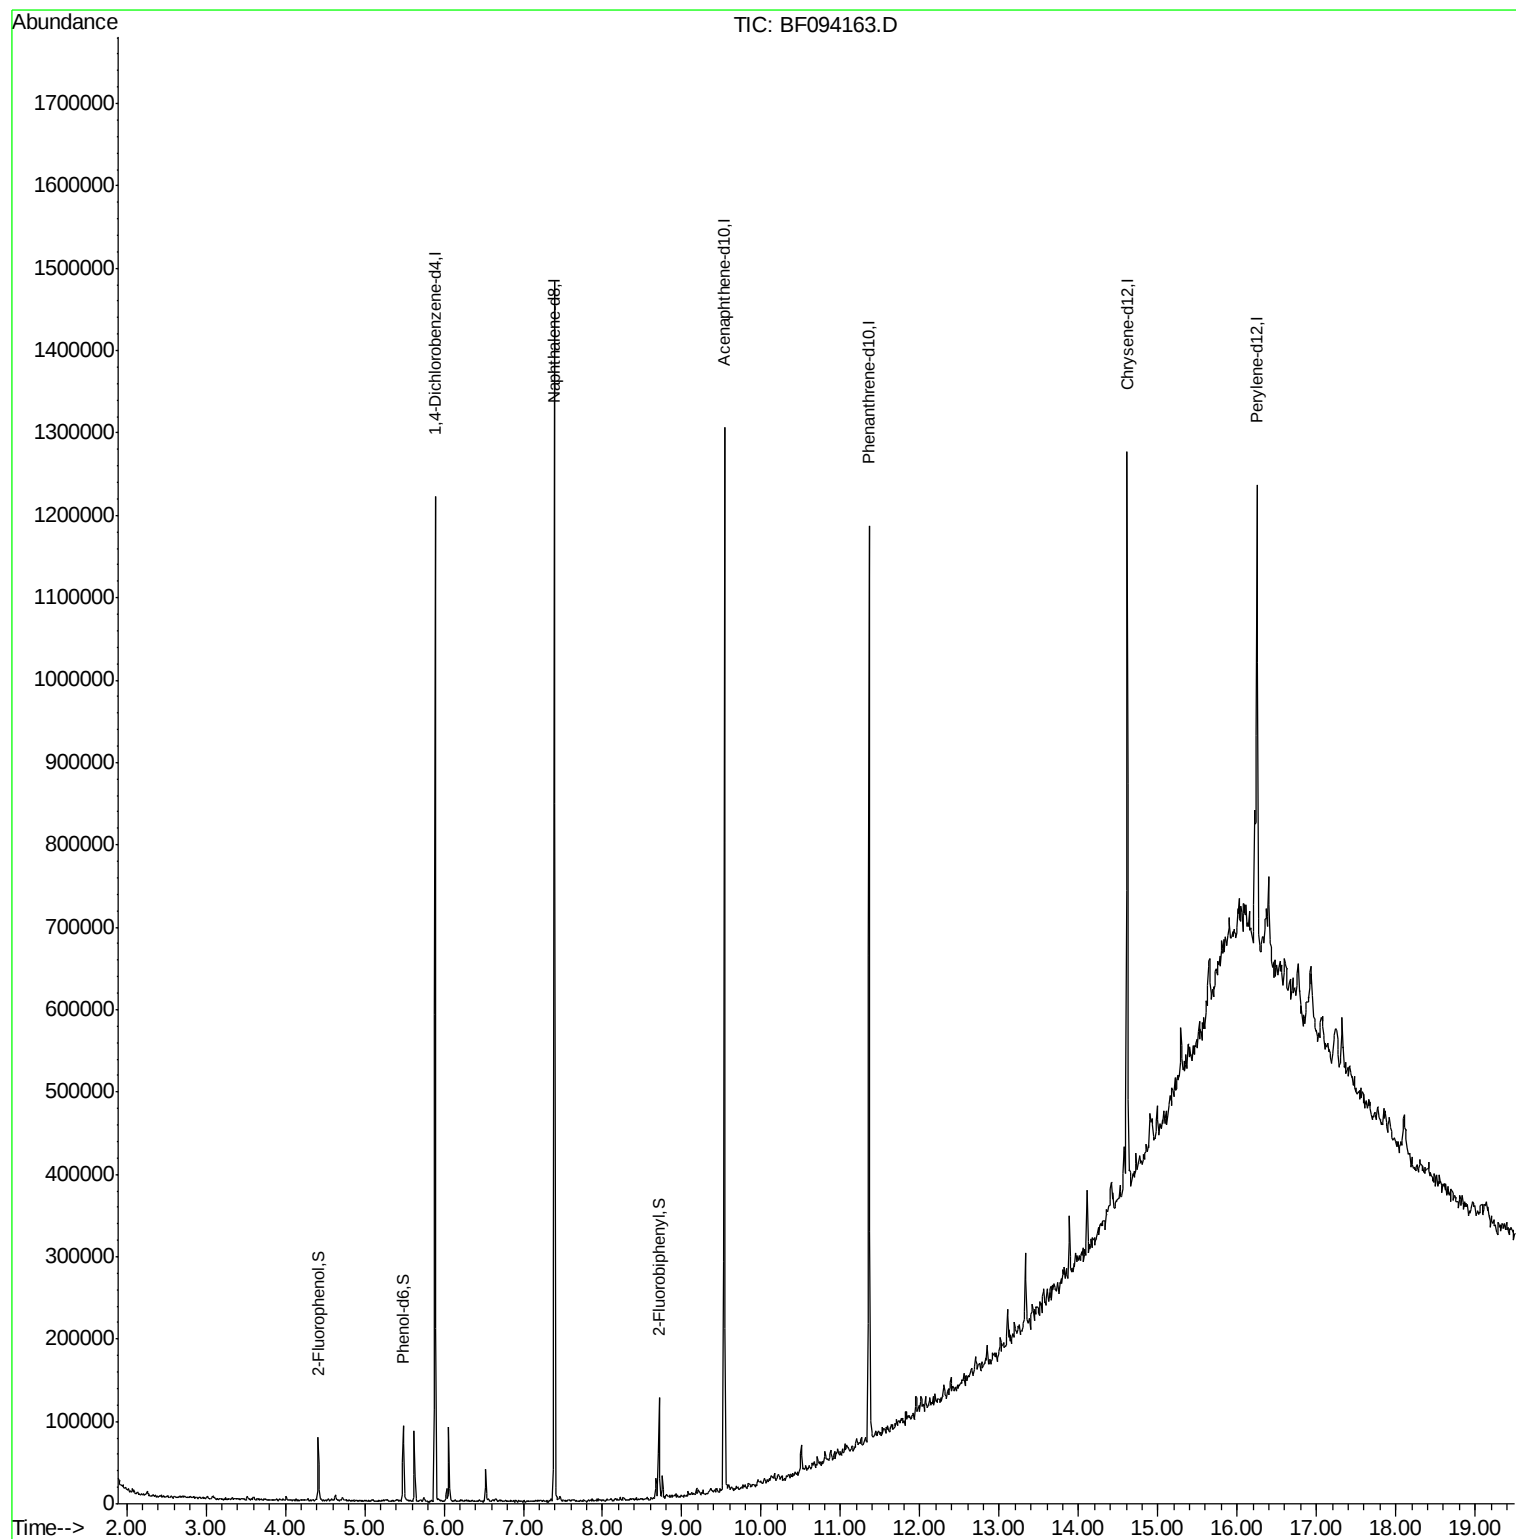

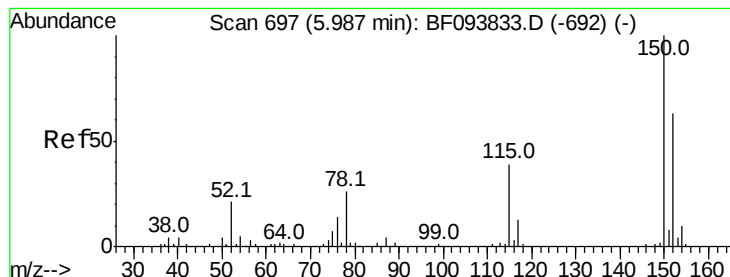

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 5.89 min Scan# 680

Delta R.T. -0.02 min

Lab File: BF094163.D

Acq: 4 Apr 2017 12:12

Instrument :

BNA_F

ClientSampleId :

E2-W-V-4-5-BASE


Tot Ion:152 Resp: 184446

Ion Ratio Lower Upper

152 100

150 159.7 126.2 189.2




115 62.0 52.2 78.2

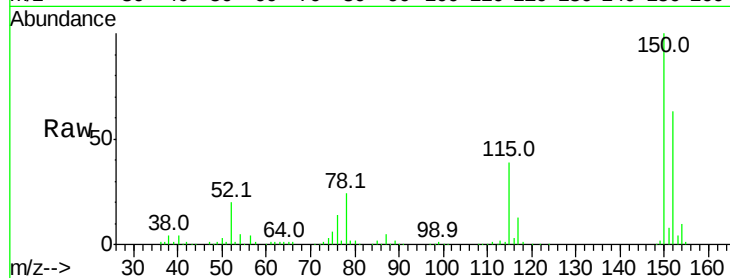

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

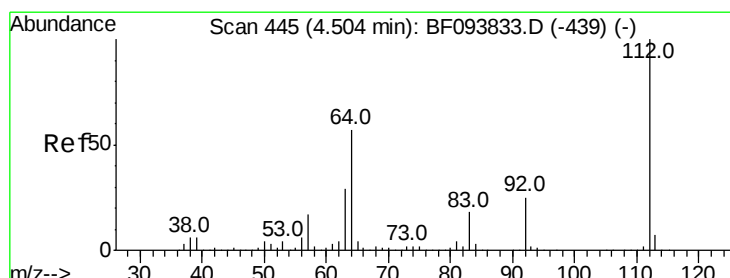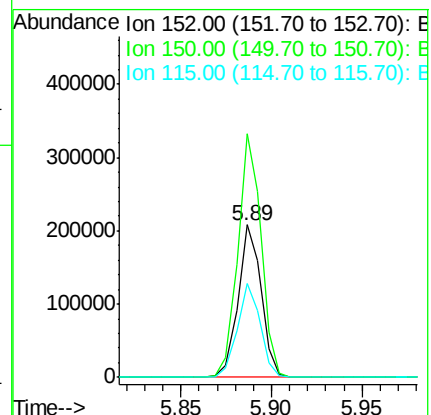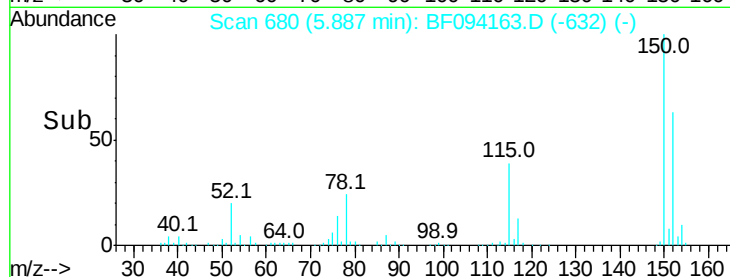

#5

2-Fluorophenol

Concen: 2.14 ng

RT: 4.42 min Scan# 430

Delta R.T. -0.02 min

Lab File: BF094163.D

Acq: 4 Apr 2017 12:12


Tgt Ion:112 Resp: 23424

Ion Ratio Lower Upper

112 100

64 58.5 46.0 69.0



63 24.7 23.4 35.0

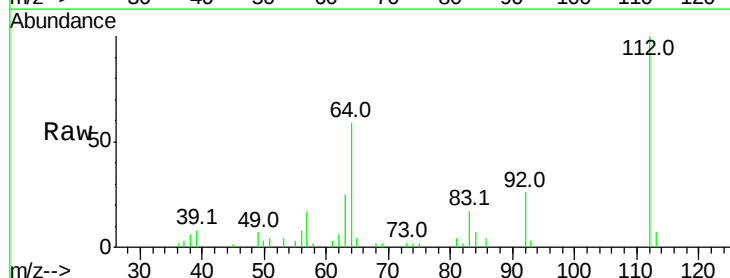

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

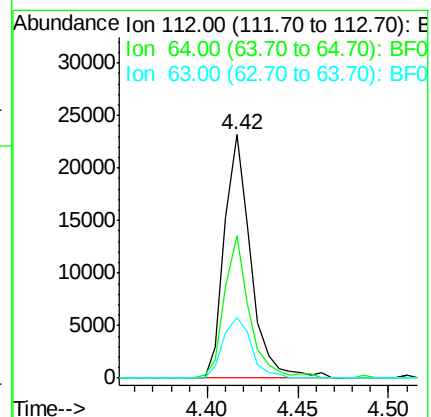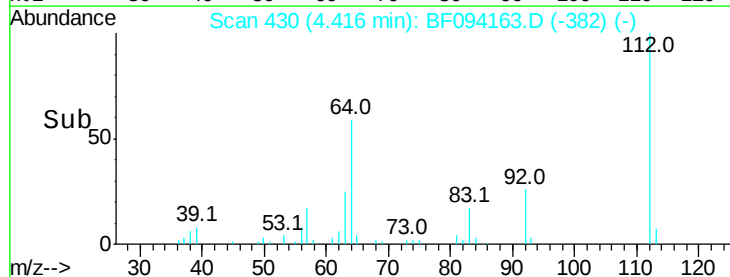



#7

Phenol-d6

Concen: 2.14 ng

RT: 5.49 min Scan# 612

Delta R.T. -0.02 min

Lab File: BF094163.D

Acq: 4 Apr 2017 12:12

Instrument :

BNA_F

ClientSampleId :

E2-W-V-4-5-BASE


Tot Ion: 99 Resp: 28965

Ion Ratio Lower Upper

99 100

42 19.8 13.5 20.3




71 39.2 24.5 36.7#

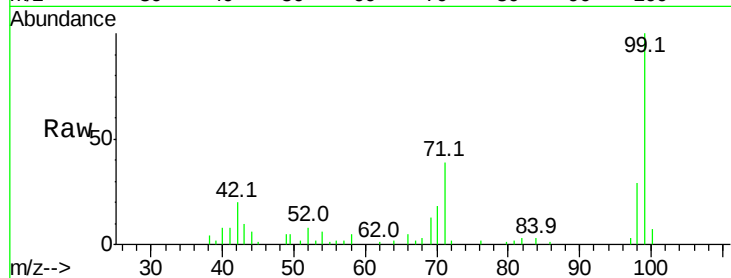

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

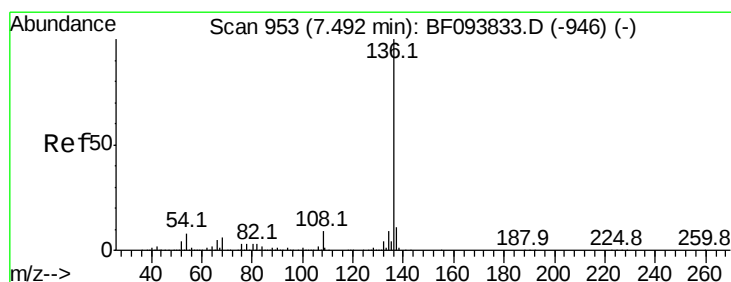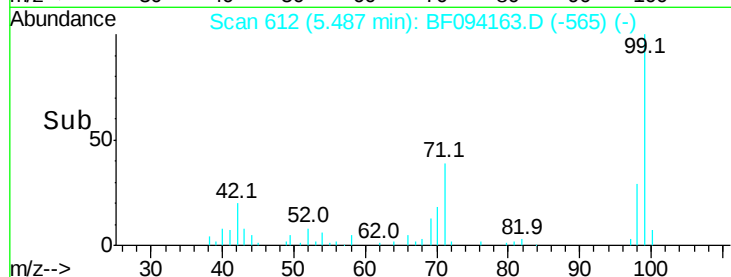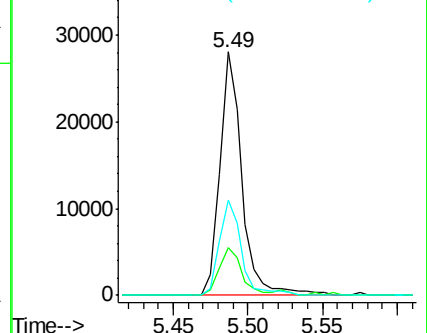

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.39 min Scan# 936

Delta R.T. -0.02 min

Lab File: BF094163.D

Acq: 4 Apr 2017 12:12

Tgt Ion: 136 Resp: 691247


Ion Ratio Lower Upper

136 100

137 10.9 8.5 12.7

54 7.1 4.9 7.3

68 5.8 4.1 6.1


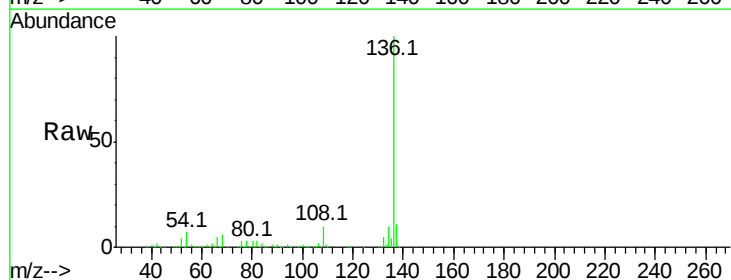



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

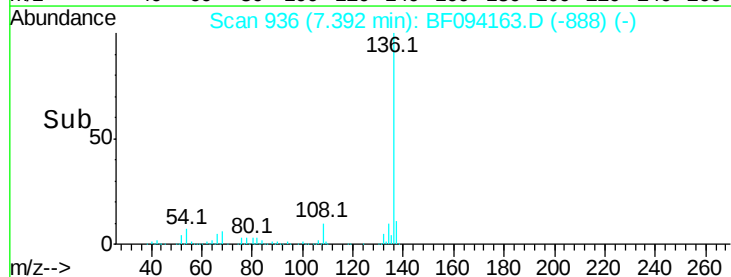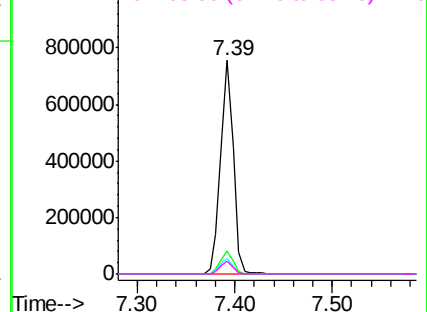


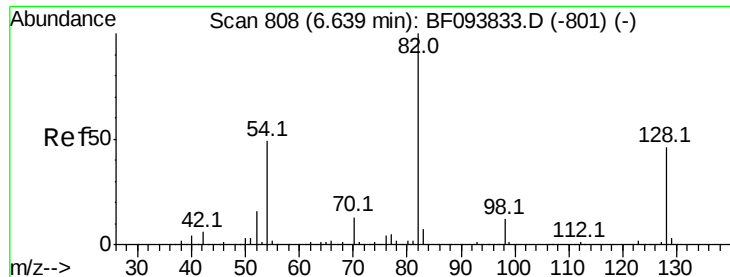




#23
Nitrobenzene-d5
Concen: 1.07 ng
RT: 6.53 min Scan# 789
Delta R.T. -0.03 min
Lab File: BF094163.D
Acq: 4 Apr 2017 12:12

Instrument :
BNA_F
ClientSampleId :
E2-W-V-4-5-BASE

Tot Ion: 82 Resp: 12988
Ion Ratio Lower Upper
82 100
128 37.8 34.0 51.0
54 47.2 42.2 63.2

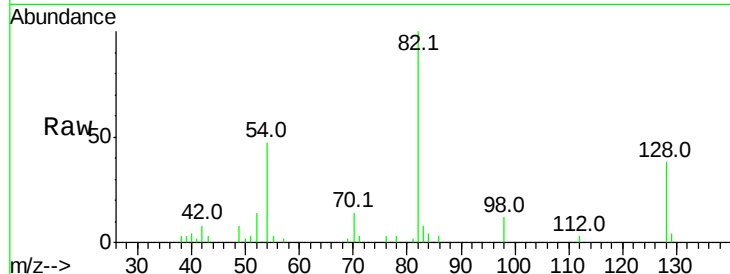


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

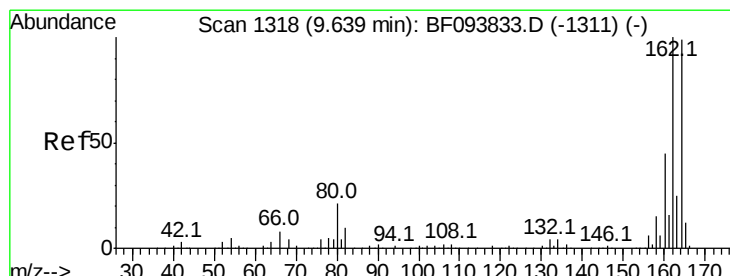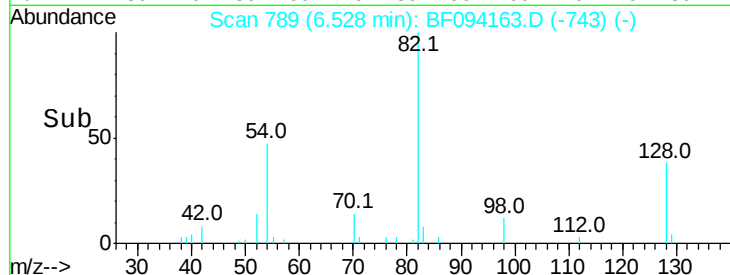
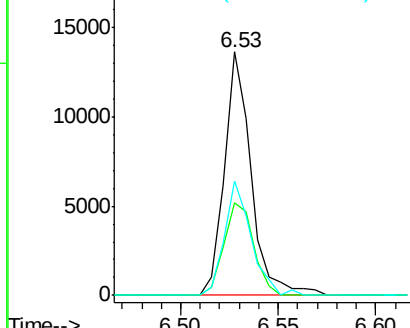


#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.53 min Scan# 1300
Delta R.T. -0.02 min
Lab File: BF094163.D
Acq: 4 Apr 2017 12:12

Tgt Ion:164 Resp: 268489
Ion Ratio Lower Upper
164 100
162 100.9 82.6 123.8
160 45.0 36.2 54.2

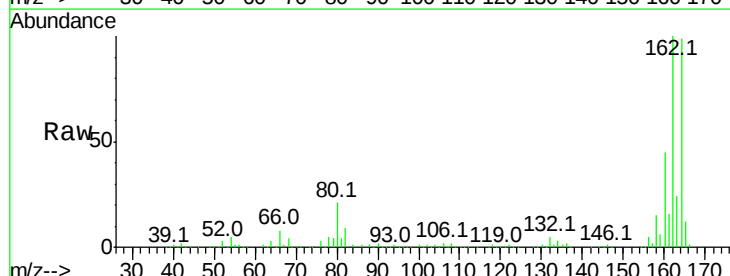

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E



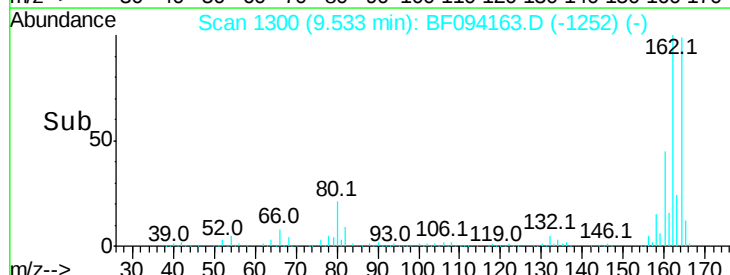
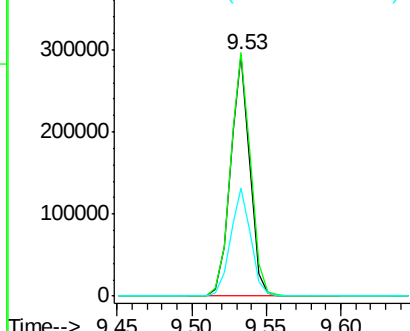




#41
 2,4,6-Tribromophenol
 Concen: 1.76 ng
 RT: 10.50 min Scan# 1465
 Delta R.T. -0.02 min
 Lab File: BF094163.D
 Acq: 4 Apr 2017 12:12




Instrument :
 BNA_F
 ClientSampleId :
 E2-W-V-4-5-BASE


Tot Ion:330 Resp: 3739
 Ion Ratio Lower Upper
 330 100
 332 102.5 76.6 115.0
 141 76.4 31.4 47.2#

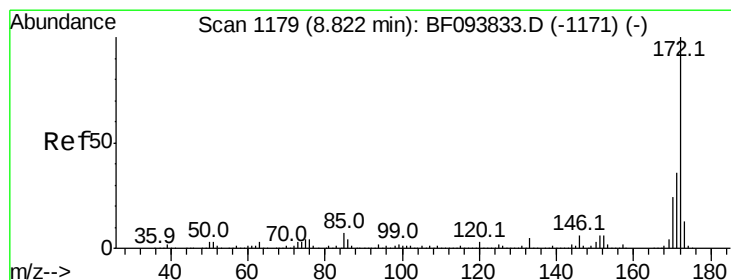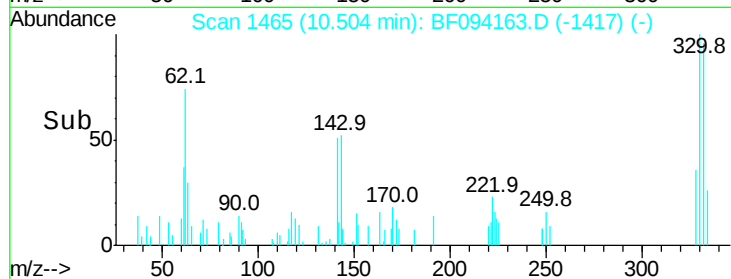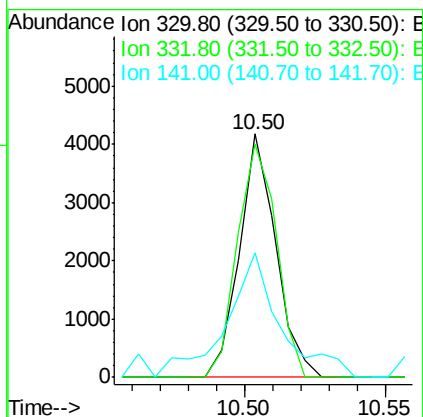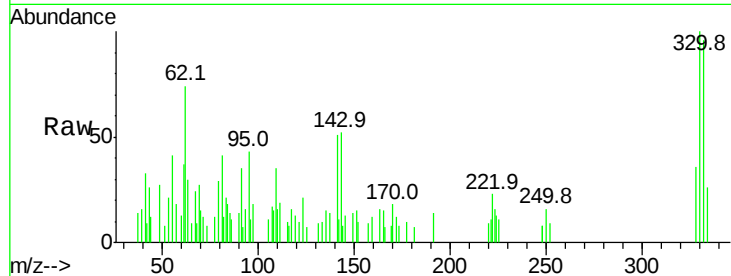

#44
 2-Fluorobiphenyl
 Concen: 2.19 ng
 RT: 8.71 min Scan# 1160
 Delta R.T. -0.02 min
 Lab File: BF094163.D
 Acq: 4 Apr 2017 12:12

Tgt Ion:172 Resp: 38632
 Ion Ratio Lower Upper
 172 100
 171 36.2 29.6 44.4
 170 23.9 19.8 29.8

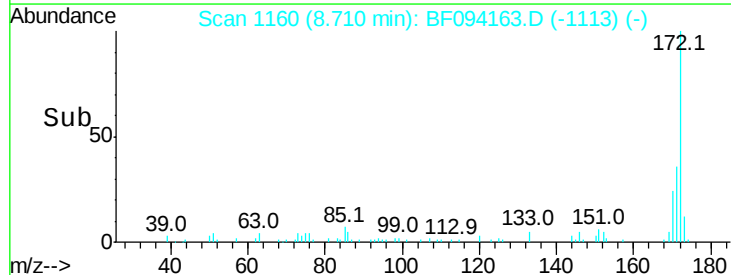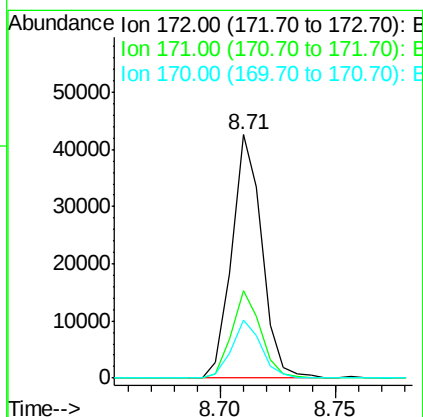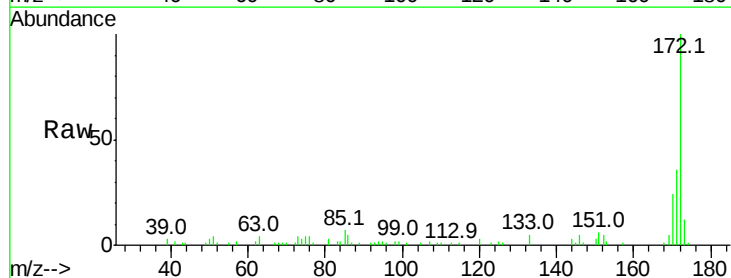


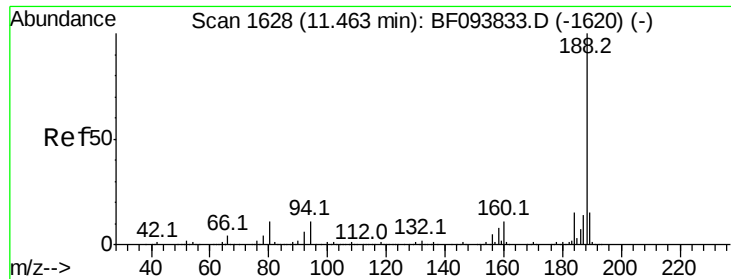




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.36 min Scan# 1610
Delta R.T. -0.02 min
Lab File: BF094163.D
Acq: 4 Apr 2017 12:12

Instrument :
BNA_F
ClientSampleId :
E2-W-V-4-5-BASE

Tot Ion:188 Resp: 423344
Ion Ratio Lower Upper
188 100
94 10.9 9.4 14.2
80 11.9 10.2 15.2

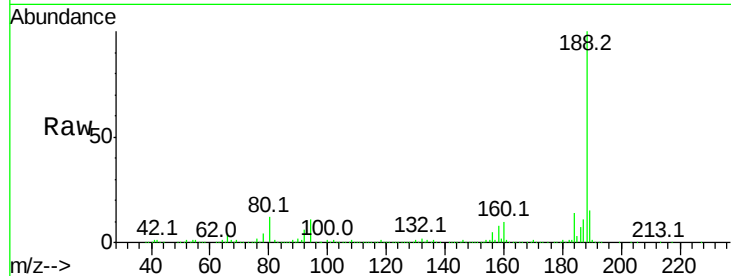


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

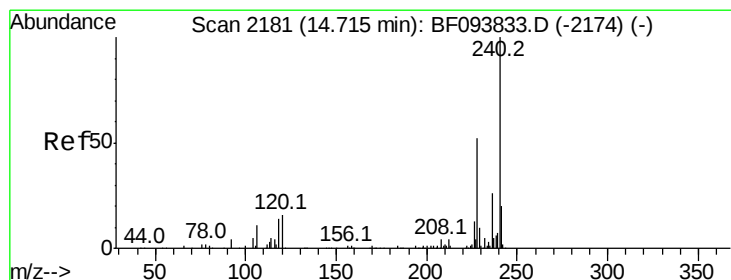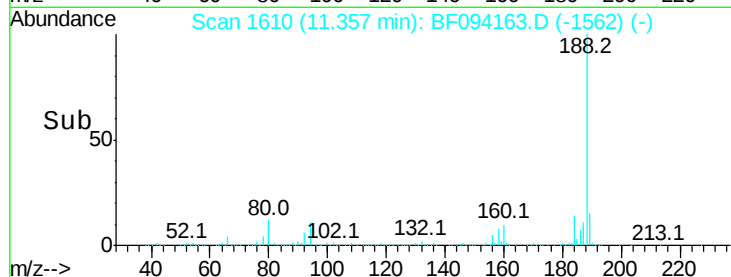
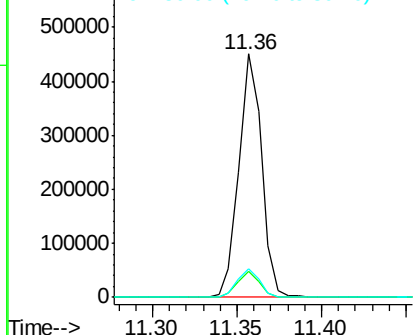



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.62 min Scan# 2164
Delta R.T. -0.01 min
Lab File: BF094163.D
Acq: 4 Apr 2017 12:12

Tgt Ion:240 Resp: 360216
Ion Ratio Lower Upper
240 100
120 14.0 5.8 8.8#
236 24.9 20.5 30.7

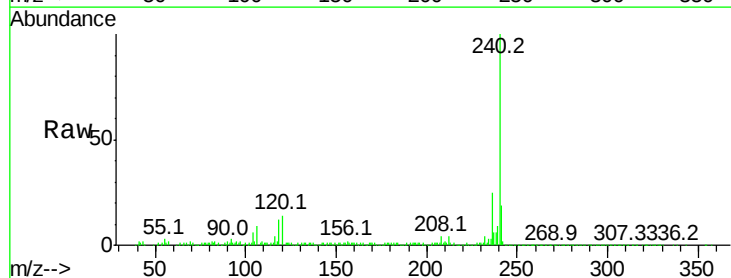

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



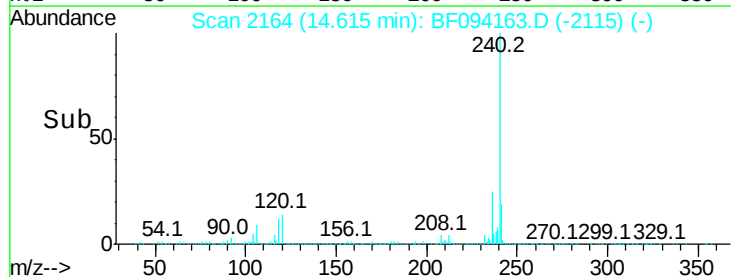
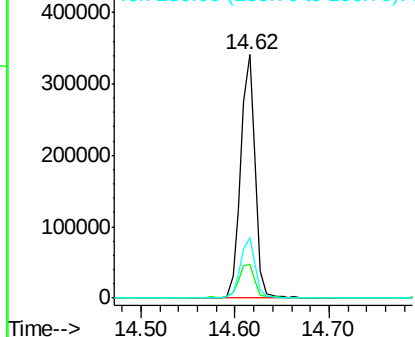


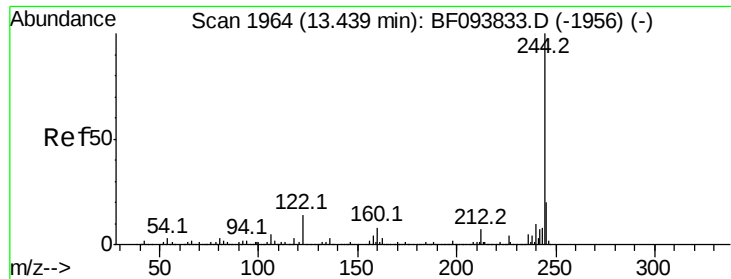

#78
 Terphenyl-d14
 Concen: 1.71 ng
 RT: 13.33 min Scan# 1946
 Delta R.T. -0.02 min
 Lab File: BF094163.D
 Acq: 4 Apr 2017 12:12

Instrument :
 BNA_F
 ClientSampleId :
 E2-W-V-4-5-BASE

Tot Ion:244 Resp: 27548
 Ion Ratio Lower Upper
 244 100
 212 9.0 6.0 9.0
 122 17.1 10.3 15.5#

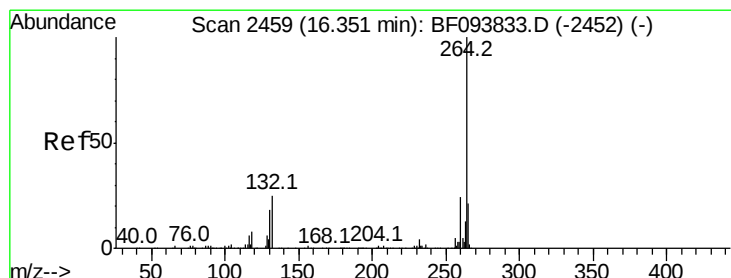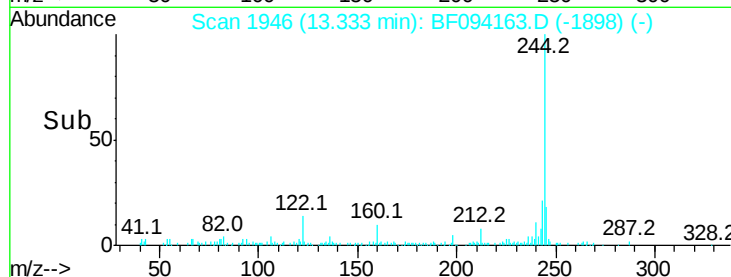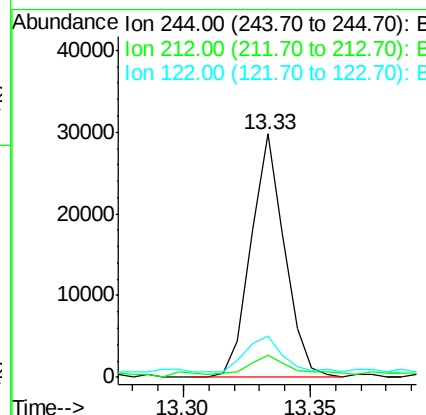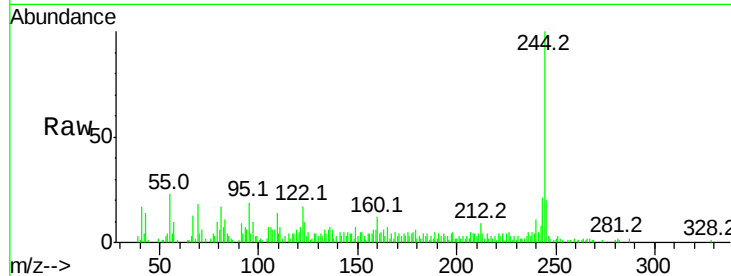

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 16.25 min Scan# 2442
 Delta R.T. -0.00 min
 Lab File: BF094163.D
 Acq: 4 Apr 2017 12:12

Tgt Ion:264 Resp: 230517
 Ion Ratio Lower Upper
 264 100
 260 24.5 19.5 29.3
 265 22.5 17.2 25.8

