

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040317\
 Data File : BF094131.D
 Acq On : 3 Apr 2017 20:00
 Operator : SJ/MA
 Sample : I2495-01 4X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LSS-SP01-COMP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.275	62	66	75	rVB3	18230	23413	1.59%	0.161%
2	3.087	198	204	211	rVB	18711	23011	1.56%	0.158%
3	4.010	358	361	368	rVB	87226	92621	6.30%	0.635%
4	4.387	421	425	426	rBV	27291	29137	1.98%	0.200%
5	4.410	426	429	433	rVB	847377	825523	56.11%	5.663%
6	4.640	465	468	474	rVB2	17922	17665	1.20%	0.121%
7	5.357	585	590	594	rBV	21653	23923	1.63%	0.164%
8	5.445	602	605	607	rBV2	15533	15485	1.05%	0.106%
9	5.487	607	612	618	rVV	889667	873971	59.40%	5.996%
10	5.534	618	620	628	rVB	15284	17242	1.17%	0.118%
11	5.628	632	636	640	rBV	1063591	927630	63.05%	6.364%
12	5.693	644	647	649	rBV	47365	40188	2.73%	0.276%
13	5.887	675	680	683	rBV	1187494	1076041	73.14%	7.382%
14	5.957	689	692	698	rBV3	14586	19593	1.33%	0.134%
15	6.063	706	710	713	rBV	822776	741229	50.38%	5.085%
16	6.263	740	744	747	rBV2	23651	22644	1.54%	0.155%
17	6.528	783	789	797	rBV	629462	575353	39.11%	3.947%
18	6.822	837	839	844	rBV2	18058	15846	1.08%	0.109%
19	7.081	880	883	889	rBV5	13600	20113	1.37%	0.138%
20	7.287	915	918	921	rBV	25163	21926	1.49%	0.150%
21	7.387	930	935	939	rBV	1450085	1430997	97.26%	9.817%
22	7.822	1005	1009	1011	rBV	14684	15119	1.03%	0.104%
23	8.257	1079	1083	1086	rBV	46804	41732	2.84%	0.286%
24	8.322	1090	1094	1100	rVV	25619	35208	2.39%	0.242%
25	8.375	1100	1103	1109	rVB	25653	23450	1.59%	0.161%
26	8.710	1152	1160	1164	rBV	1204007	1042739	70.87%	7.153%
27	9.022	1211	1213	1220	rVB4	11493	16135	1.10%	0.111%
28	9.204	1241	1244	1248	rBV	77590	75978	5.16%	0.521%
29	9.351	1265	1269	1274	rVB	26188	32313	2.20%	0.222%
30	9.528	1292	1299	1304	rBV2	1385851	1471288	100.00%	10.093%
31	9.792	1340	1344	1348	rBV6	10920	18569	1.26%	0.127%
32	10.122	1396	1400	1403	rBV	30284	26284	1.79%	0.180%
33	10.204	1411	1414	1418	rBV4	16477	17937	1.22%	0.123%
34	10.498	1460	1464	1470	rBV	501023	471092	32.02%	3.232%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040317\
Data File : BF094131.D
Acq On : 3 Apr 2017 20:00
Operator : SJ/MA
Sample : I2495-01 4X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SP01-COMP

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.710	1496	1500	1502	rBV	32411	41818	2.84%	0.287%
36	11.069	1555	1561	1564	rBV7	12599	23861	1.62%	0.164%
37	11.110	1564	1568	1572	rBV7	24558	32354	2.20%	0.222%
38	11.192	1578	1582	1584	rBV4	13636	20135	1.37%	0.138%
39	11.263	1591	1594	1597	rVB2	25744	26636	1.81%	0.183%
40	11.357	1605	1610	1613	rBV	1165515	1248100	84.83%	8.562%
41	11.380	1613	1614	1618	rVB	92899	58038	3.94%	0.398%
42	11.445	1622	1625	1629	rVV	29595	30465	2.07%	0.209%
43	12.016	1719	1722	1725	rBV2	30005	31303	2.13%	0.215%
44	12.104	1734	1737	1740	rBV2	43869	58479	3.97%	0.401%
45	12.845	1860	1863	1866	rVB	152569	150454	10.23%	1.032%
46	13.121	1907	1910	1914	rVB	161539	162906	11.07%	1.118%
47	13.327	1942	1945	1952	rVB	596746	616185	41.88%	4.227%
48	14.610	2159	2163	2166	rBV	769271	835629	56.80%	5.733%
49	16.245	2437	2441	2455	rVB	773595	1119188	76.07%	7.678%


Sum of corrected areas: 14576946

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040317\
Data File : BF094131.D
Acq On : 3 Apr 2017 20:00
Operator : SJ/MA
Sample : I2495-01 4X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SP01-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

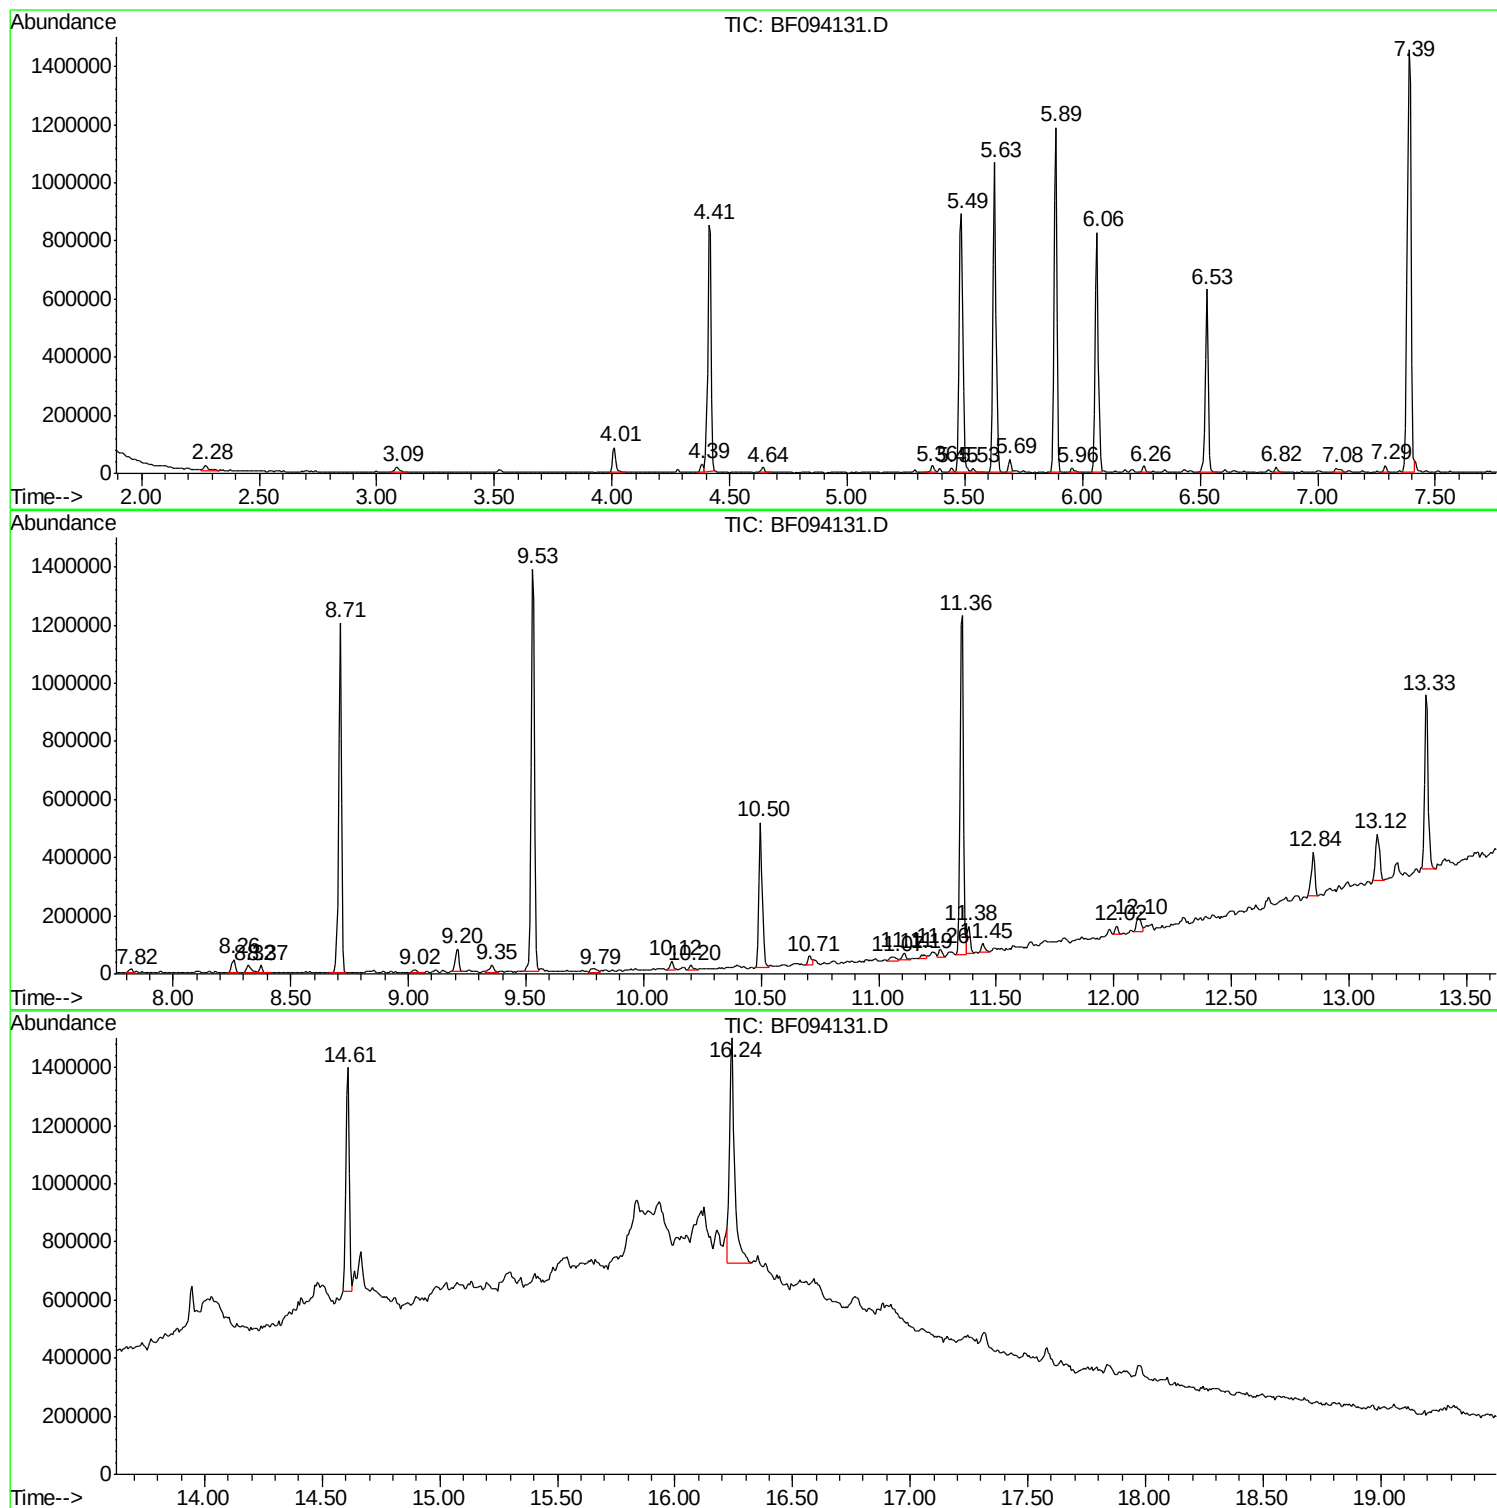

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040317\
Data File : BF094131.D
Acq On : 3 Apr 2017 20:00
Operator : SJ/MA
Sample : I2495-01 4X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SP01-COMP










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.63 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.63	17.24 ng	927630	1,4-Dichlorobenzene-d4	5.89

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
2		5-Aminoindole	132	C8H8N2	005192-03-0	10
3		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
4		1-Aminoindan	133	C9H11N	034698-41-4	9
5		Xenon	132	Xe	007440-63-3	9

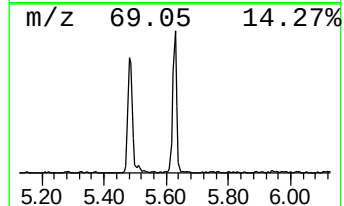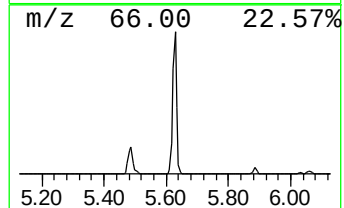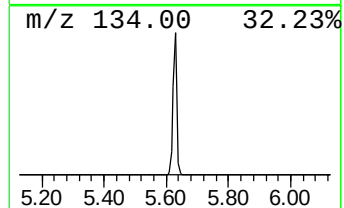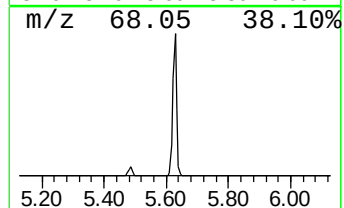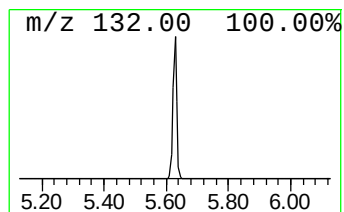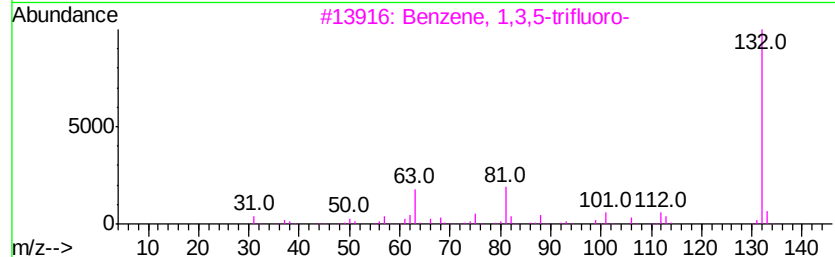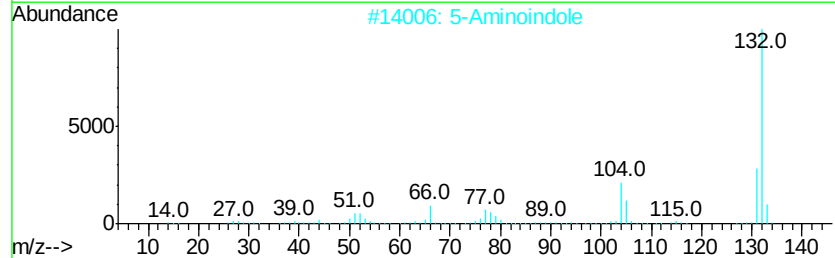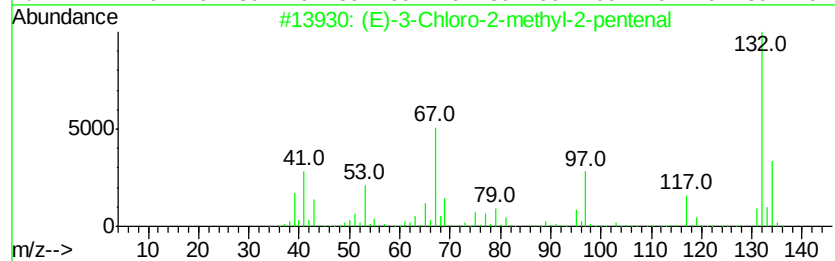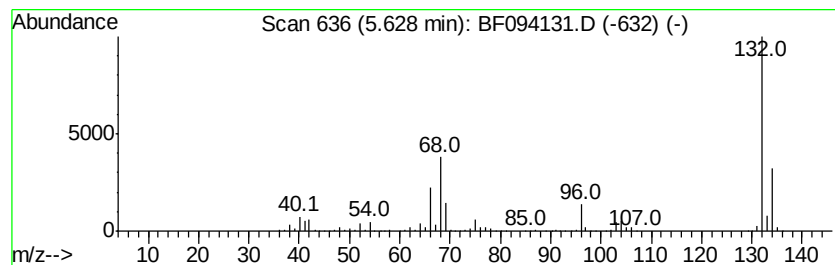

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040317\
Data File : BF094131.D
Acq On : 3 Apr 2017 20:00
Operator : SJ/MA
Sample : I2495-01 4X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SP01-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.63	5.63	17.2	ng	927630	1	5.89	1076040	20.0