

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040317\
 Data File : BF094142.D
 Acq On : 4 Apr 2017 1:03
 Operator : SJ/MA
 Sample : I2495-06 5X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LSS-SP03-COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.263	60	64	68	rBV	75155	84512	6.72%	0.697%
2	4.010	358	361	370	rVB	52256	52150	4.14%	0.430%
3	4.387	419	425	426	rBV	16822	19120	1.52%	0.158%
4	4.416	426	430	436	rVB	752168	681905	54.19%	5.627%
5	4.640	462	468	475	rBV6	13022	23718	1.88%	0.196%
6	5.381	588	594	602	rVB2	22636	42162	3.35%	0.348%
7	5.492	609	613	619	rBV	760212	797800	63.40%	6.584%
8	5.634	632	637	641	rBV	790966	743405	59.08%	6.135%
9	5.692	645	647	654	rVB	30233	33161	2.64%	0.274%
10	5.886	676	680	684	rBV	1079756	968151	76.94%	7.990%
11	5.957	690	692	699	rBV4	11267	16896	1.34%	0.139%
12	6.063	706	710	714	rBV	652821	593935	47.20%	4.901%
13	6.263	740	744	749	rBV2	19077	19589	1.56%	0.162%
14	6.528	784	789	793	rBV	363537	344656	27.39%	2.844%
15	6.822	837	839	842	rBV	15577	14957	1.19%	0.123%
16	7.086	879	884	890	rBV5	13427	25172	2.00%	0.208%
17	7.292	915	919	924	rBV5	17283	19013	1.51%	0.157%
18	7.392	931	936	939	rBV	1420790	1258314	100.00%	10.384%
19	7.822	1004	1009	1012	rBV	19184	22718	1.81%	0.187%
20	8.263	1079	1084	1088	rVB	30679	30015	2.39%	0.248%
21	8.322	1089	1094	1099	rBV	32730	42960	3.41%	0.355%
22	8.380	1101	1104	1107	rVB	16304	16127	1.28%	0.133%
23	8.710	1156	1160	1164	rVB	872009	815338	64.80%	6.728%
24	9.210	1239	1245	1248	rBV	55856	52059	4.14%	0.430%
25	9.357	1262	1270	1276	rBV2	38976	78829	6.26%	0.651%
26	9.533	1296	1300	1304	rVB2	1259620	1206992	95.92%	9.961%
27	9.574	1304	1307	1313	rVB3	15286	22220	1.77%	0.183%
28	9.786	1339	1343	1348	rVB6	10473	18935	1.50%	0.156%
29	10.127	1397	1401	1404	rBV	25709	23860	1.90%	0.197%
30	10.210	1412	1415	1420	rVB5	16317	20751	1.65%	0.171%
31	10.504	1461	1465	1470	rBV	311027	298593	23.73%	2.464%
32	10.592	1476	1480	1485	rBV6	24604	38586	3.07%	0.318%
33	10.710	1497	1500	1503	rBV	29692	32528	2.59%	0.268%
34	11.110	1564	1568	1572	rVB5	36462	42498	3.38%	0.351%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040317\
Data File : BF094142.D
Acq On : 4 Apr 2017 1:03
Operator : SJ/MA
Sample : I2495-06 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SP03-COMP

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.268	1593	1595	1597	rVB2	25562	18862	1.50%	0.156%
36	11.304	1599	1601	1605	rVV5	19102	22949	1.82%	0.189%
37	11.357	1606	1610	1613	rVV	1018369	994513	79.04%	8.207%
38	11.386	1613	1615	1618	rVB	108360	91747	7.29%	0.757%
39	11.451	1623	1626	1629	rVB	33193	32740	2.60%	0.270%
40	12.851	1861	1864	1867	rBV	152221	144473	11.48%	1.192%
41	13.127	1908	1911	1914	rVB	164253	176978	14.06%	1.460%
42	13.333	1943	1946	1950	rVB	482141	501192	39.83%	4.136%
43	13.945	2048	2050	2056	rVB	184580	175964	13.98%	1.452%
44	14.615	2160	2164	2167	rBV	780180	812734	64.59%	6.707%
45	16.251	2439	2442	2449	rVB	550702	643943	51.18%	5.314%


Sum of corrected areas: 12117720

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040317\
Data File : BF094142.D
Acq On : 4 Apr 2017 1:03
Operator : SJ/MA
Sample : I2495-06 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SP03-COMP

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

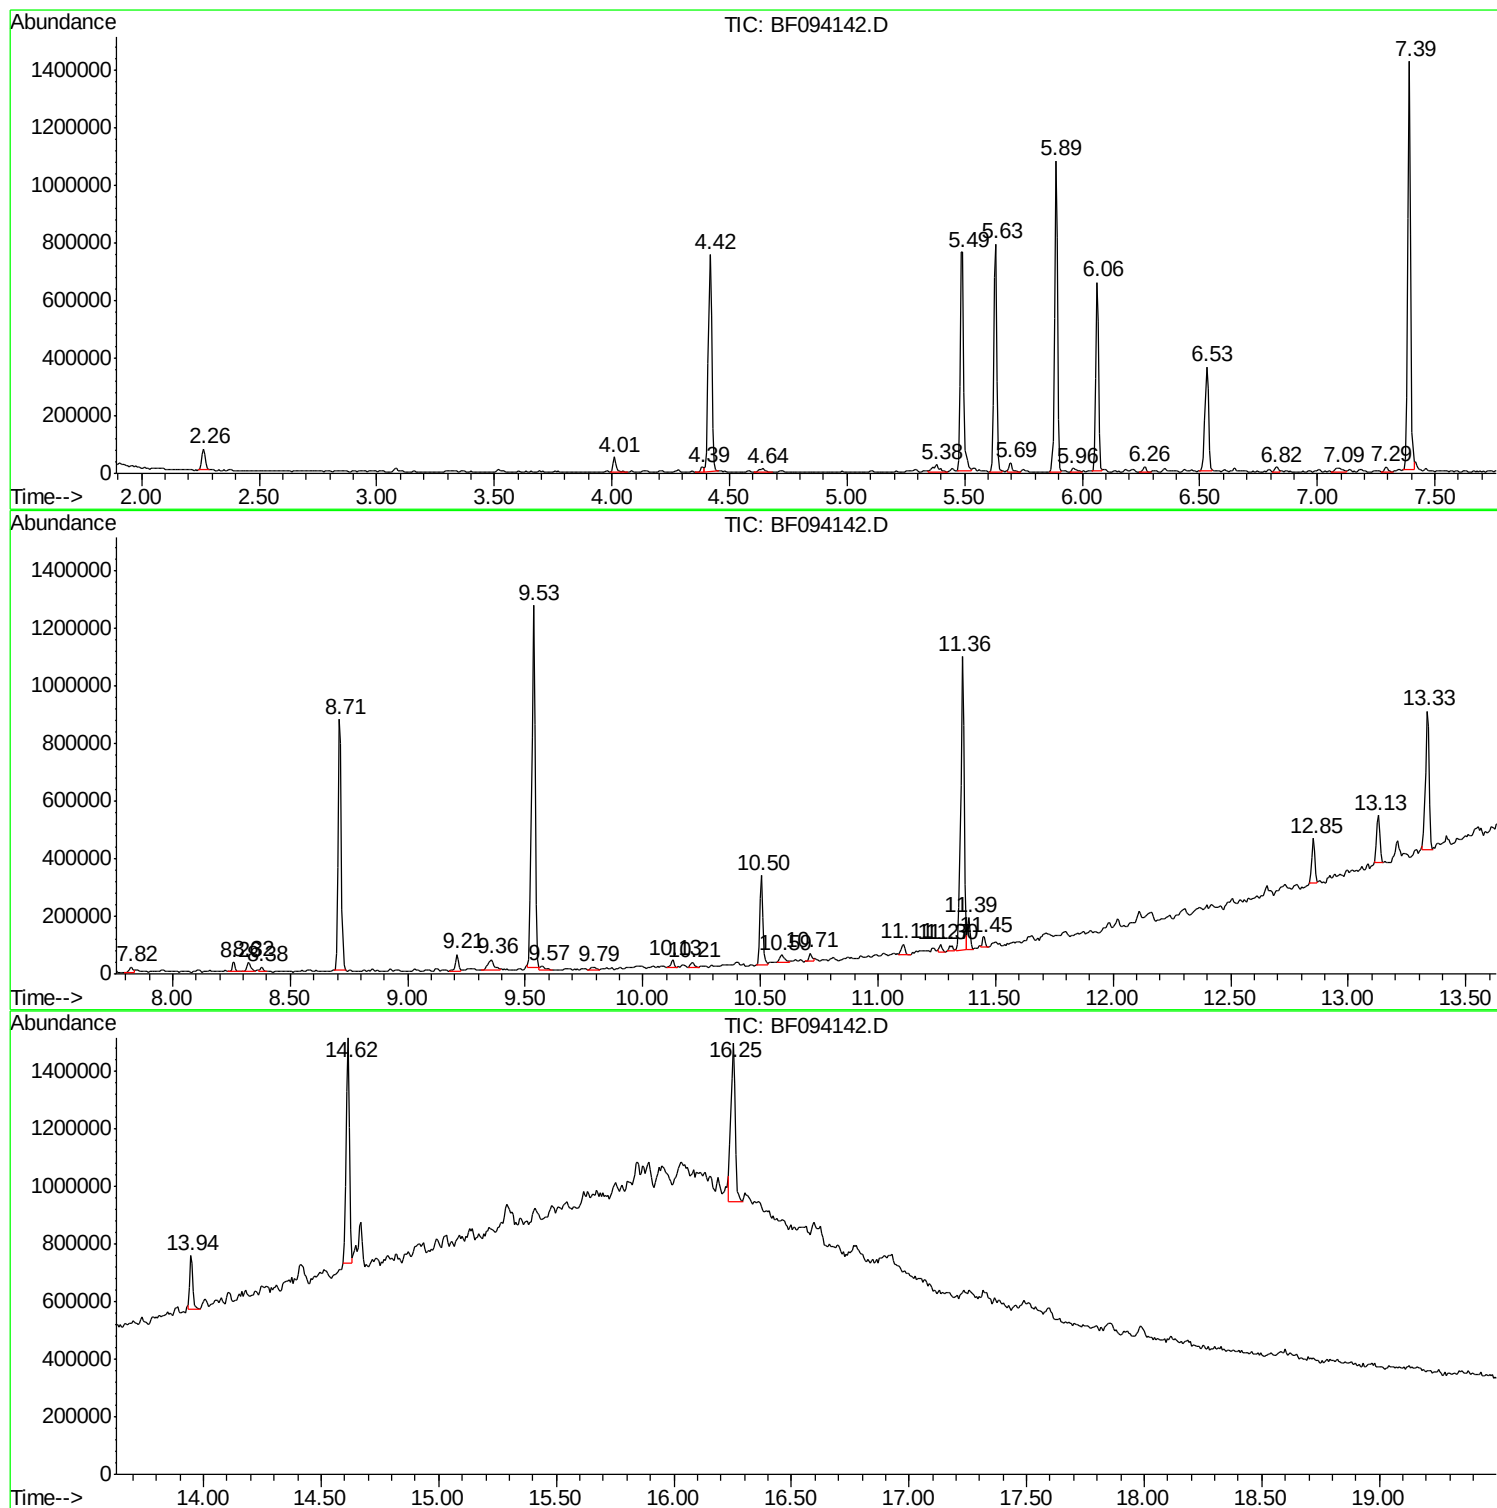

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040317\
Data File : BF094142.D
Acq On : 4 Apr 2017 1:03
Operator : SJ/MA
Sample : I2495-06 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SP03-COMP










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.63 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.63	15.36 ng	743405	1,4-Dichlorobenzene-d4	5.89

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	35
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9

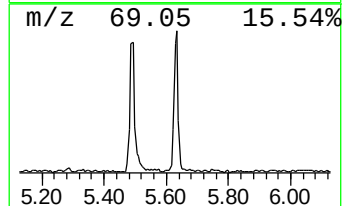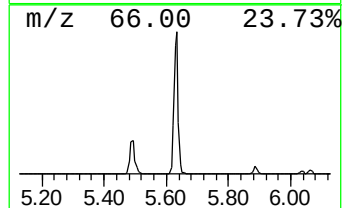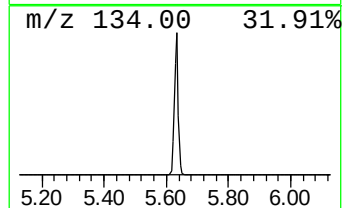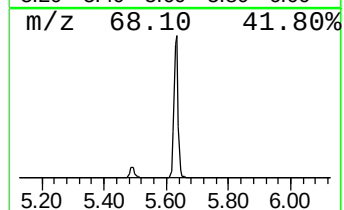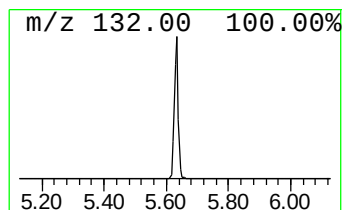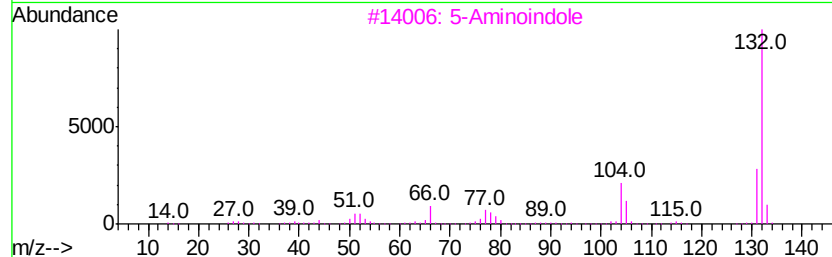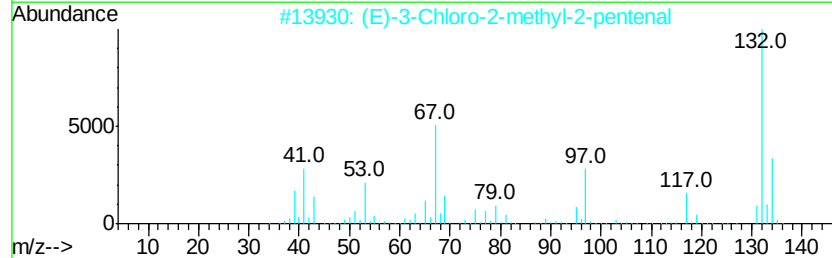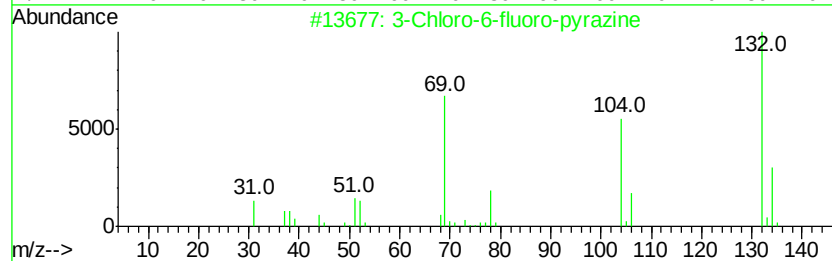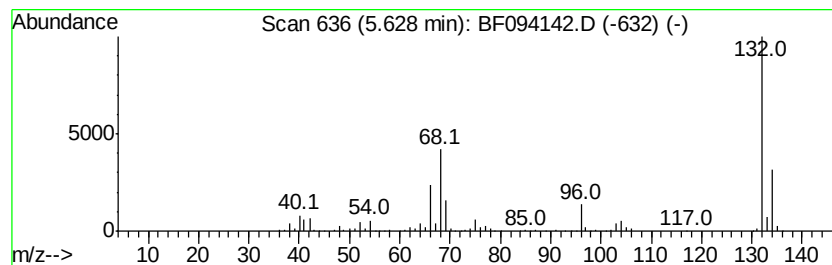

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040317\
Data File : BF094142.D
Acq On : 4 Apr 2017 1:03
Operator : SJ/MA
Sample : I2495-06 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SP03-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.63	5.63	15.4	ng	743405	1	5.89	968151	20.0