

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040317\
 Data File : BF094143.D
 Acq On : 4 Apr 2017 1:31
 Operator : SJ/MA
 Sample : I2495-08 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LSS-SP04-COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.263	60	64	69	rBV	57573	72420	7.44%	0.667%
2	3.081	199	203	208	rBV	23026	26502	2.72%	0.244%
3	4.010	358	361	370	rBV	47585	53960	5.55%	0.497%
4	4.281	403	407	410	rBV	17595	15469	1.59%	0.142%
5	4.387	422	425	427	rBV	46399	50959	5.24%	0.469%
6	4.416	427	430	436	rVB	749254	723215	74.33%	6.661%
7	4.645	462	469	473	rBV2	24670	33776	3.47%	0.311%
8	5.363	588	591	594	rBV	30822	27642	2.84%	0.255%
9	5.398	594	597	601	rVB	19043	16531	1.70%	0.152%
10	5.445	601	605	608	rBV2	14546	14233	1.46%	0.131%
11	5.487	608	612	619	rBV	838872	870103	89.43%	8.014%
12	5.634	633	637	641	rBV	823211	768260	78.96%	7.076%
13	5.692	644	647	650	rBV	40989	40633	4.18%	0.374%
14	5.886	676	680	684	rBV	845886	752763	77.37%	6.934%
15	6.063	706	710	714	rBV	717840	639277	65.70%	5.888%
16	6.263	741	744	747	rBV	23248	20263	2.08%	0.187%
17	6.528	784	789	794	rBV	346222	337369	34.67%	3.107%
18	6.828	837	840	845	rBV3	17473	18159	1.87%	0.167%
19	7.086	880	884	890	rBV6	15566	26524	2.73%	0.244%
20	7.292	915	919	925	rBV2	22298	25034	2.57%	0.231%
21	7.392	932	936	939	rBV	1104013	972970	100.00%	8.962%
22	7.416	939	940	943	rVB	38273	23340	2.40%	0.215%
23	7.822	1003	1009	1012	rBV3	27488	34621	3.56%	0.319%
24	8.263	1080	1084	1087	rVB	43018	41562	4.27%	0.383%
25	8.322	1091	1094	1100	rVV	47708	59555	6.12%	0.549%
26	8.380	1100	1104	1108	rVB	23591	26466	2.72%	0.244%
27	8.710	1156	1160	1164	rBV	892525	852418	87.61%	7.852%
28	9.027	1211	1214	1219	rVB3	10076	16075	1.65%	0.148%
29	9.122	1227	1230	1233	rBV4	13662	15123	1.55%	0.139%
30	9.210	1242	1245	1248	rVB	50611	42009	4.32%	0.387%
31	9.357	1263	1270	1276	rBV2	40304	73049	7.51%	0.673%
32	9.533	1296	1300	1305	rVB2	924513	880747	90.52%	8.113%
33	9.798	1340	1345	1348	rBV7	10945	14958	1.54%	0.138%
34	10.127	1398	1401	1404	rVB	21462	20486	2.11%	0.189%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040317\
Data File : BF094143.D
Acq On : 4 Apr 2017 1:31
Operator : SJ/MA
Sample : I2495-08 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SP04-COMP

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.204	1412	1414	1420	rBV7	16401	18755	1.93%	0.173%
36	10.504	1461	1465	1470	rBV	325875	308398	31.70%	2.841%
37	10.592	1476	1480	1485	rVB6	22720	37376	3.84%	0.344%
38	10.710	1497	1500	1502	rBV2	29827	31417	3.23%	0.289%
39	10.769	1508	1510	1512	rBV3	13462	14522	1.49%	0.134%
40	11.110	1565	1568	1574	rVB6	32710	40306	4.14%	0.371%
41	11.268	1593	1595	1598	rVB3	28247	23294	2.39%	0.215%
42	11.310	1598	1602	1605	rBV3	28312	37198	3.82%	0.343%
43	11.357	1606	1610	1613	rBV	705107	711356	73.11%	6.552%
44	11.386	1613	1615	1620	rVB	83018	70344	7.23%	0.648%
45	11.451	1623	1626	1629	rVB2	35117	39784	4.09%	0.366%
46	12.851	1861	1864	1867	rBV	146518	137923	14.18%	1.270%
47	13.127	1908	1911	1915	rVB	167209	160592	16.51%	1.479%
48	13.333	1943	1946	1952	rVB	508264	542799	55.79%	5.000%
49	14.615	2160	2164	2167	rBV	633868	674775	69.35%	6.215%
50	16.250	2440	2442	2446	rVB	389671	401355	41.25%	3.697%


Sum of corrected areas: 10856665

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040317\
Data File : BF094143.D
Acq On : 4 Apr 2017 1:31
Operator : SJ/MA
Sample : I2495-08 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
LSS-SP04-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

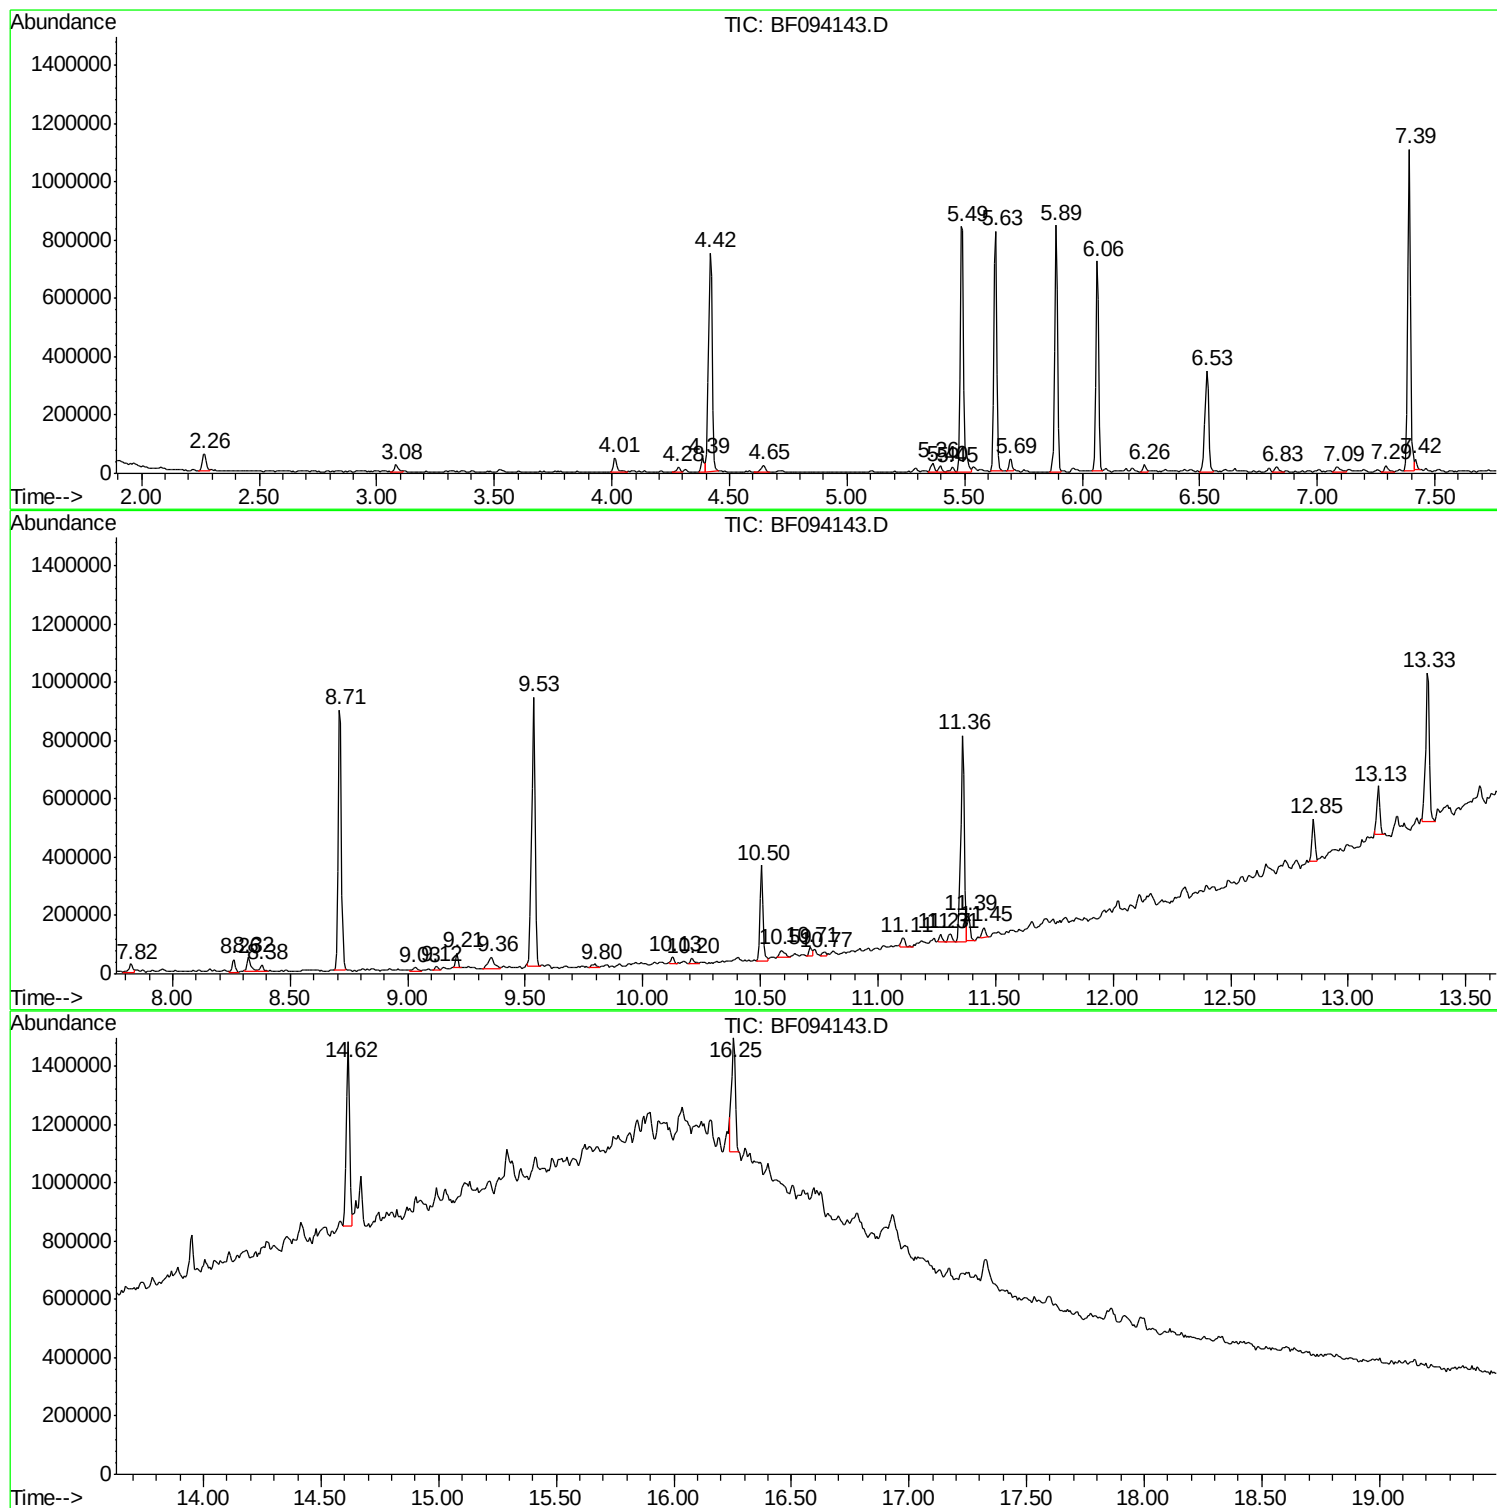

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040317\
Data File : BF094143.D
Acq On : 4 Apr 2017 1:31
Operator : SJ/MA
Sample : I2495-08 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SP04-COMP










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.63 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.63	20.41 ng	768260	1,4-Dichlorobenzene-d4	5.89

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		Xenon	132	Xe	007440-63-3	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

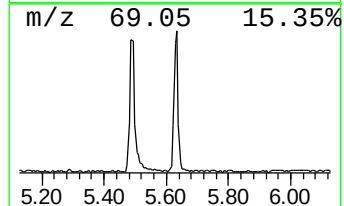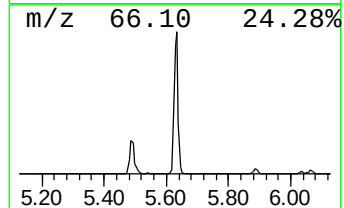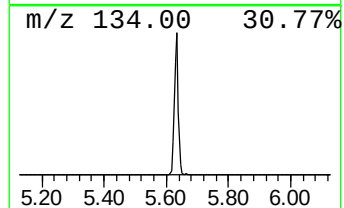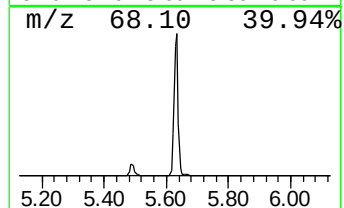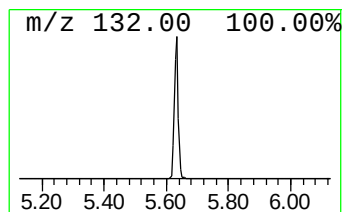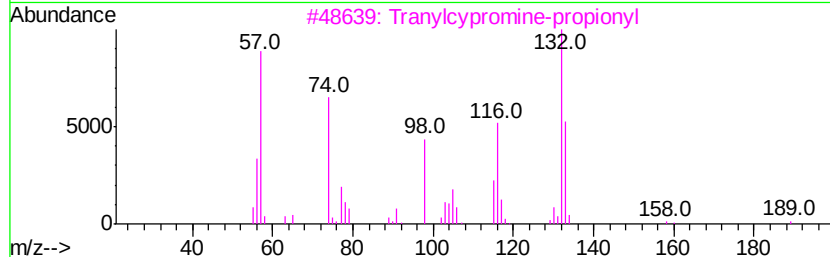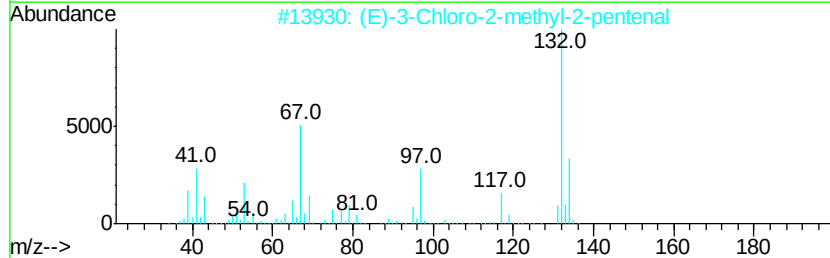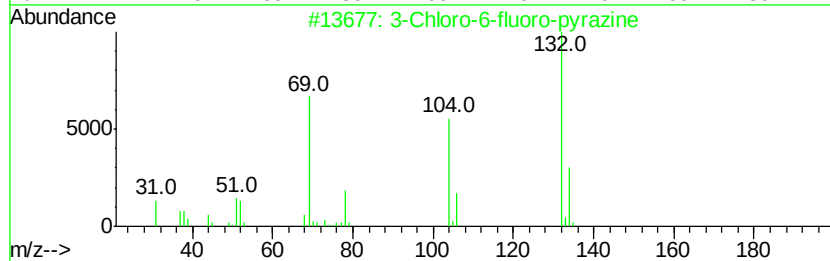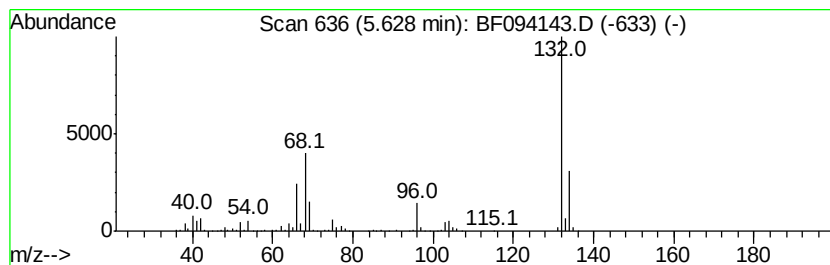

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040317\
Data File : BF094143.D
Acq On : 4 Apr 2017 1:31
Operator : SJ/MA
Sample : I2495-08 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SP04-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.63	5.63	20.4	ng	768260	1	5.89	752763	20.0