


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040317\
 Data File : BF094117.D
 Acq On : 3 Apr 2017 13:28
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 31 14:38:29 2017

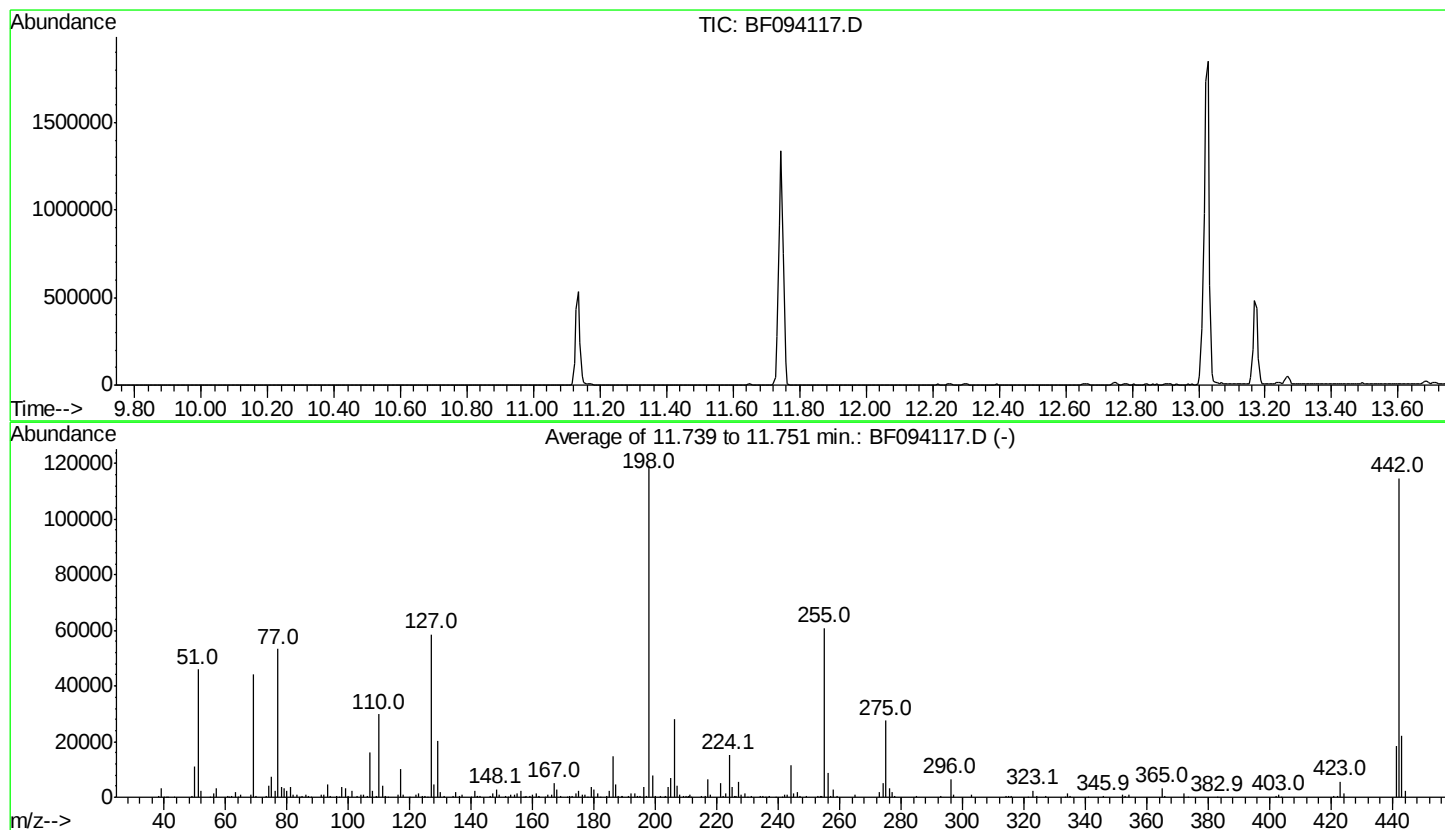

AutoFind: Scans 1675, 1676, 1677; Background Corrected with Scan 1669

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	46013	PASS
68	69	0.00	2	1.8	814	PASS
69	198	0.00	100	37.2	44322	PASS
70	69	0.00	2	0.7	310	PASS
127	198	10	80	49.2	58626	PASS
197	198	0.00	2	0.3	409	PASS
198	198	100	100	100.0	119253	PASS
199	198	5	9	6.5	7787	PASS
275	198	10	60	23.1	27501	PASS
365	198	1	100	2.7	3230	PASS
441	442	0.01	24	15.9	18251	PASS
442	198	50	100	96.2	114768	PASS
443	442	15	24	19.1	21918	PASS