


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040317\
 Data File : BF094144.D
 Acq On : 4 Apr 2017 3:22
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 31 14:38:29 2017

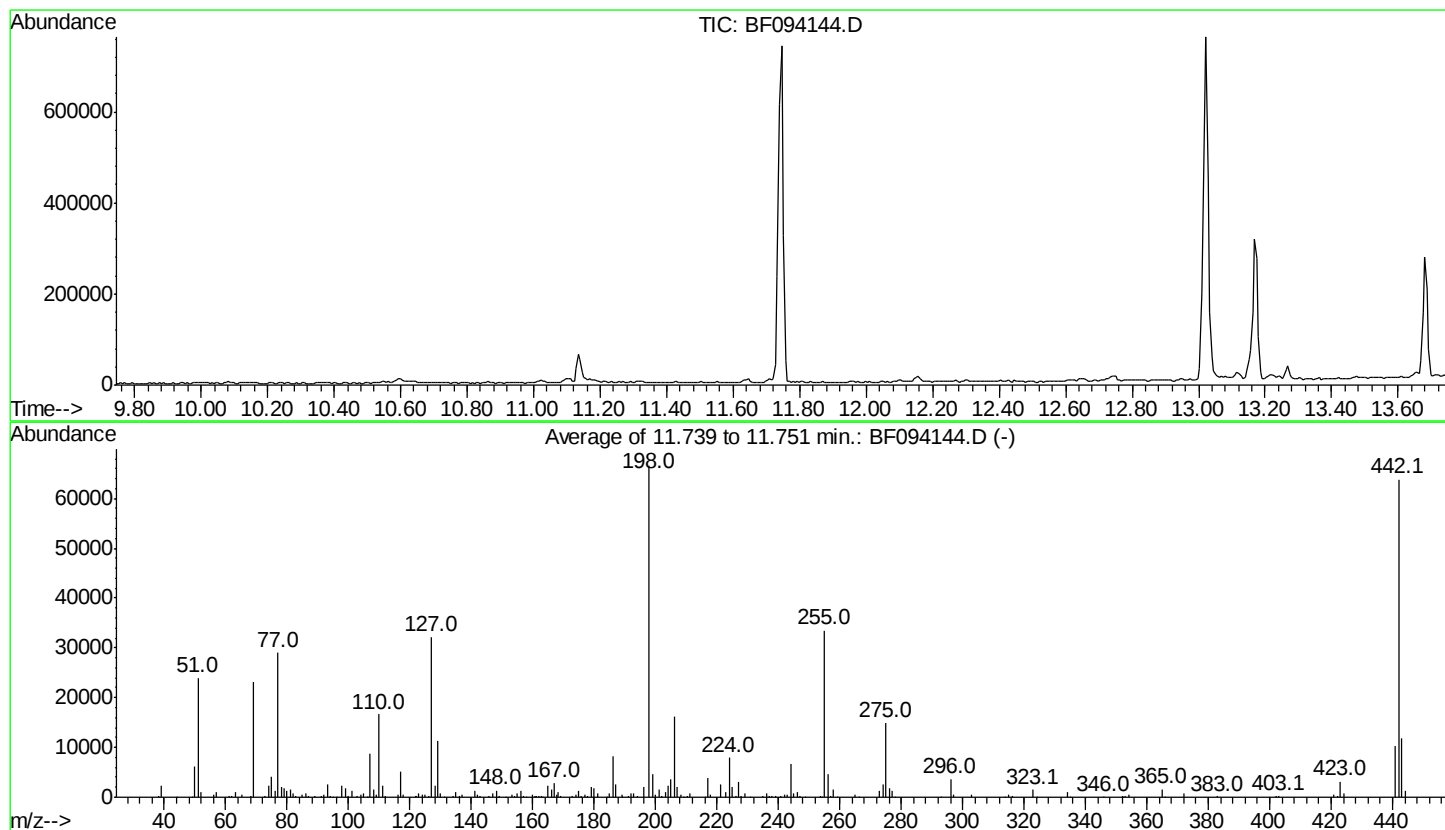

AutoFind: Scans 1675, 1676, 1677; Background Corrected with Scan 1670

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	24029	PASS
68	69	0.00	2	1.1	252	PASS
69	198	0.00	100	34.8	23164	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.3	32208	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	66616	PASS
199	198	5	9	6.9	4599	PASS
275	198	10	60	22.4	14947	PASS
365	198	1	100	2.4	1603	PASS
441	442	0.01	24	16.1	10276	PASS
442	198	50	100	95.9	63874	PASS
443	442	15	24	18.6	11860	PASS