
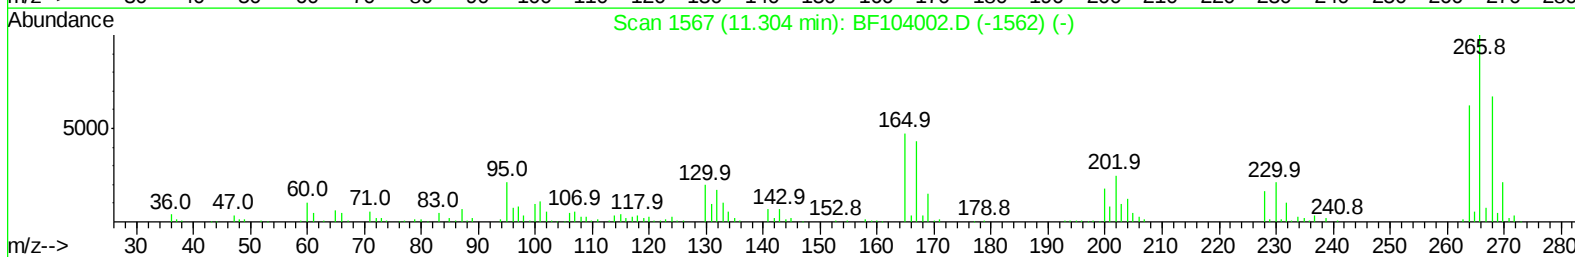
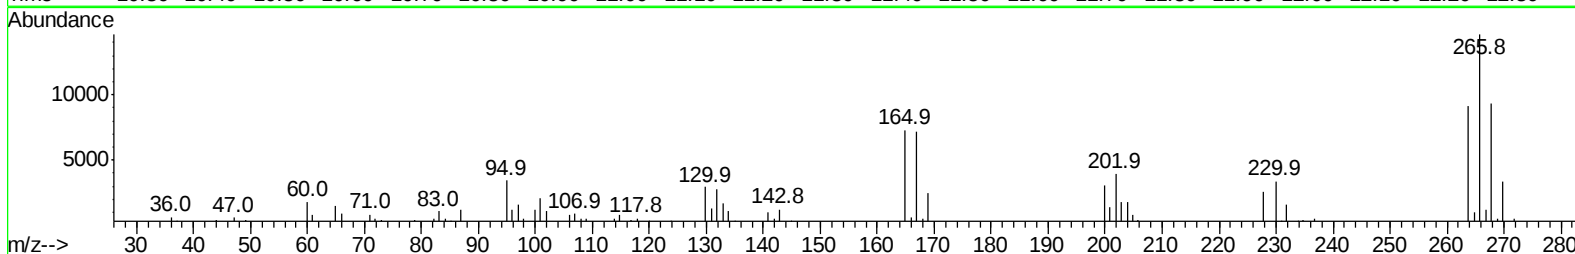


Data Path : Z:\HPCHEM1\BNA F\DATA\BF040318\
Data File : BF104174.D
Acq On : 3 Apr 2018 11:00
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 03:46:35 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 03 15:22:43 2018
Response via : Initial Calibration

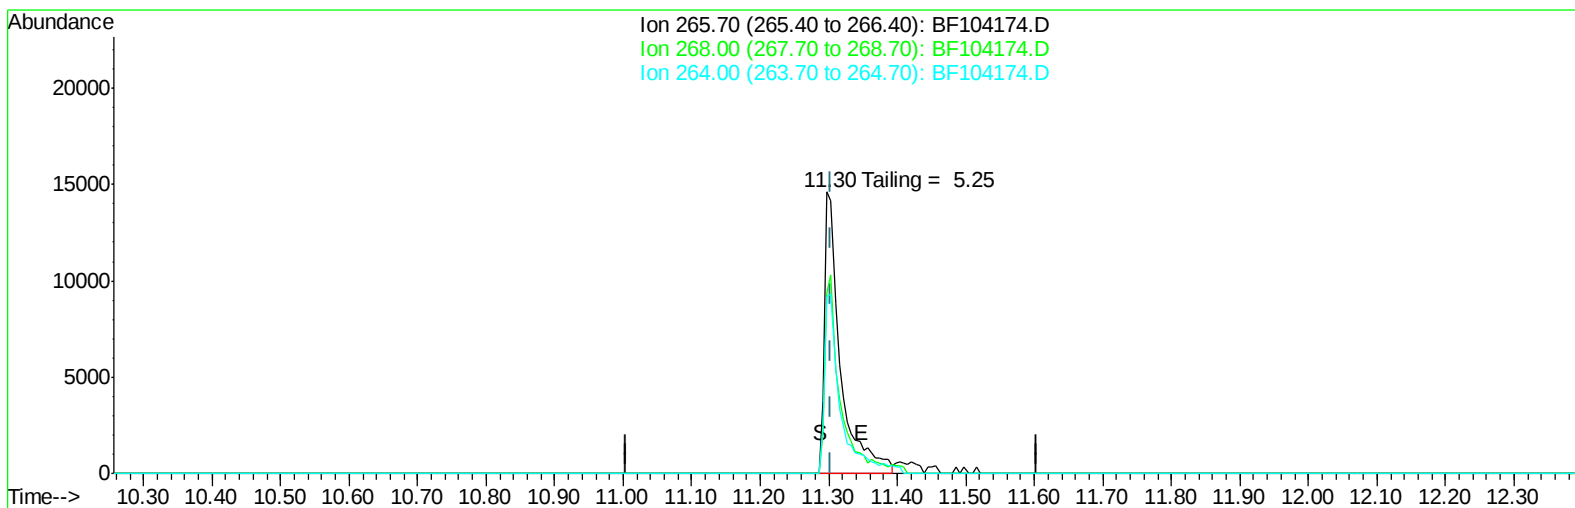

TIC: BF104174.D

(69) Pentachlorophenol (C)




11.298min (-0.006) 0.00ng

response 23360

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.14
264.00	61.90	62.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040318\
Data File : BF104174.D
Acq On : 3 Apr 2018 11:00
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 03:46:35 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 03 15:22:43 2018
Response via : Initial Calibration

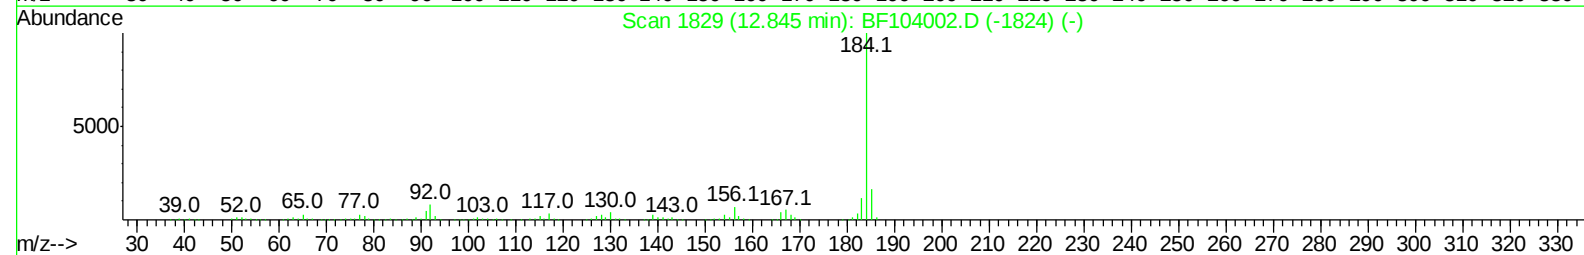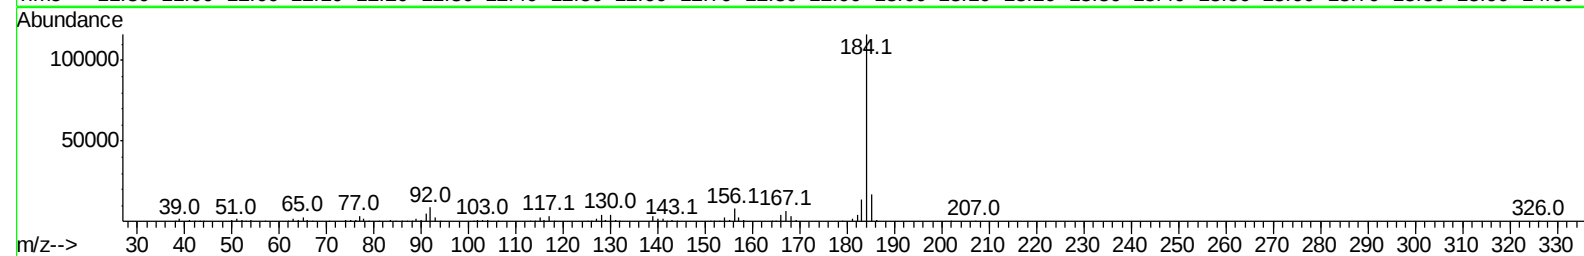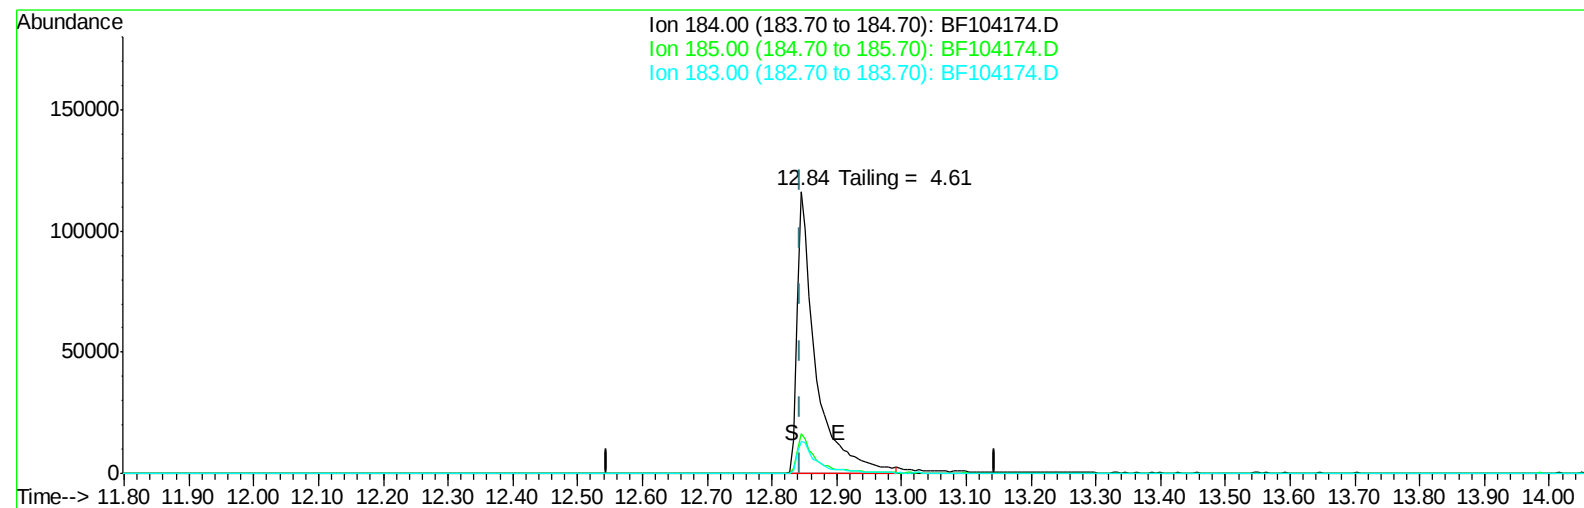

TIC: BF104174.D

(76) Benzidine

12.845min (-0.000) 0.00ng

response 236410

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.31
183.00	11.60	11.60
0.00	0.00	0.00