
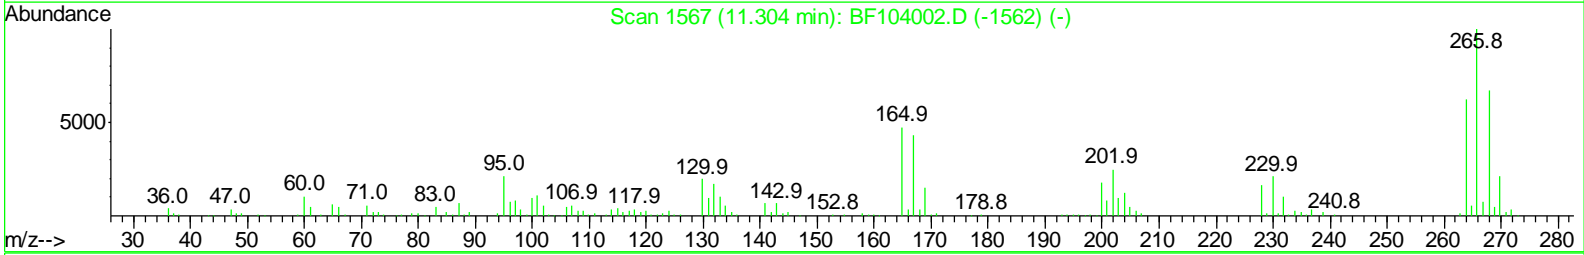
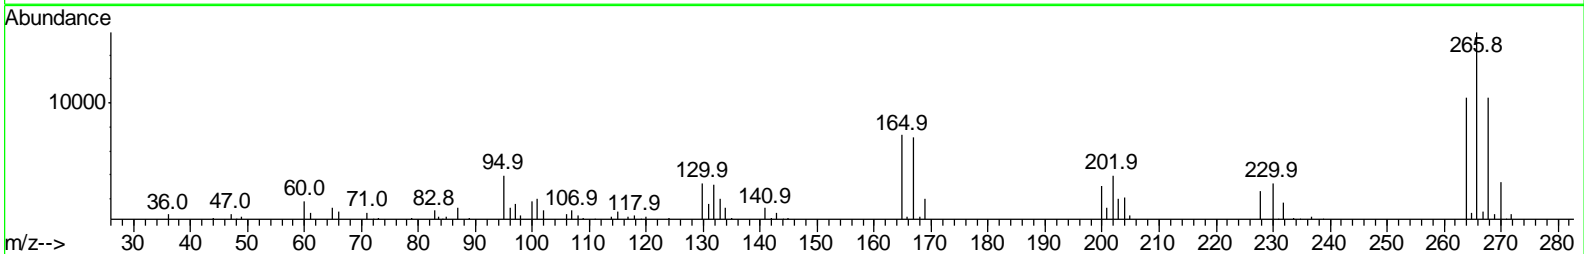


Data Path : Z:\HPCHEM1\BNA F\DATA\BF040318\
 Data File : BF104210.D
 Acq On : 4 Apr 2018 6:34
 Operator : JU/SJ
 Sample : DF7PP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 08:53:46 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 03 15:22:43 2018
 Response via : Initial Calibration

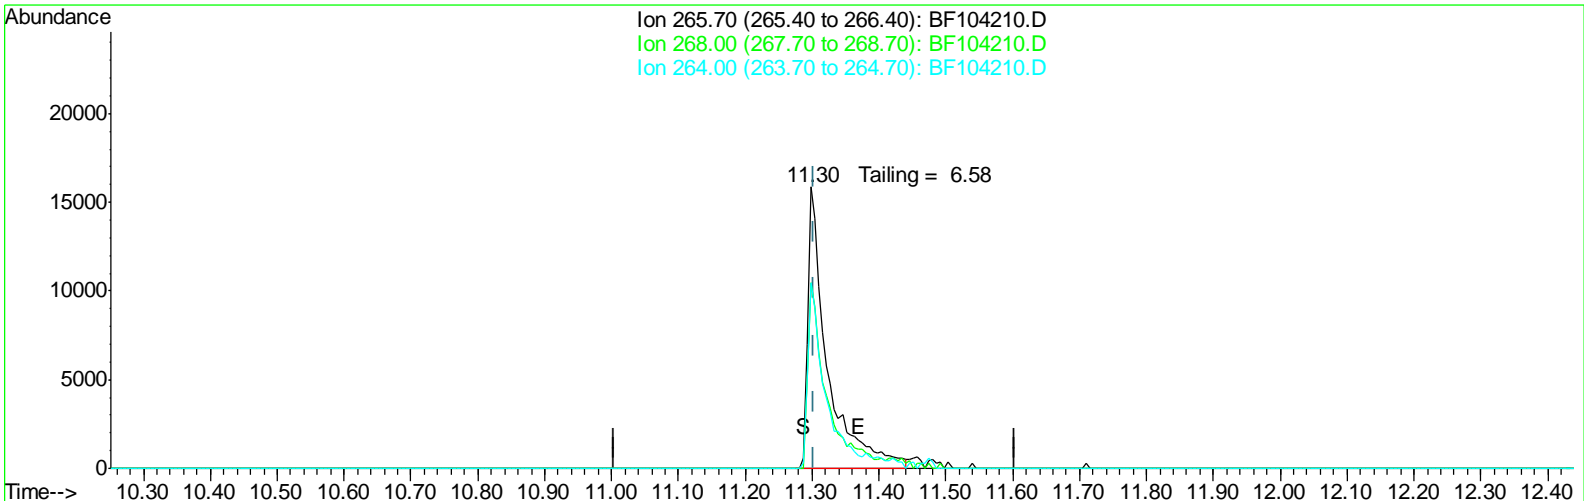




TIC: BF104210.D

(69) Pentachlorophenol (C)
 11.298min (-0.006) 39354.63ng
 response 32781

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.76
264.00	61.90	65.73
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040318\
 Data File : BF104210.D
 Acq On : 4 Apr 2018 6:34
 Operator : JU/SJ
 Sample : DF7TPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 08:53:46 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 03 15:22:43 2018
 Response via : Initial Calibration

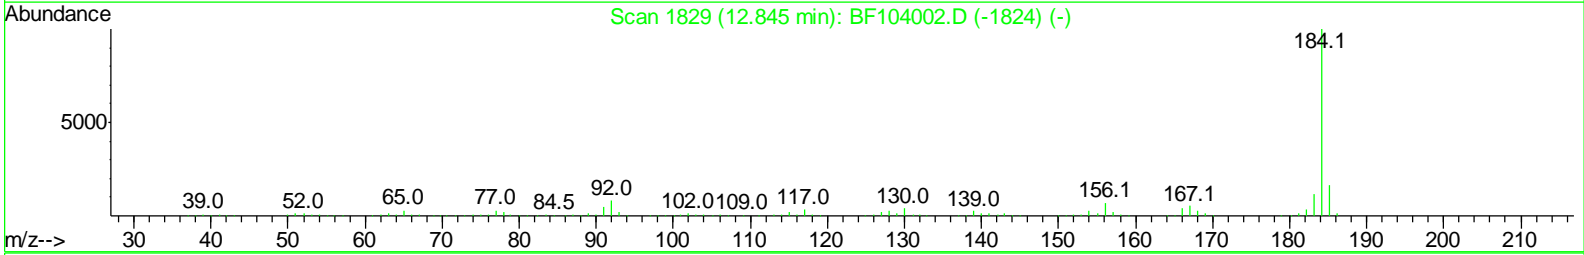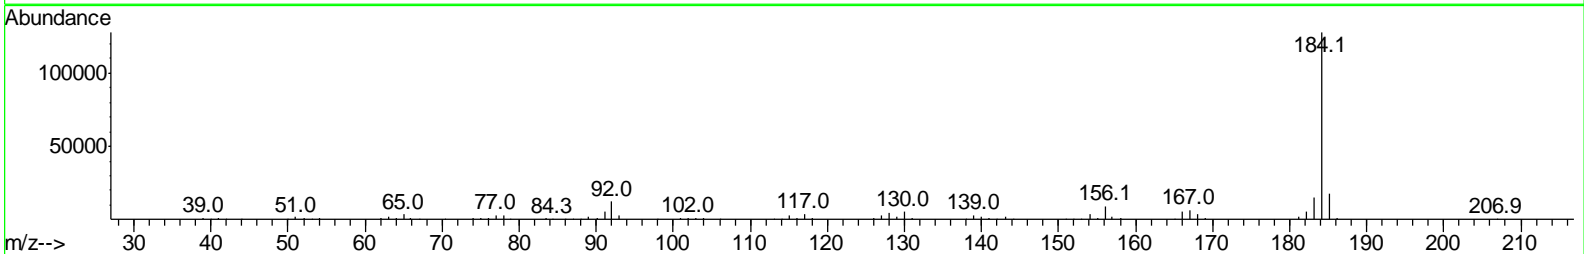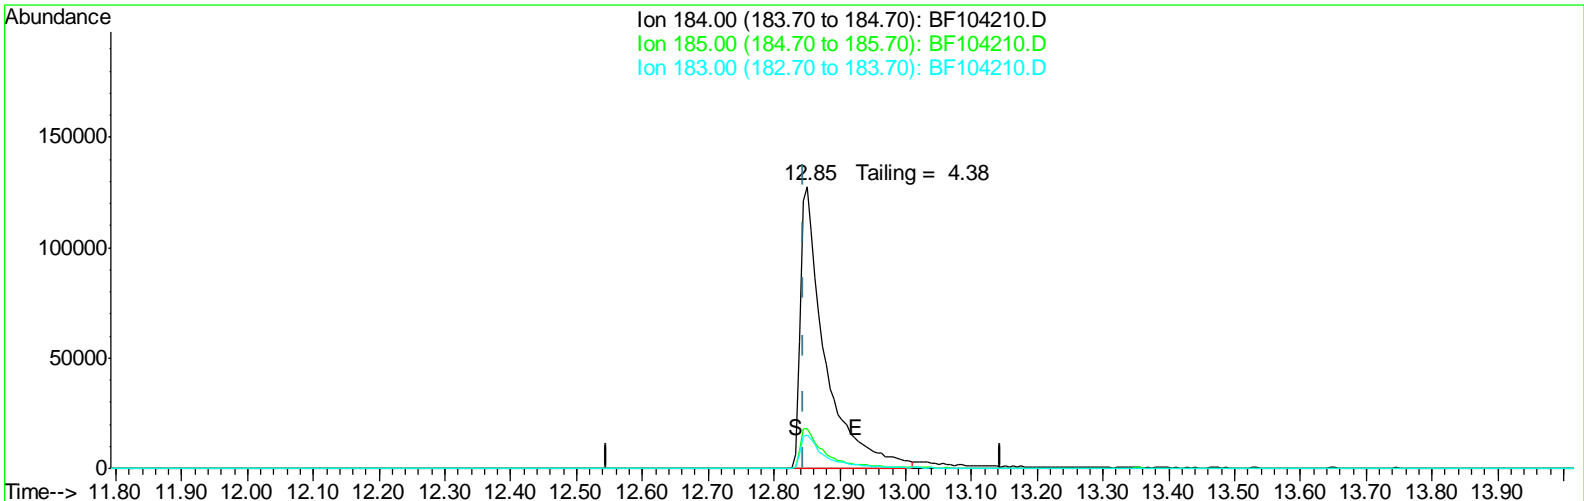

TIC: BF104210.D

(76) Benzidine

12.851min (+0.006) 0.00ng

response 332656

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.23
183.00	11.60	11.81
0.00	0.00	0.00