


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040318\
 Data File : BF104184.D
 Acq On : 3 Apr 2018 17:01
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 03 15:22:43 2018

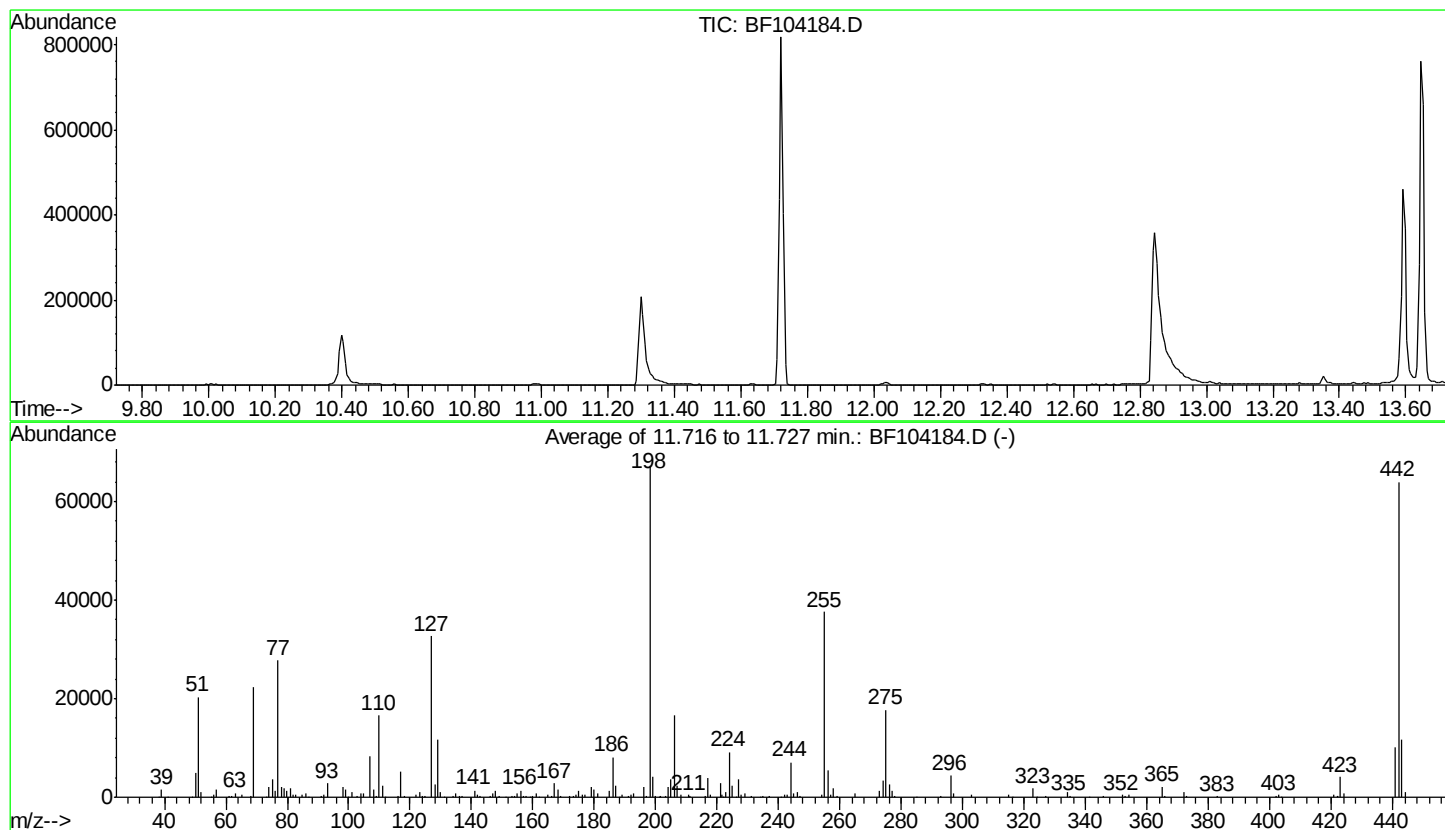

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.3	20385	PASS
68	69	0.00	2	1.7	382	PASS
69	198	0.00	100	33.3	22424	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.6	32709	PASS
197	198	0.00	2	0.2	163	PASS
198	198	100	100	100.0	67290	PASS
199	198	5	9	6.3	4215	PASS
275	198	10	60	26.5	17802	PASS
365	198	1	100	3.2	2184	PASS
441	443	0.01	100	86.6	10236	PASS
442	198	50	100	95.0	63933	PASS
443	442	15	24	18.5	11826	PASS