
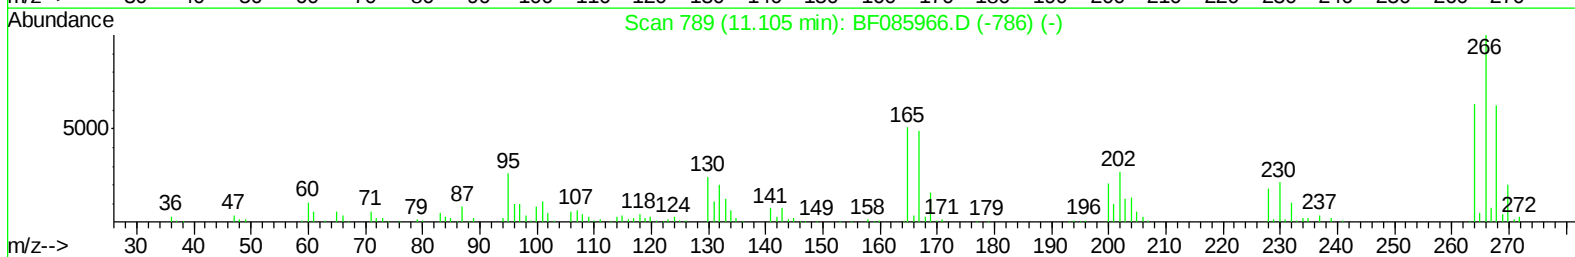
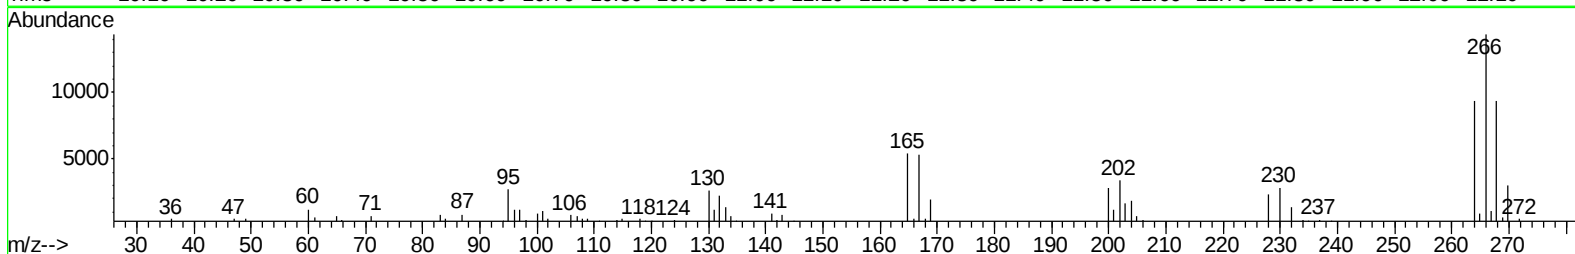


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040416\
Data File : BF086059.D
Acq On : 5 Apr 2016 2:48
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 07:25:49 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

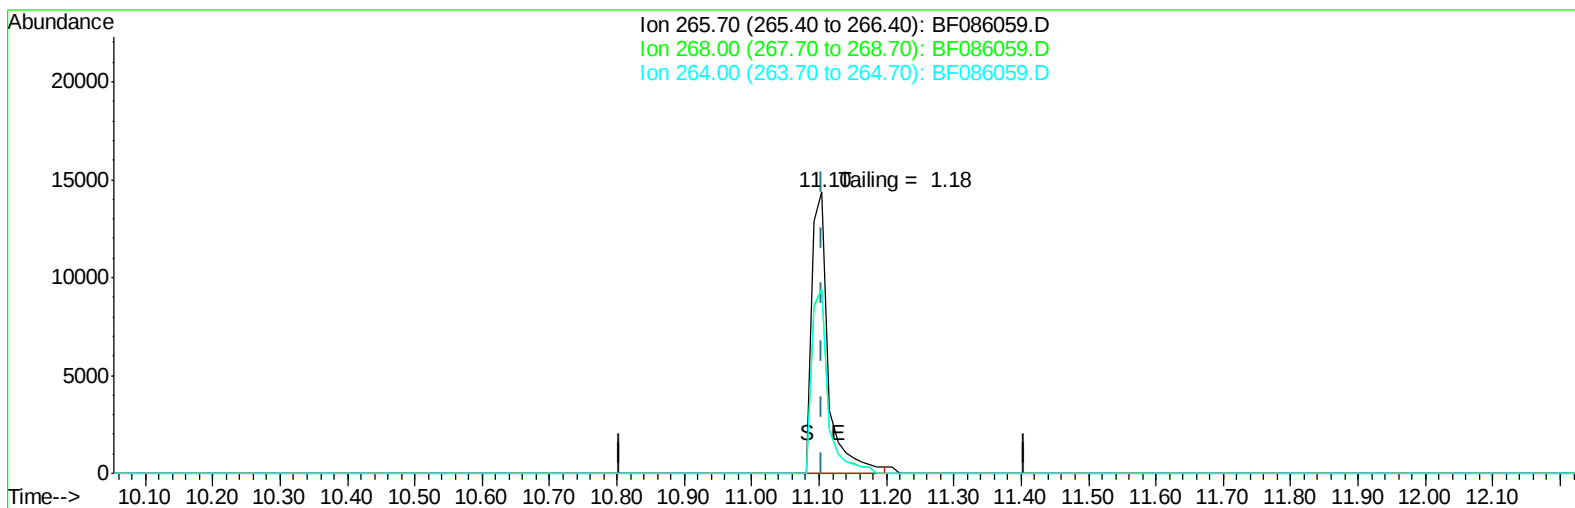

TIC: BF086059.D

(69) Pentachlorophenol (C)




11.105min (-0.000) 0.00ng

response 24645

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	65.32
264.00	63.30	65.41
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040416\
Data File : BF086059.D
Acq On : 5 Apr 2016 2:48
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 07:25:49 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

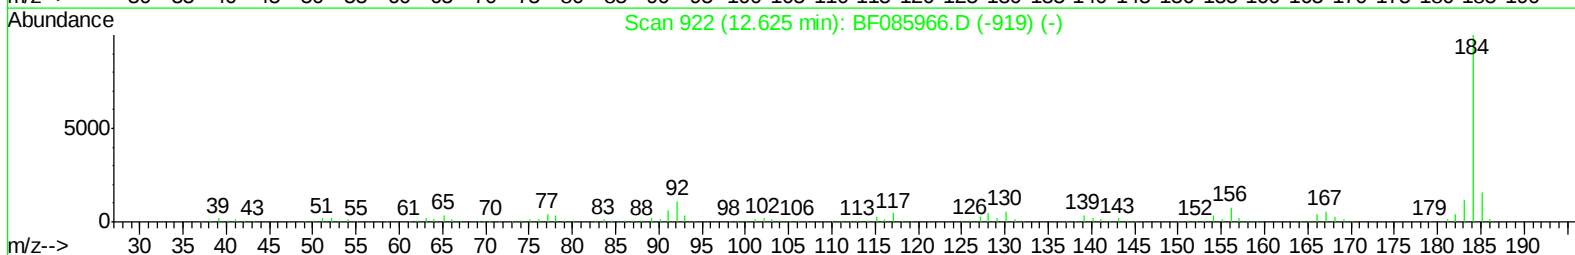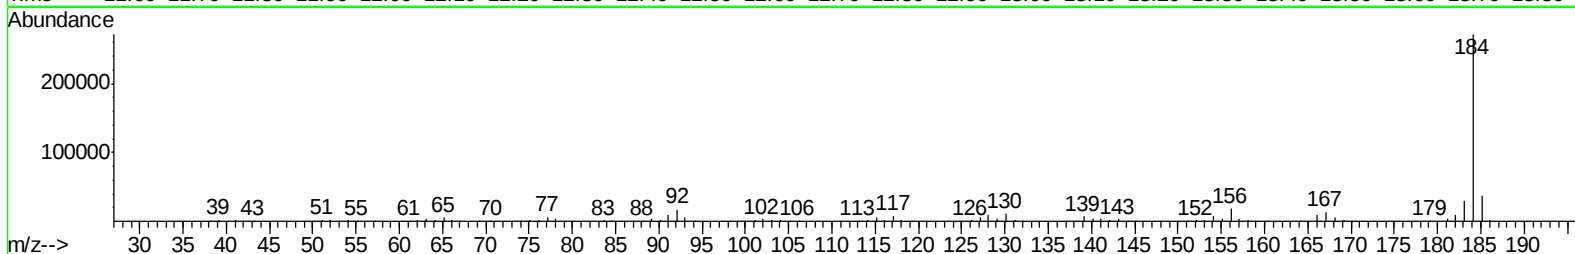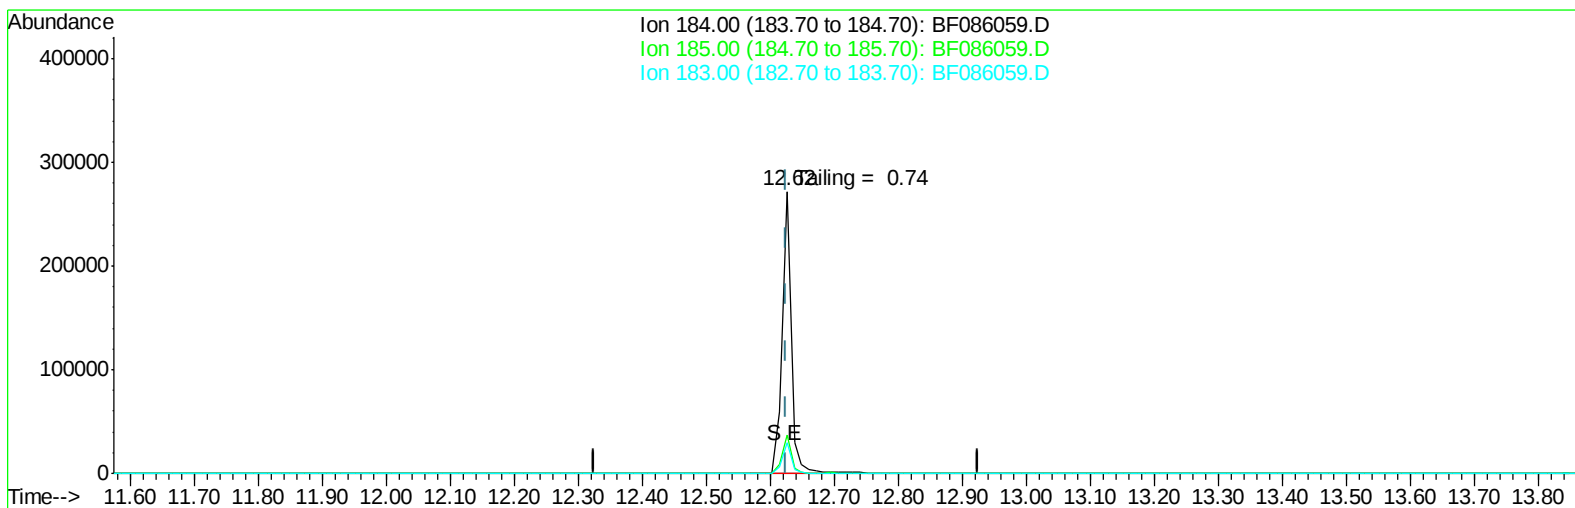

TIC: BF086059.D

(76) Benzidine

12.625min (-0.000) 0.00ng

response 265539

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	13.77
183.00	11.80	11.11
0.00	0.00	0.00