

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040416\
 Data File : BF086069.D
 Acq On : 5 Apr 2016 7:25
 Operator : UM/SJ
 Sample : H2183-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AMBOY-SB-11(0.5-20.0)

Quant Time: Apr 05 08:26:05 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 01 23:17:06 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.76	152	115152	20.00	ng	-0.01
21) Naphthalene-d8	8.04	136	392170	20.00	ng	-0.02
38) Acenaphthene-d10	9.80	164	167031	20.00	ng	-0.01
63) Phenanthrene-d10	11.28	188	257009	20.00	ng	-0.02
75) Chrysene-d12	13.92	240	211588	20.00	ng	-0.01
86) Perylene-d12	15.32	264	165963	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	935533	138.87	ng	0.00
7) Phenol-d6	6.41	99	1181458	138.07	ng	-0.01
23) Nitrobenzene-d5	7.33	82	687530	103.39	ng	-0.01
41) 2,4,6-Tribromophenol	10.59	330	193746	123.58	ng	-0.01
44) 2-Fluorobiphenyl	9.13	172	1111747	110.67	ng	-0.01
78) Terphenyl-d14	12.86	244	723187	80.34	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.52	163	117528	9.49	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040416\
Data File : BF086069.D
Acq On : 5 Apr 2016 7:25
Operator : UM/SJ
Sample : H2183-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AMBOY-SB-11(0.5-20.0)

Quant Time: Apr 05 08:26:05 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

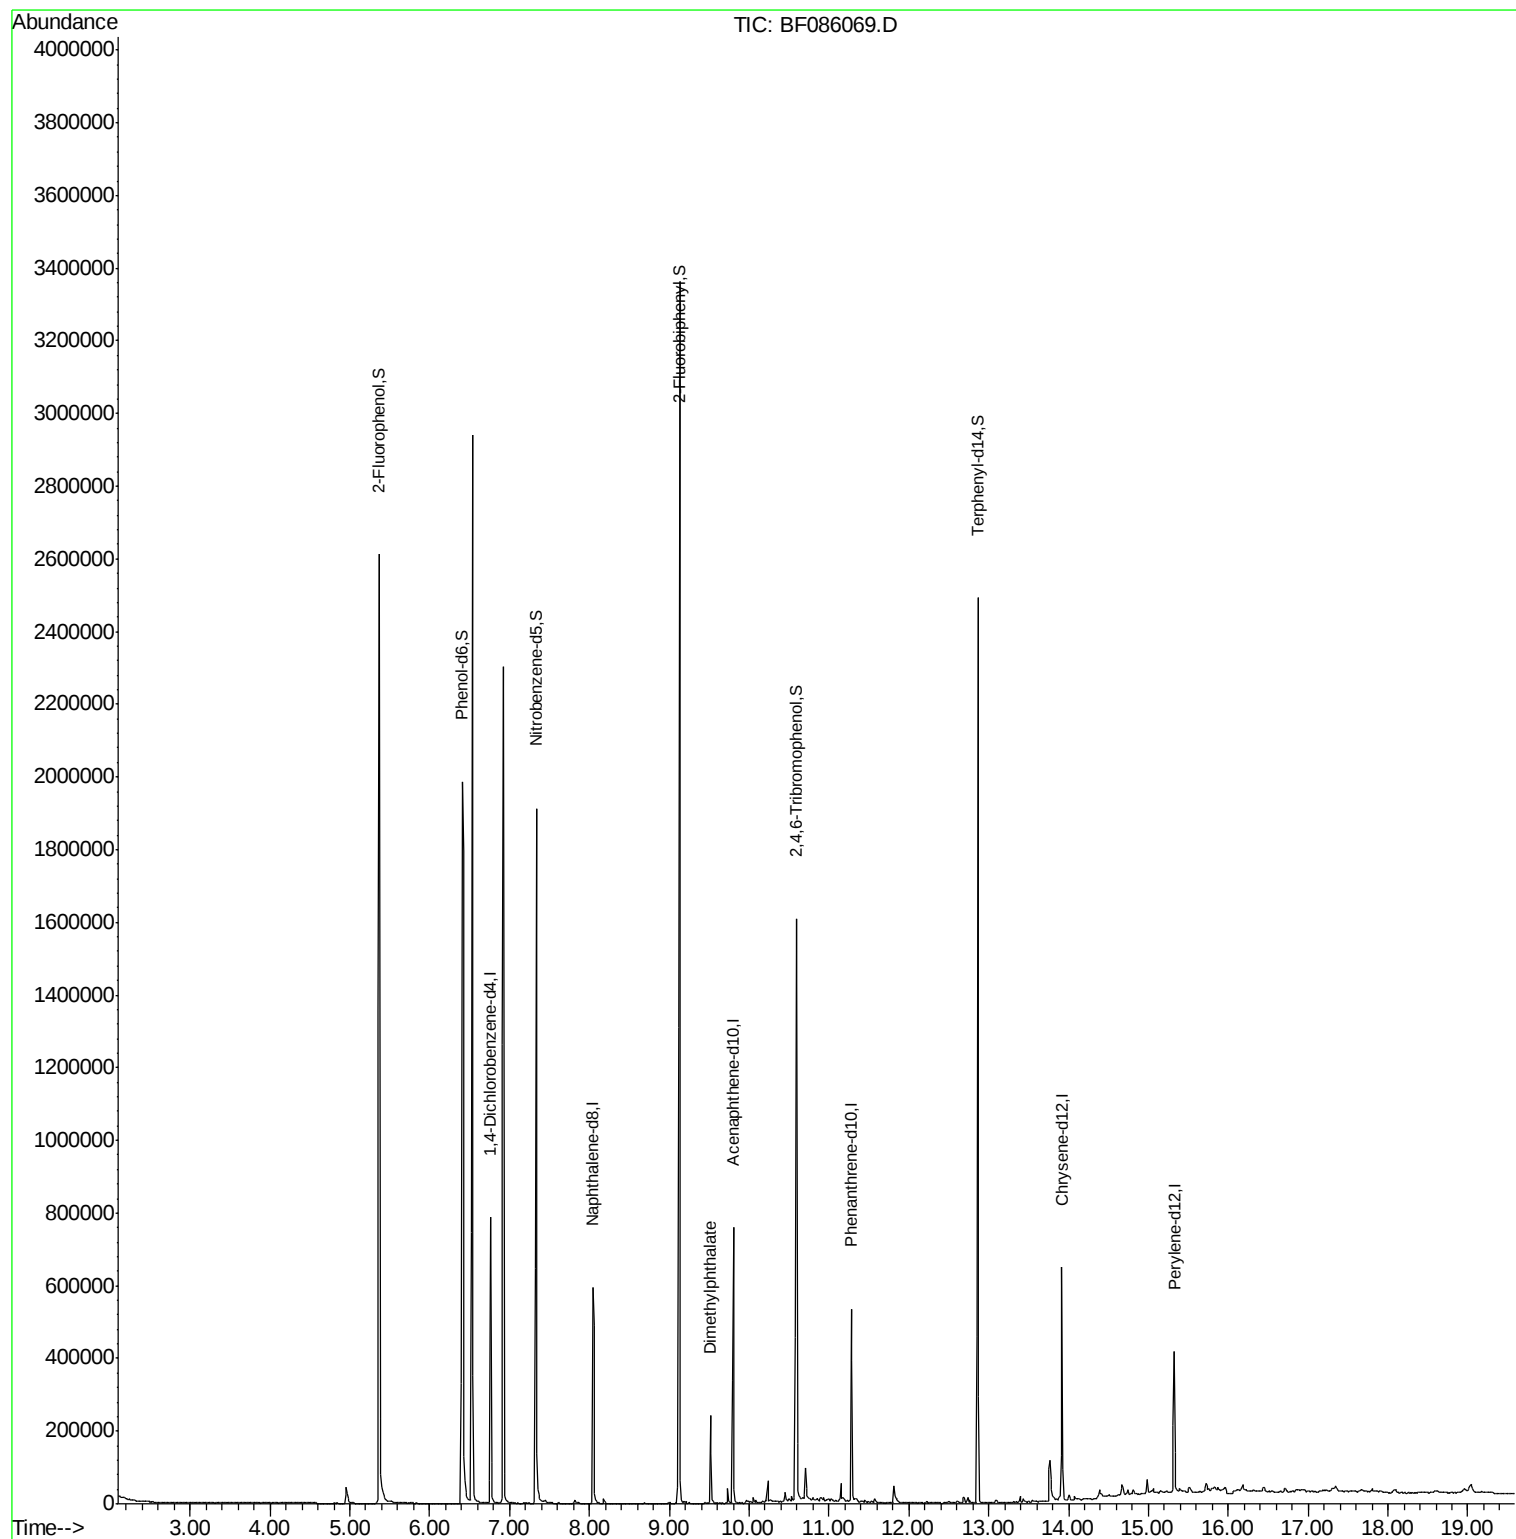



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.76 min Scan# 409

Delta R.T. -0.01 min

Lab File: BF086069.D

Acq: 5 Apr 2016 7:25

Instrument :

BNA_F

ClientSampleId :

AMBOY-SB-11(0.5-20.0)




Tot Ion:152 Resp: 115152

Ion Ratio Lower Upper

152 100

150 157.8 124.2 186.2

115 63.0 47.0 70.6

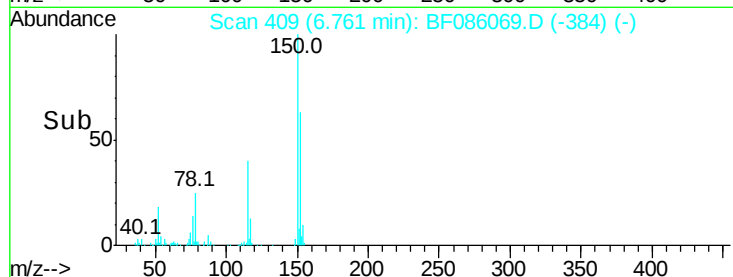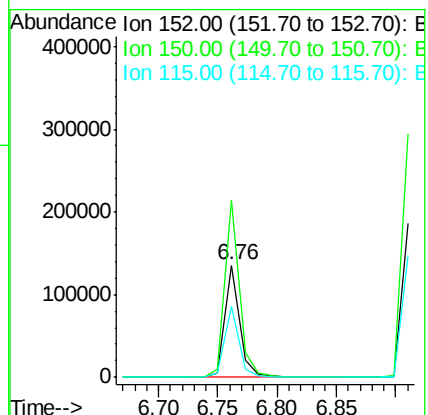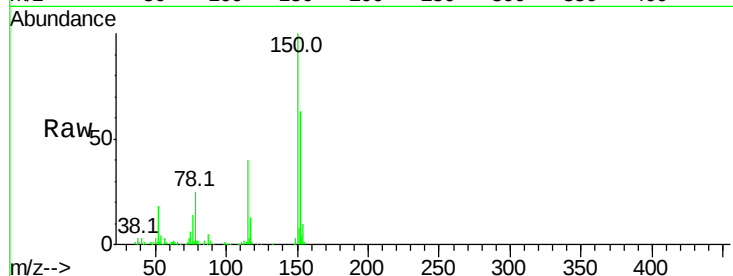

#5

2-Fluorophenol

Concen: 138.87 ng

RT: 5.37 min Scan# 287

Delta R.T. 0.00 min

Lab File: BF086069.D

Acq: 5 Apr 2016 7:25




Tgt Ion:112 Resp: 935533

Ion Ratio Lower Upper

112 100

64 51.7 39.9 59.9

63 26.6 20.2 30.2

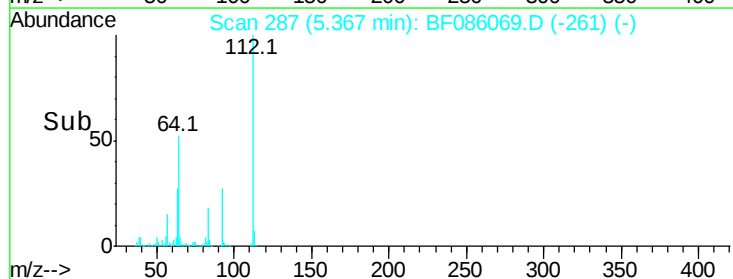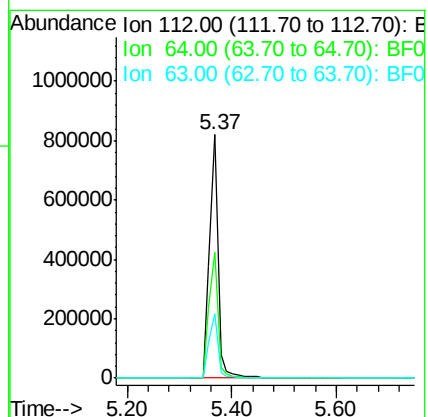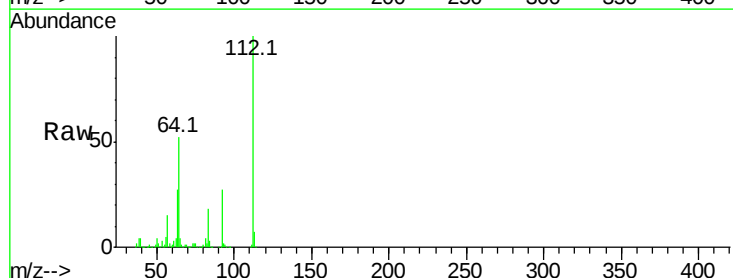



#7

Phenol-d6

Concen: 138.07 ng

RT: 6.41 min Scan# 378

Delta R.T. -0.01 min

Lab File: BF086069.D

Acq: 5 Apr 2016 7:25

Instrument :

BNA_F

ClientSampleId :

AMBOY-SB-11(0.5-20.0)





Tot Ion: 99 Resp: 1181458

Ion Ratio Lower Upper

99 100

42 15.6 11.1 16.7

71 33.1 24.9 37.3

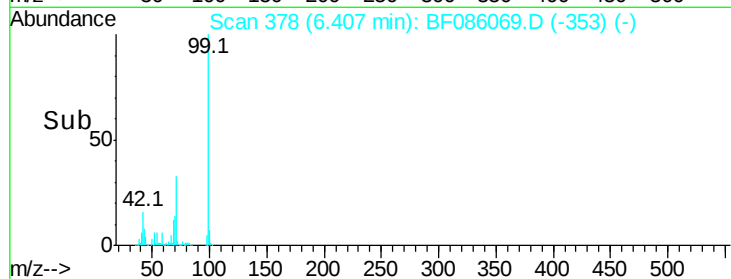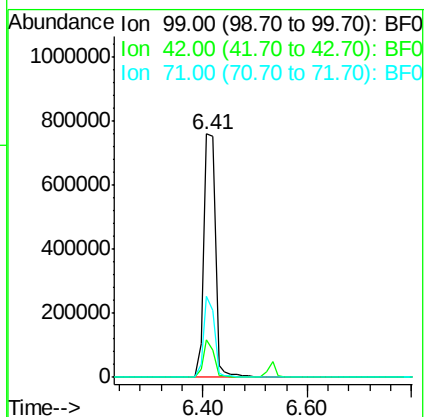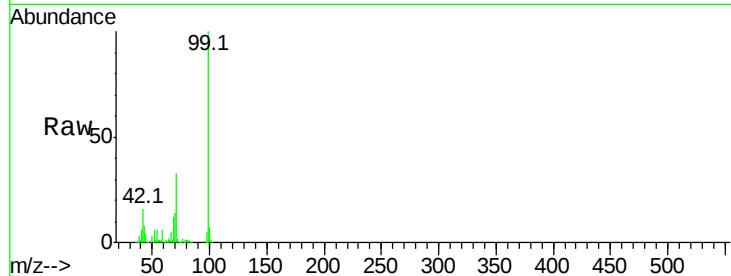

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.04 min Scan# 521

Delta R.T. -0.02 min

Lab File: BF086069.D

Acq: 5 Apr 2016 7:25

Tgt Ion: 136 Resp: 392170




Ion Ratio Lower Upper

136 100

137 11.4 9.1 13.7

54 10.0 7.4 11.0

68 7.8 5.8 8.8


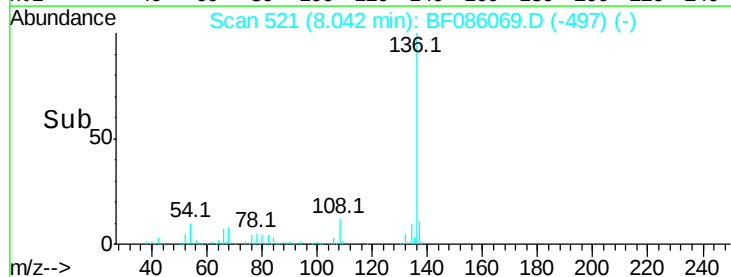
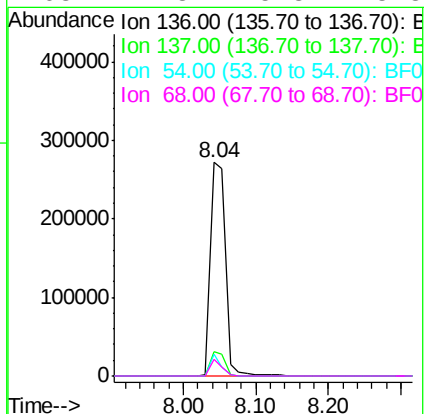





#23
 Nitrobenzene-d5
 Concen: 103.39 ng
 RT: 7.33 min Scan# 459
 Delta R.T. -0.01 min
 Lab File: BF086069.D
 Acq: 5 Apr 2016 7:25




Instrument :
 BNA_F
 ClientSampleId :
 AMBOY-SB-11(0.5-20.0)


Tot Ion: 82 Resp: 687530
 Ion Ratio Lower Upper
 82 100
 128 45.4 41.8 62.8
 54 45.2 33.4 50.0

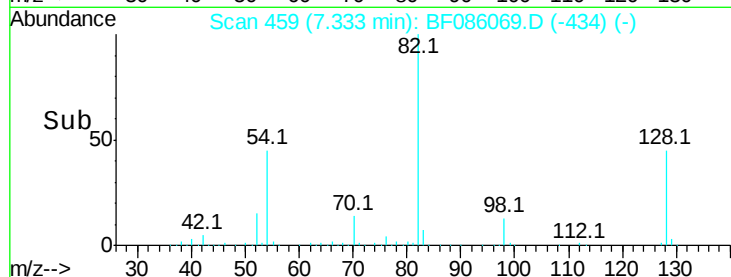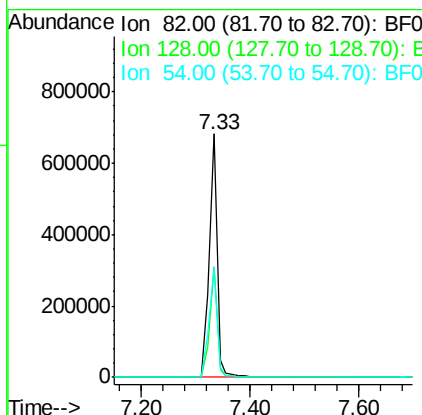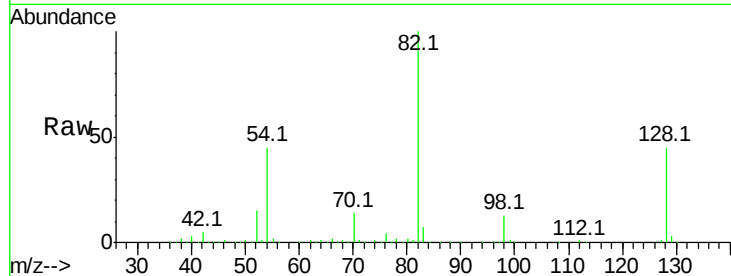

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.80 min Scan# 675
 Delta R.T. -0.01 min
 Lab File: BF086069.D
 Acq: 5 Apr 2016 7:25

Tgt Ion:164 Resp: 167031
 Ion Ratio Lower Upper
 164 100
 162 103.1 82.1 123.1
 160 47.9 37.4 56.2

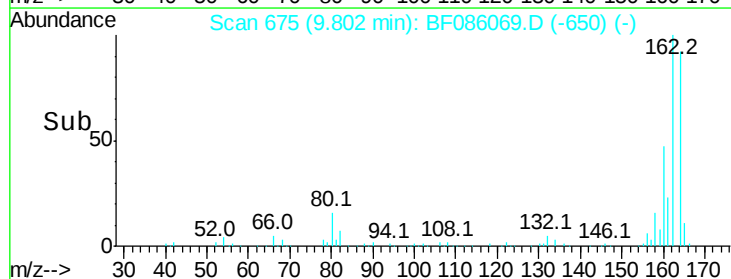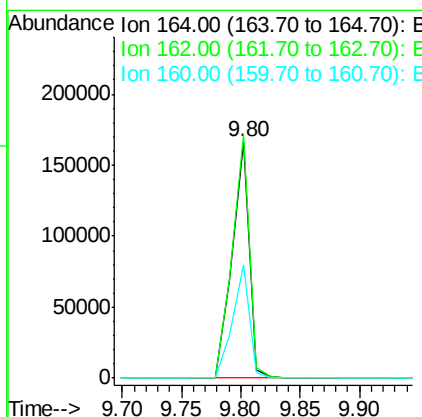


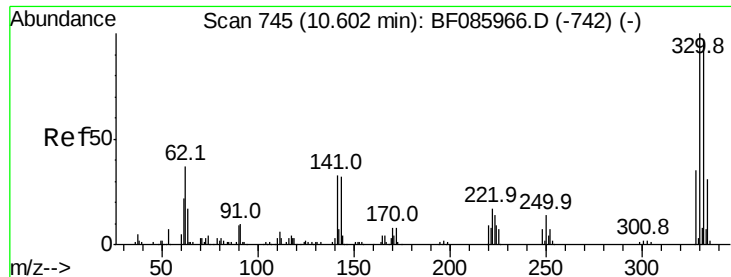



#41
 2,4,6-Tribromophenol
 Concen: 123.58 ng
 RT: 10.59 min Scan# 744
 Delta R.T. -0.01 min
 Lab File: BF086069.D
 Acq: 5 Apr 2016 7:25

Instrument :
 BNA_F
 ClientSampleId :
 AMBOY-SB-11(0.5-20.0)

Tot Ion:330 Resp: 193746
 Ion Ratio Lower Upper
 330 100
 332 94.5 78.2 117.2
 141 38.3 31.5 47.3

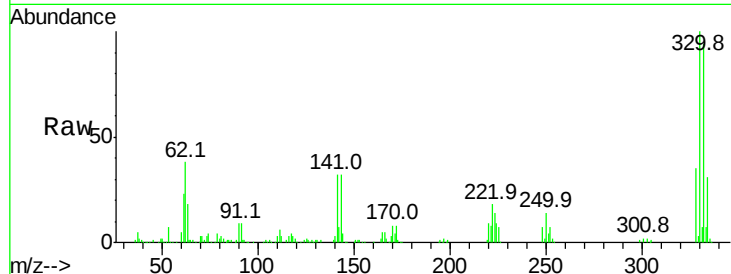


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

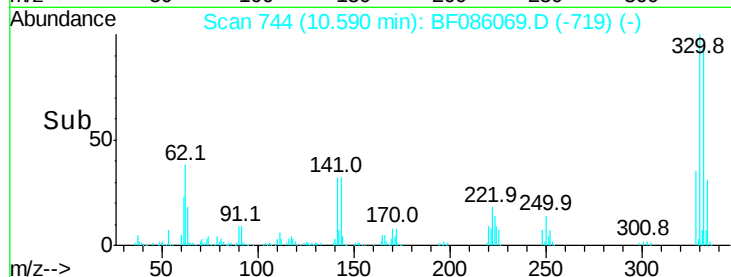
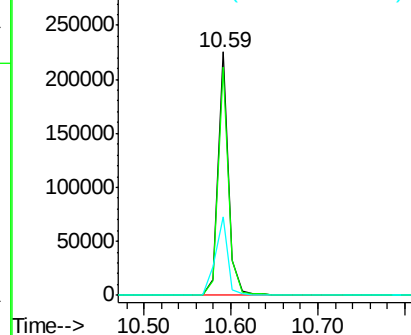



#44
 2-Fluorobiphenyl
 Concen: 110.67 ng
 RT: 9.13 min Scan# 616
 Delta R.T. -0.01 min
 Lab File: BF086069.D
 Acq: 5 Apr 2016 7:25

Tgt Ion:172 Resp: 1111747
 Ion Ratio Lower Upper
 172 100
 171 36.6 29.4 44.2
 170 24.5 19.8 29.6

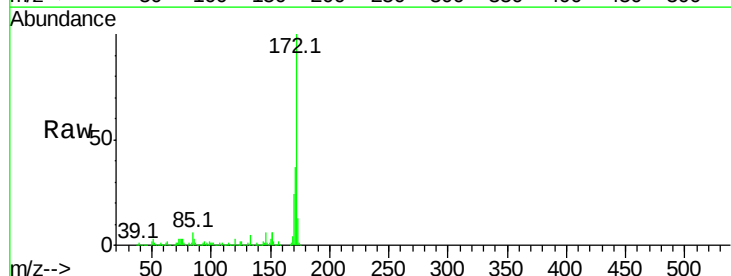

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

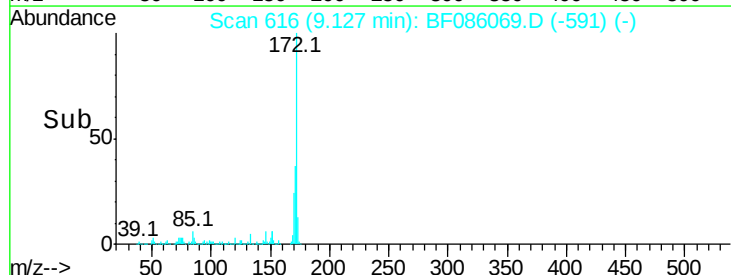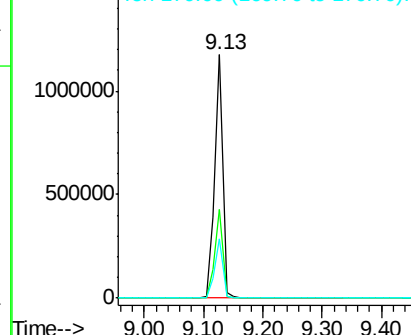

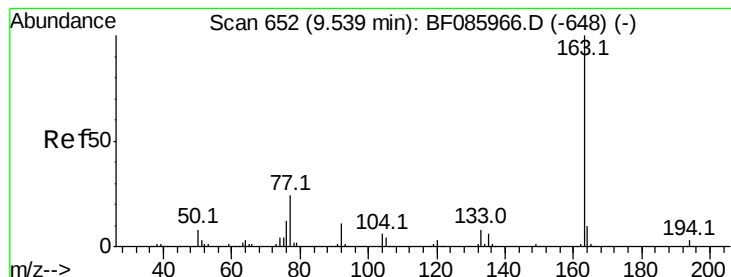

#49

Dimethylphthalate

Concen: 9.49 ng

RT: 9.52 min Scan# 650

Delta R.T. -0.02 min

Lab File: BF086069.D

Acq: 5 Apr 2016 7:25

Instrument :

BNA_F

ClientSampleId :

AMBOY-SB-11(0.5-20.0)


Tot Ion:163 Resp: 117528

Ion Ratio Lower Upper

163 100

194 3.1 2.9 4.3




164 10.9 8.3 12.5



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

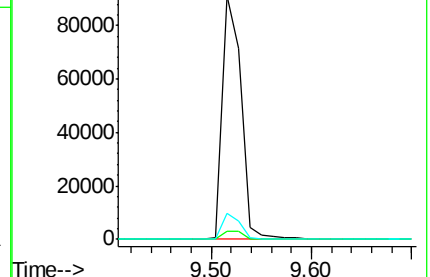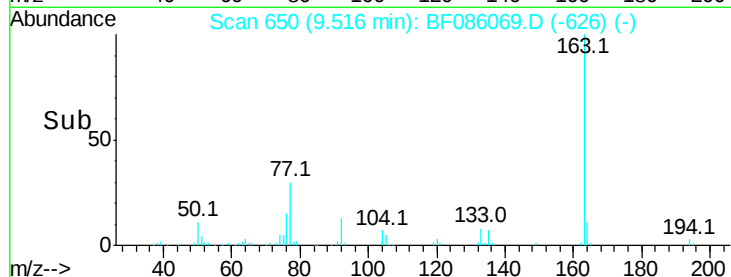

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.28 min Scan# 804

Delta R.T. -0.02 min

Lab File: BF086069.D

Acq: 5 Apr 2016 7:25


Tgt Ion:188 Resp: 257009

Ion Ratio Lower Upper

188 100

94 13.0 5.4 8.0#



80 14.9 5.5 8.3#




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

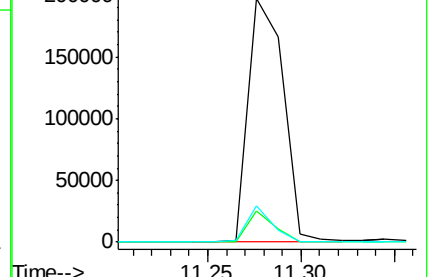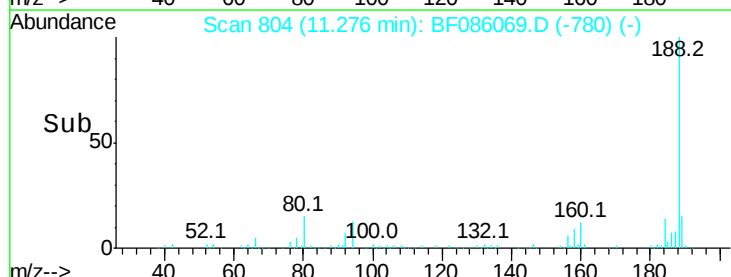

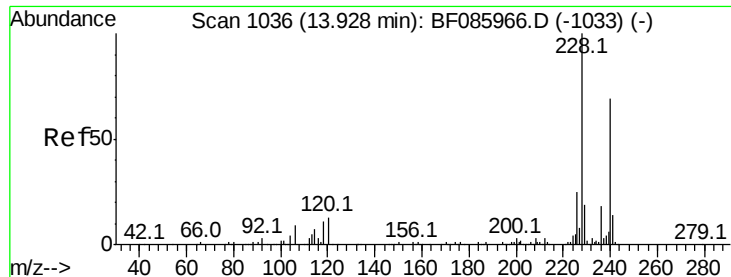

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.92 min Scan# 1035

Delta R.T. -0.01 min

Lab File: BF086069.D

Acq: 5 Apr 2016 7:25

Instrument :

BNA_F

ClientSampleId :

AMBOY-SB-11(0.5-20.0)


Tot Ion:240 Resp: 211588

Ion Ratio Lower Upper

240 100

120 11.9 13.8 20.8#




236 26.6 20.6 30.8



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

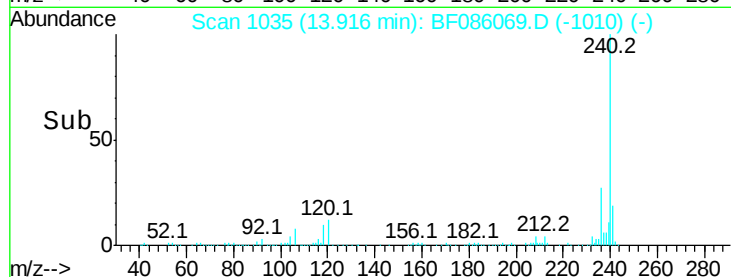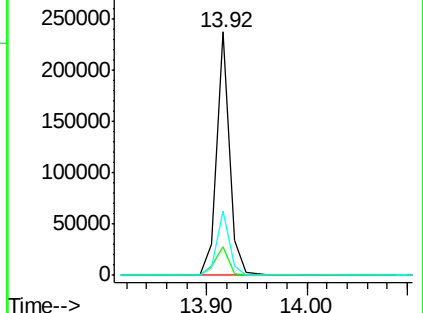

#78

Terphenyl-d14

Concen: 80.34 ng

RT: 12.86 min Scan# 943

Delta R.T. -0.01 min

Lab File: BF086069.D

Acq: 5 Apr 2016 7:25


Tgt Ion:244 Resp: 723187

Ion Ratio Lower Upper

244 100

212 7.6 6.1 9.1



122 13.2 10.2 15.4




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

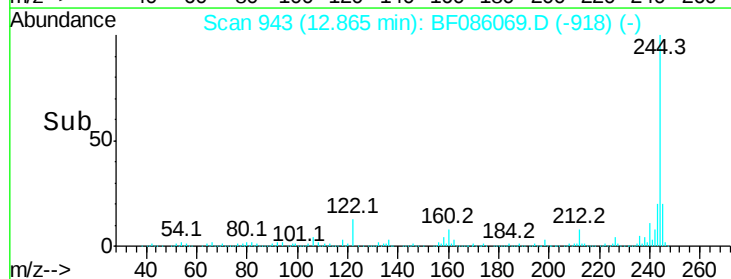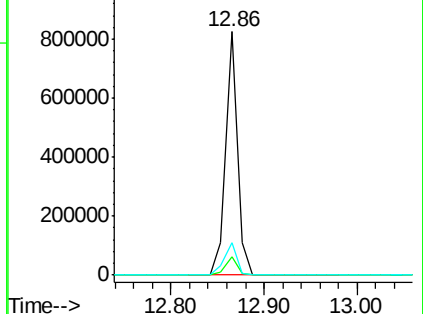


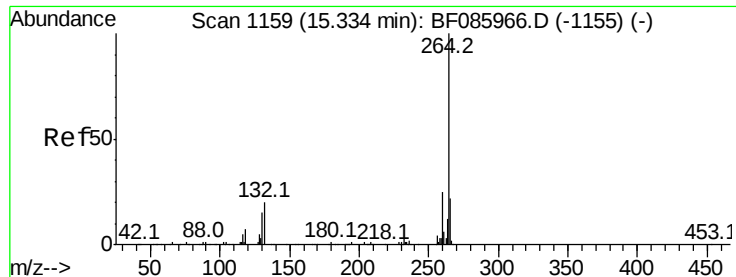

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.32 min Scan# 1158
 Delta R.T. -0.01 min
 Lab File: BF086069.D
 Acq: 5 Apr 2016 7:25

Instrument :
 BNA_F
 ClientSampleId :
 AMBOY-SB-11(0.5-20.0)

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.7	19.4	29.2
265	21.1	17.2	25.8

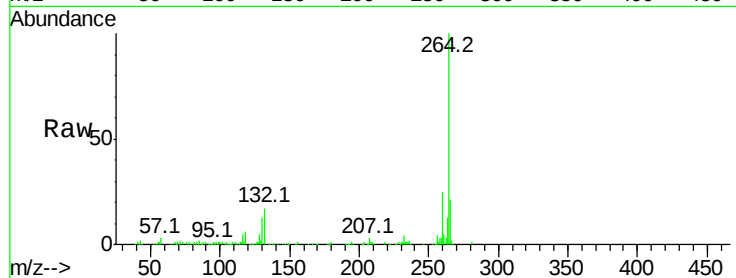

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

