

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040416\
 Data File : BF086078.D
 Acq On : 5 Apr 2016 11:34
 Operator : UM/SJ
 Sample : H2027-09
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GRID-18COMP

Quant Time: Apr 05 12:55:00 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 01 23:17:06 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.76	152	119506	20.00	ng	-0.01
21) Naphthalene-d8	8.04	136	426338	20.00	ng	-0.02
38) Acenaphthene-d10	9.80	164	184449	20.00	ng	-0.01
63) Phenanthrene-d10	11.28	188	291916	20.00	ng	-0.02
75) Chrysene-d12	13.92	240	224779	20.00	ng	-0.01
86) Perylene-d12	15.32	264	174381	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.38	112	932426	133.37	ng	0.01
7) Phenol-d6	6.42	99	1094447	123.24	ng	0.00
23) Nitrobenzene-d5	7.33	82	694432	96.06	ng	-0.01
41) 2,4,6-Tribromophenol	10.59	330	232814	134.48	ng	-0.01
44) 2-Fluorobiphenyl	9.13	172	1234481	111.28	ng	-0.01
78) Terphenyl-d14	12.87	244	843573	88.22	ng	-0.01


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040416\
Data File : BF086078.D
Acq On : 5 Apr 2016 11:34
Operator : UM/SJ
Sample : H2027-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GRID-18COMP

Quant Time: Apr 05 12:55:00 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

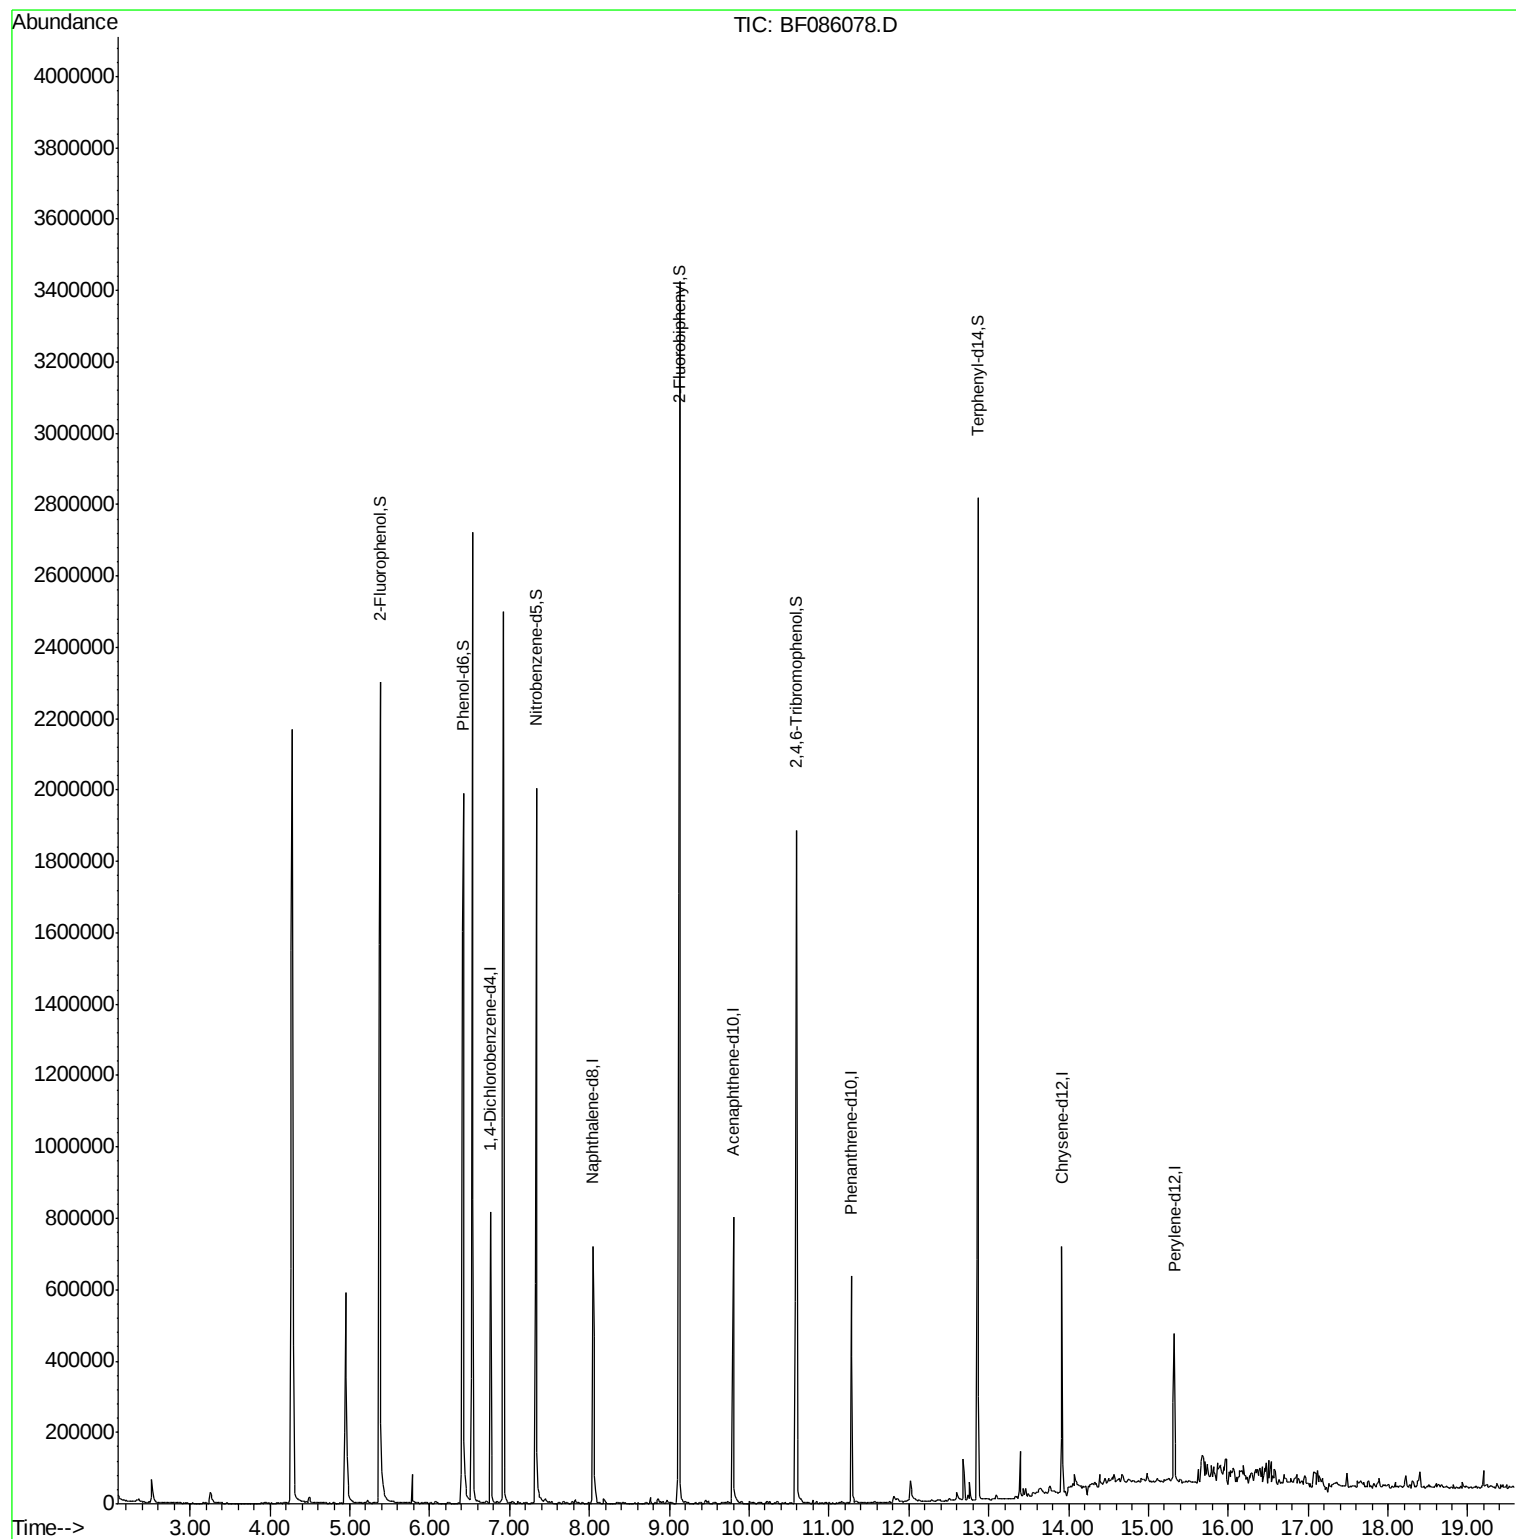







#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.76 min Scan# 409
Delta R.T. -0.01 min
Lab File: BF086078.D
Acq: 5 Apr 2016 11:34

Instrument :
BNA_F
ClientSampleId :
GRID-18COMP




Tot Ion:152 Resp: 119506
Ion Ratio Lower Upper
152 100
150 156.7 124.2 186.2
115 63.8 47.0 70.6

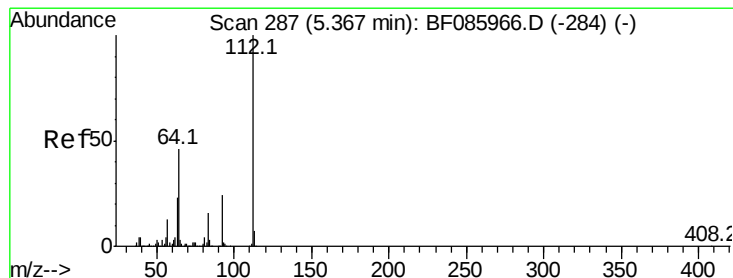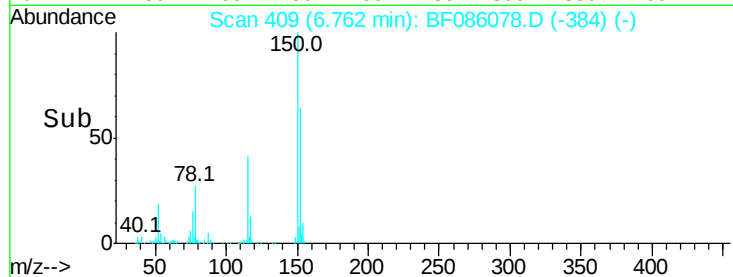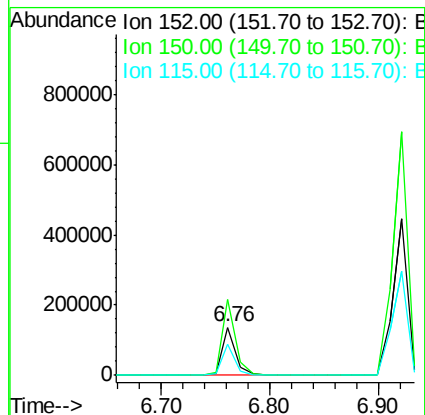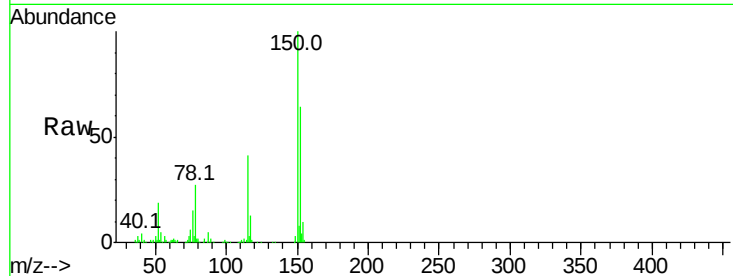


#5

2-Fluorophenol
Concen: 133.37 ng
RT: 5.38 min Scan# 288
Delta R.T. 0.01 min
Lab File: BF086078.D
Acq: 5 Apr 2016 11:34

Tgt Ion:112 Resp: 932426
Ion Ratio Lower Upper
112 100
64 48.5 39.9 59.9
63 24.7 20.2 30.2

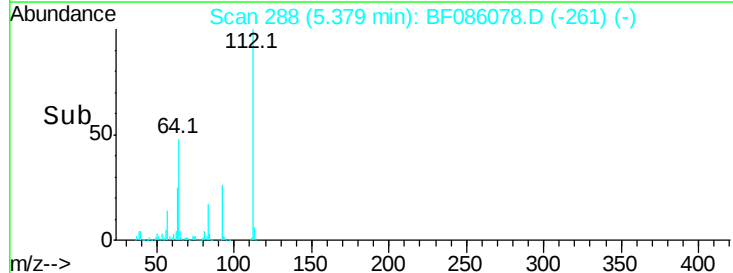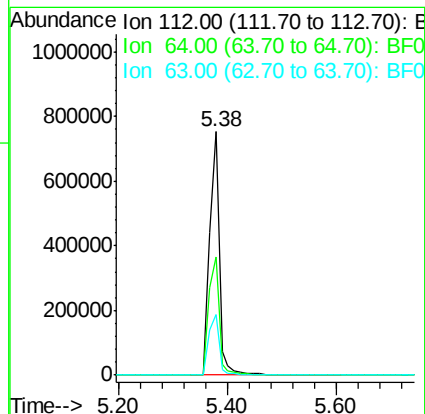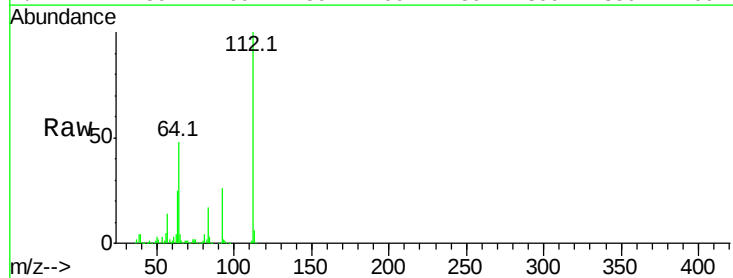

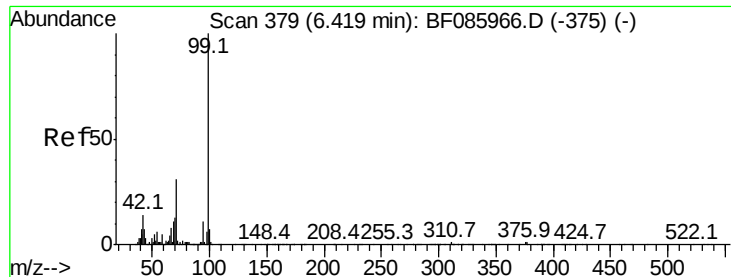

#7

Phenol-d6

Concen: 123.24 ng

RT: 6.42 min Scan# 379

Delta R.T. 0.00 min

Lab File: BF086078.D

Acq: 5 Apr 2016 11:34

Instrument :


BNA_F

ClientSampleId :

GRID-18COMP

Tot Ion: 99 Resp: 1094447




Ion	Ratio	Lower	Upper
99	100		
42	12.3	11.1	16.7
71	29.3	24.9	37.3

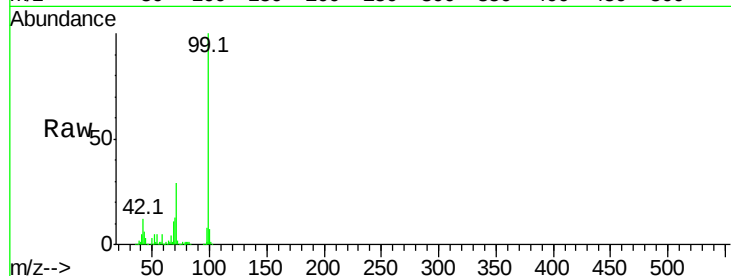

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

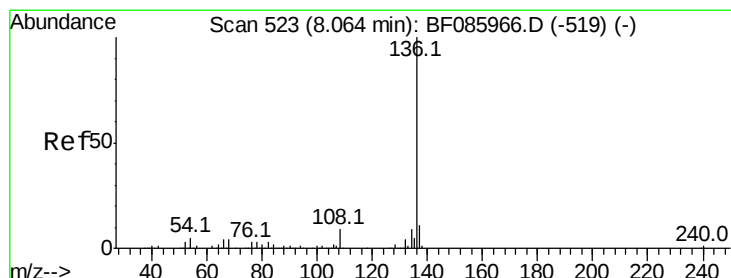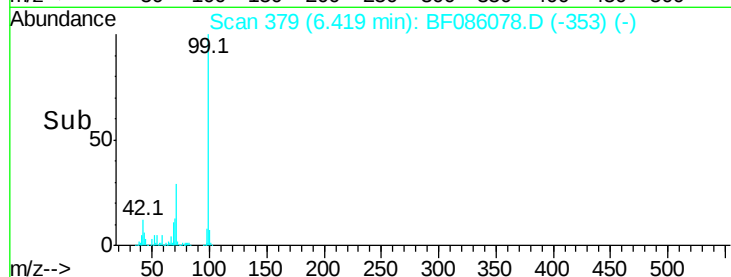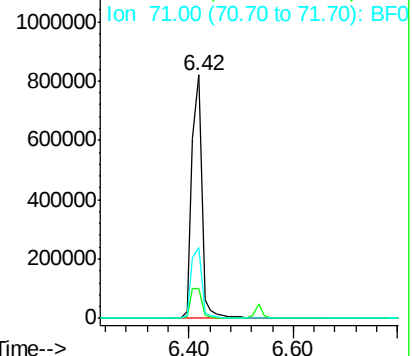

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.04 min Scan# 521


Delta R.T. -0.02 min

Lab File: BF086078.D

Acq: 5 Apr 2016 11:34

Tgt Ion: 136 Resp: 426338

Ion	Ratio	Lower	Upper
136	100		
137	11.4	9.1	13.7
54	9.3	7.4	11.0
68	7.4	5.8	8.8


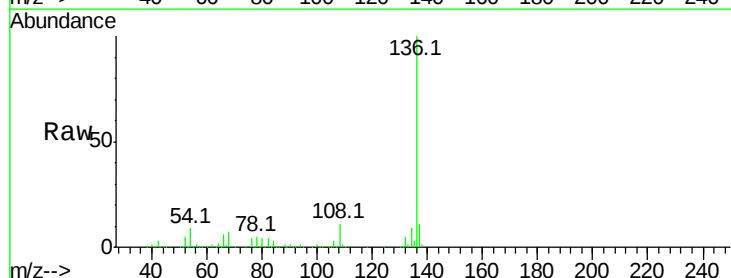



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



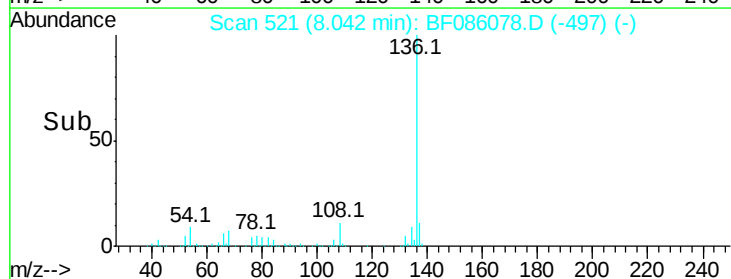
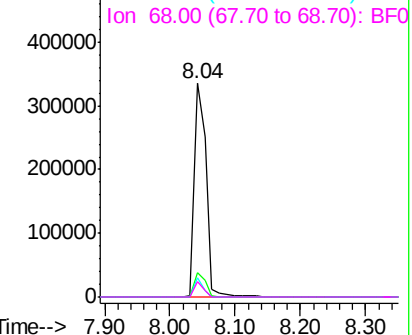


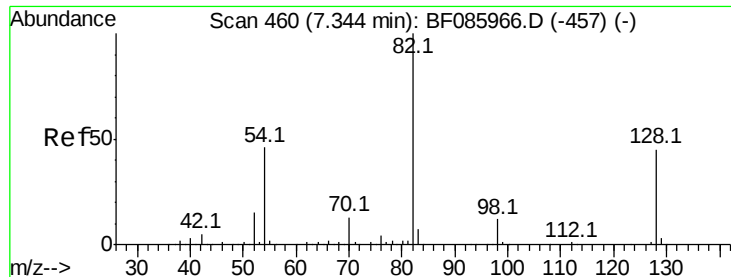

#23
 Nitrobenzene-d5
 Concen: 96.06 ng
 RT: 7.33 min Scan# 459
 Delta R.T. -0.01 min
 Lab File: BF086078.D
 Acq: 5 Apr 2016 11:34




Instrument :
 BNA_F
 ClientSampleId :
 GRID-18COMP


Tot Ion: 82 Resp: 694432
 Ion Ratio Lower Upper
 82 100
 128 45.5 41.8 62.8
 54 45.6 33.4 50.0

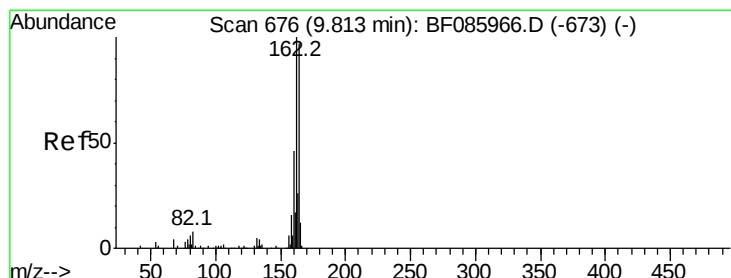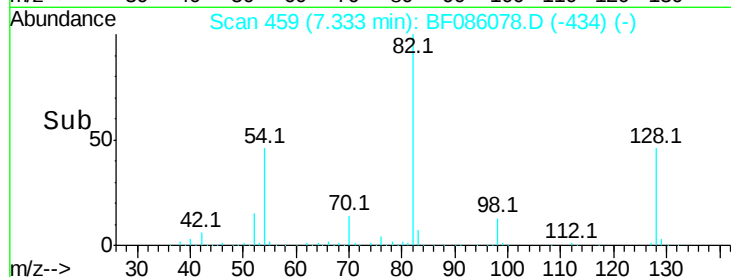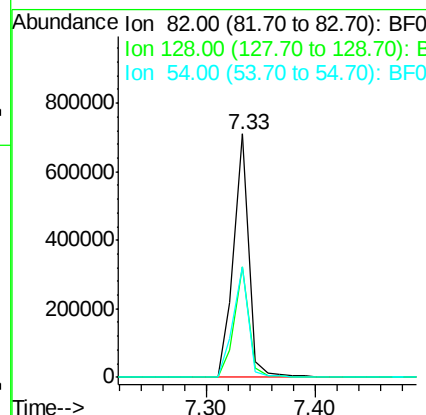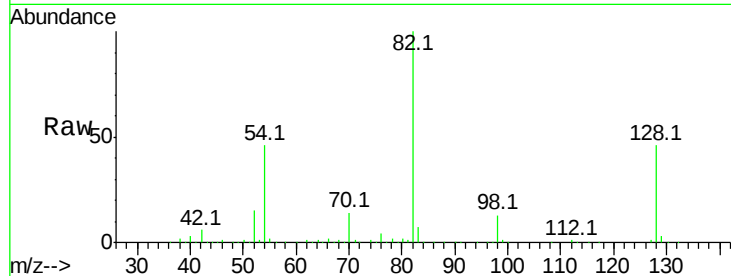

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.80 min Scan# 675
 Delta R.T. -0.01 min
 Lab File: BF086078.D
 Acq: 5 Apr 2016 11:34

Tgt Ion: 164 Resp: 184449
 Ion Ratio Lower Upper
 164 100
 162 102.3 82.1 123.1
 160 47.0 37.4 56.2

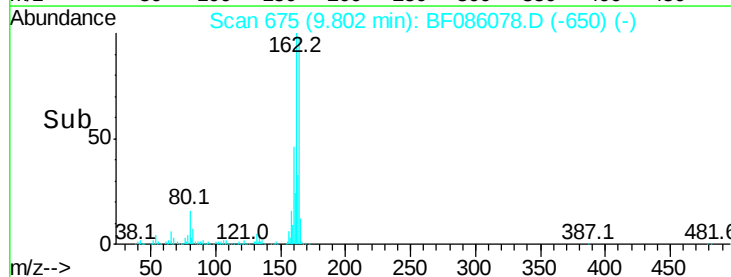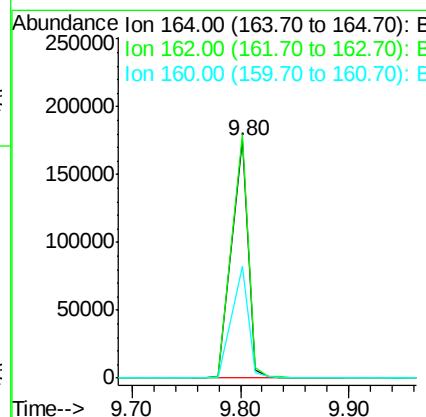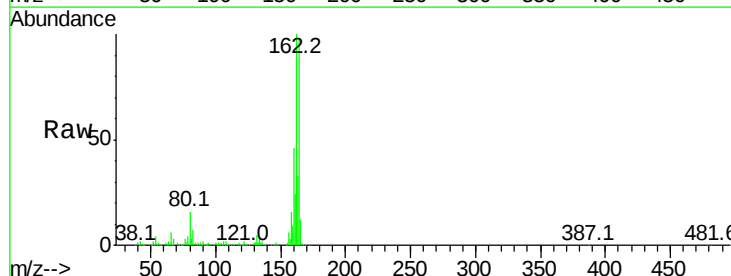


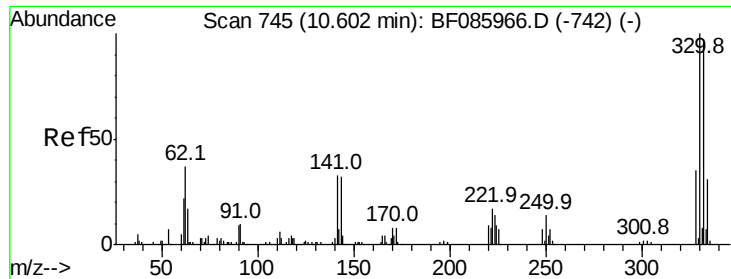



#41
 2,4,6-Tribromophenol
 Concen: 134.48 ng
 RT: 10.59 min Scan# 744
 Delta R.T. -0.01 min
 Lab File: BF086078.D
 Acq: 5 Apr 2016 11:34

Instrument :
 BNA_F
 ClientSampleId :
 GRID-18COMP

Tot Ion:330 Resp: 232814
 Ion Ratio Lower Upper
 330 100
 332 95.6 78.2 117.2
 141 37.1 31.5 47.3

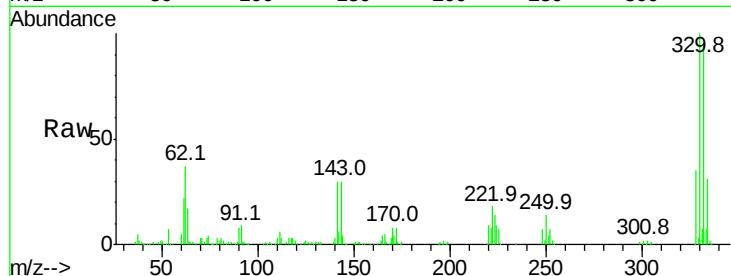


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

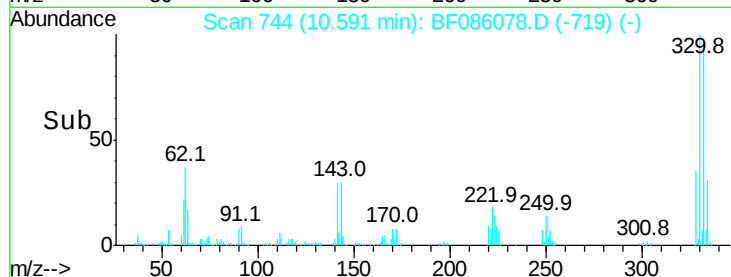
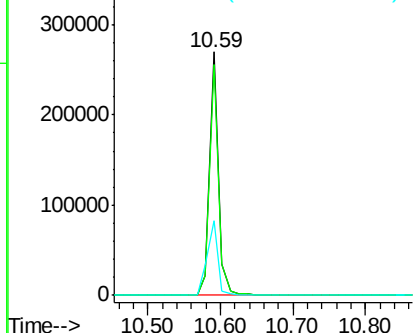



#44
 2-Fluorobiphenyl
 Concen: 111.28 ng
 RT: 9.13 min Scan# 616
 Delta R.T. -0.01 min
 Lab File: BF086078.D
 Acq: 5 Apr 2016 11:34

Tgt Ion:172 Resp: 1234481
 Ion Ratio Lower Upper
 172 100
 171 36.9 29.4 44.2
 170 24.7 19.8 29.6

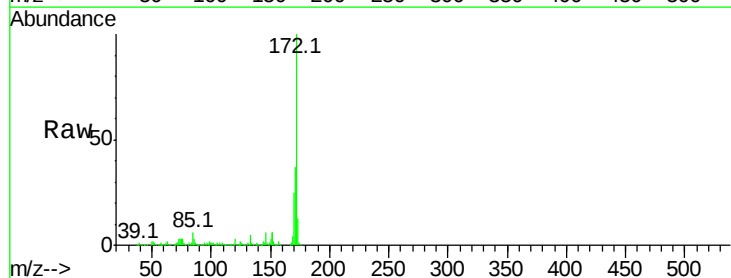

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



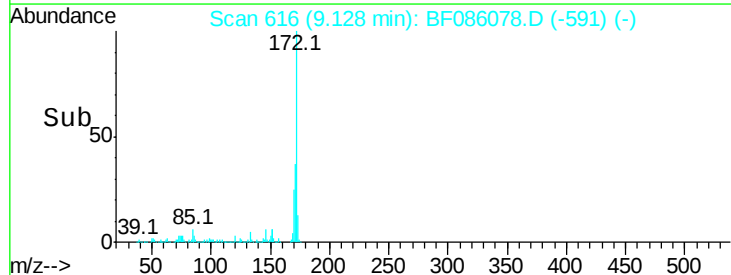
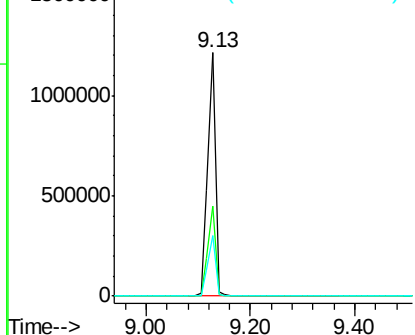


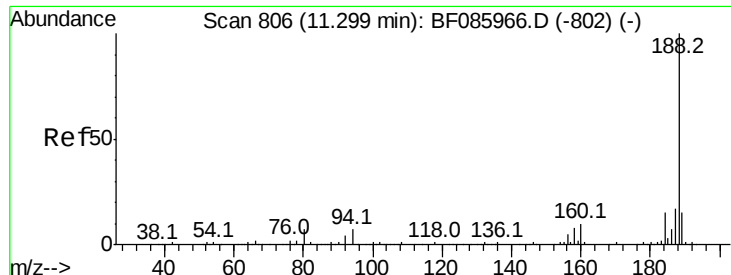

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.28 min Scan# 804
Delta R.T. -0.02 min
Lab File: BF086078.D
Acq: 5 Apr 2016 11:34




Instrument :
BNA_F
ClientSampleId :
GRID-18COMP


Tot Ion:188 Resp: 291916
Ion Ratio Lower Upper
188 100
94 13.6 5.4 8.0#
80 14.4 5.5 8.3#

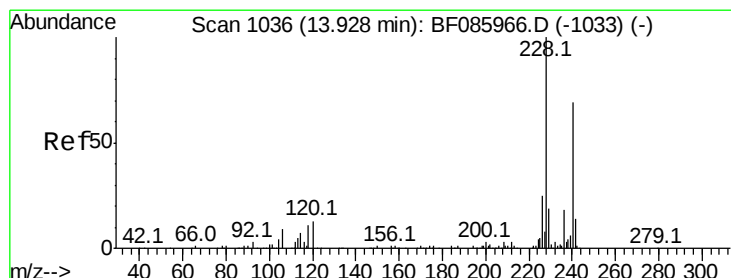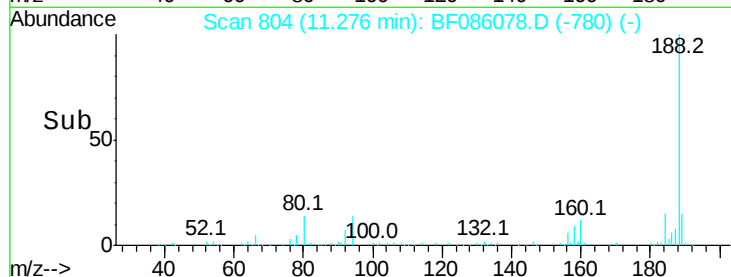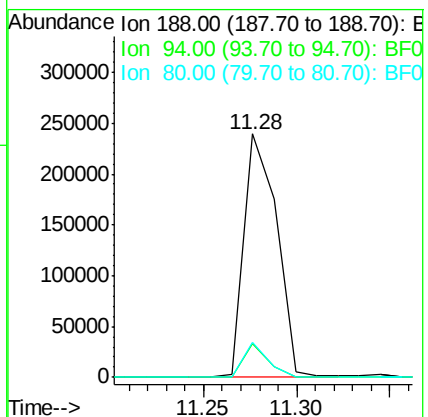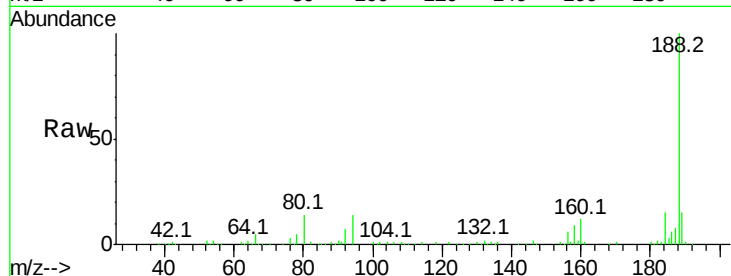

#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.92 min Scan# 1035
Delta R.T. -0.01 min
Lab File: BF086078.D
Acq: 5 Apr 2016 11:34

Tgt Ion:240 Resp: 224779
Ion Ratio Lower Upper
240 100
120 11.8 13.8 20.8#
236 26.8 20.6 30.8

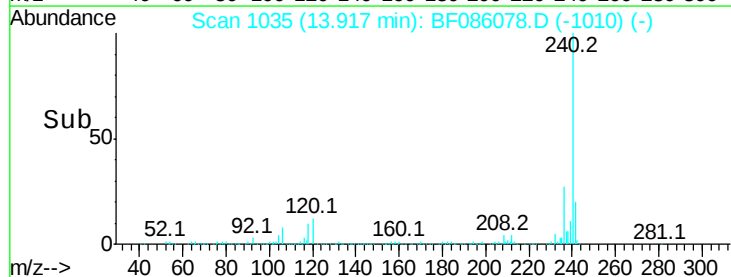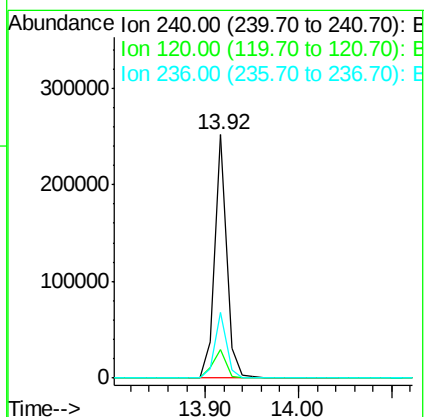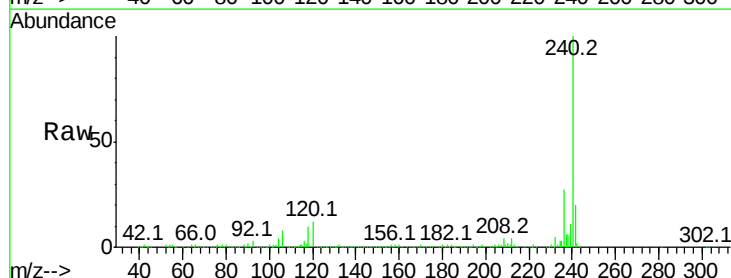

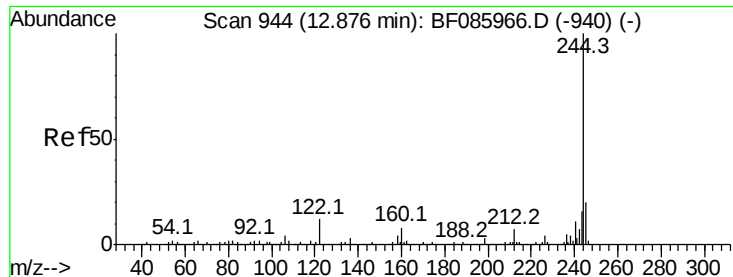

#78

Terphenyl-d14

Concen: 88.22 ng

RT: 12.87 min Scan# 943

Delta R.T. -0.01 min

Lab File: BF086078.D

Acq: 5 Apr 2016 11:34

Instrument :

BNA_F

ClientSampleId :

GRID-18COMP


Tot Ion:244 Resp: 843573

Ion Ratio Lower Upper

244 100

212 7.3 6.1 9.1




122 12.3 10.2 15.4

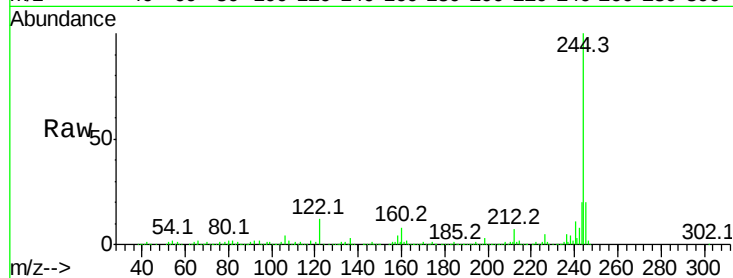

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

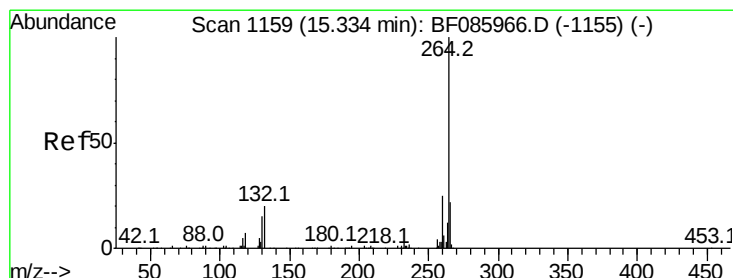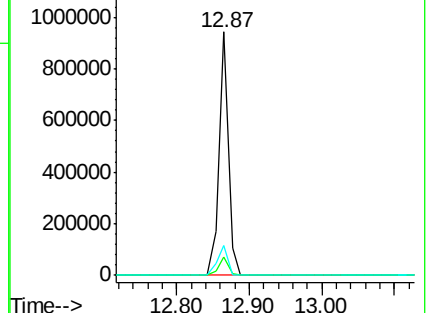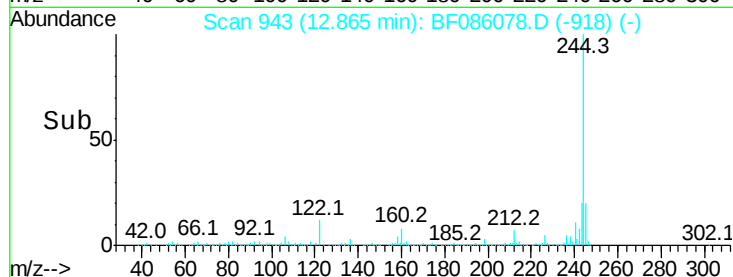

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.32 min Scan# 1158

Delta R.T. -0.01 min

Lab File: BF086078.D

Acq: 5 Apr 2016 11:34


Tgt Ion:264 Resp: 174381

Ion Ratio Lower Upper

264 100

260 24.5 19.4 29.2

265 21.8 17.2 25.8

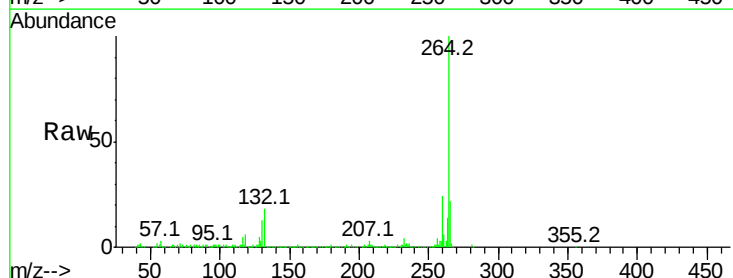

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

