


Data Path : Z:\HPCHEM1\BNA F\Data\BF040416\
 Data File : BF086035.D
 Acq On : 4 Apr 2016 13:10
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 01 23:17:06 2016

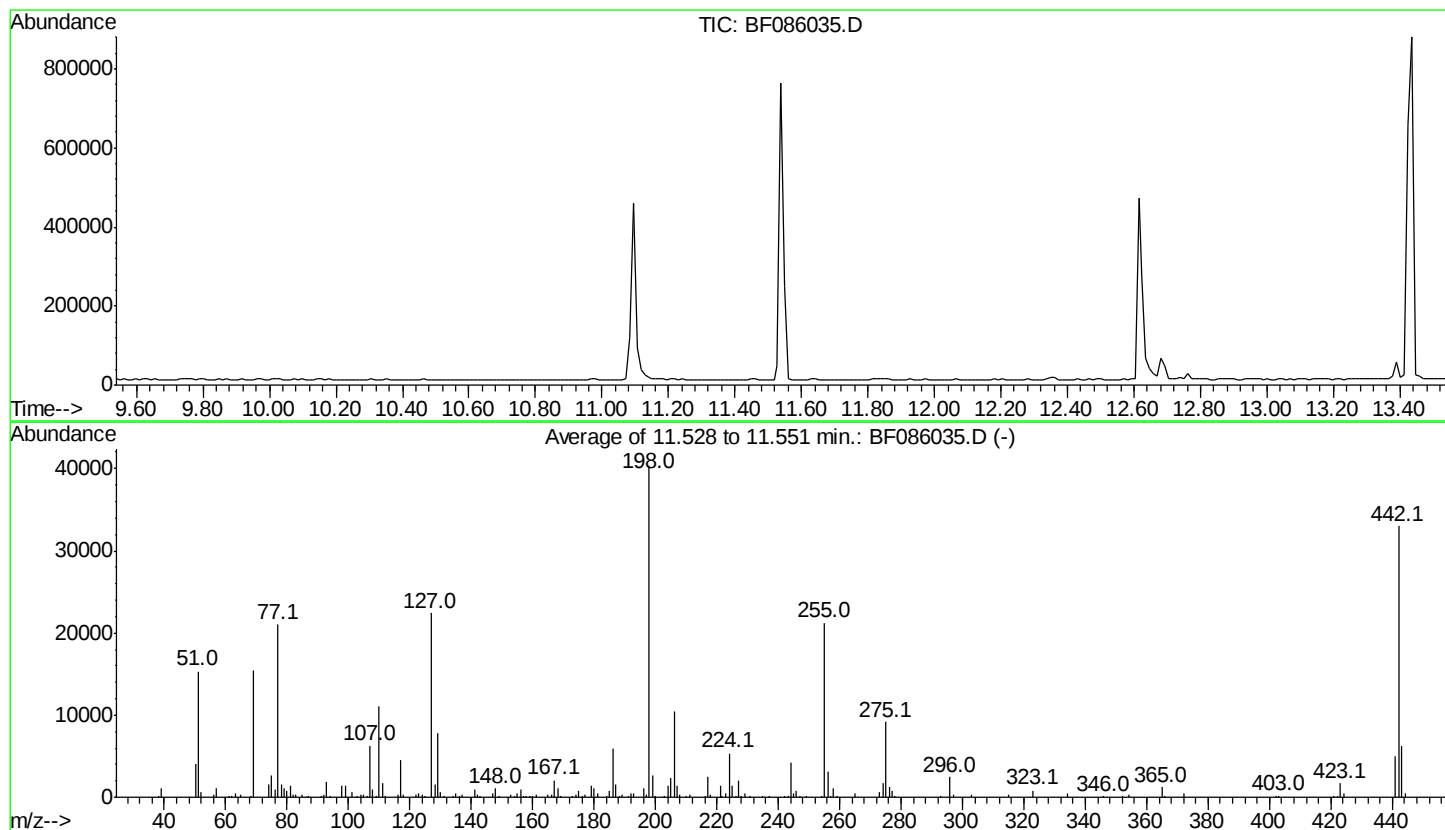

AutoFind: Scans 826, 827, 828; Background Corrected with Scan 823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	15316	PASS
68	69	0.00	2	1.4	219	PASS
69	198	0.00	100	38.3	15460	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.5	22390	PASS
197	198	0.00	2	0.6	240	PASS
198	198	100	100	100.0	40367	PASS
199	198	5	9	6.6	2656	PASS
275	198	10	60	22.7	9154	PASS
365	198	1	100	2.9	1178	PASS
441	442	0.01	24	15.3	5058	PASS
442	198	50	100	81.8	33034	PASS
443	442	15	24	19.0	6291	PASS